

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
 Data File : VW031049.D
 Acq On : 18 Nov 2024 17:12
 Operator : SY/MD
 Sample : P4872-21
 Misc : 6.41g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Y8

Quant Time: Nov 19 00:31:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 19 00:28:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	528199	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	449977	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	162938	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	114059	13.166	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.680%
7) Chloroethane-d5	2.905	69	98989	14.899	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.600%
11) 1,1-Dichloroethene-d2	4.027	65	54129	15.143	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.560%
21) 2-Butanone-d5	7.075	46	65032	45.617	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.240%
24) Chloroform-d	7.648	84	291670	18.731	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.920%
26) 1,2-Dichloroethane-d4	8.307	65	153055	19.769	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.080%
32) Benzene-d6	8.276	84	543482	19.442	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.760%
36) 1,2-Dichloropropane-d6	9.276	67	173253	21.024	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.080%
41) Toluene-d8	10.325	98	454891	18.142	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.560%
43) trans-1,3-Dichloroprop...	10.575	79	63086	18.886	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.560%
47) 2-Hexanone-d5	10.922	63	52503	49.159	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.320%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	137649	23.975	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.880%
66) 1,2-Dichlorobenzene-d4	13.848	152	142393	23.991	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.960%
Target Compounds					Qvalue	
13) Acetone	4.118	43	84426	48.488	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
Data File : VW031049.D
Acq On : 18 Nov 2024 17:12
Operator : SY/MD
Sample : P4872-21
Misc : 6.41g/10mL/MSVOA_W/SOIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29Y8

Quant Time: Nov 19 00:31:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 19 00:28:30 2024
Response via : Initial Calibration

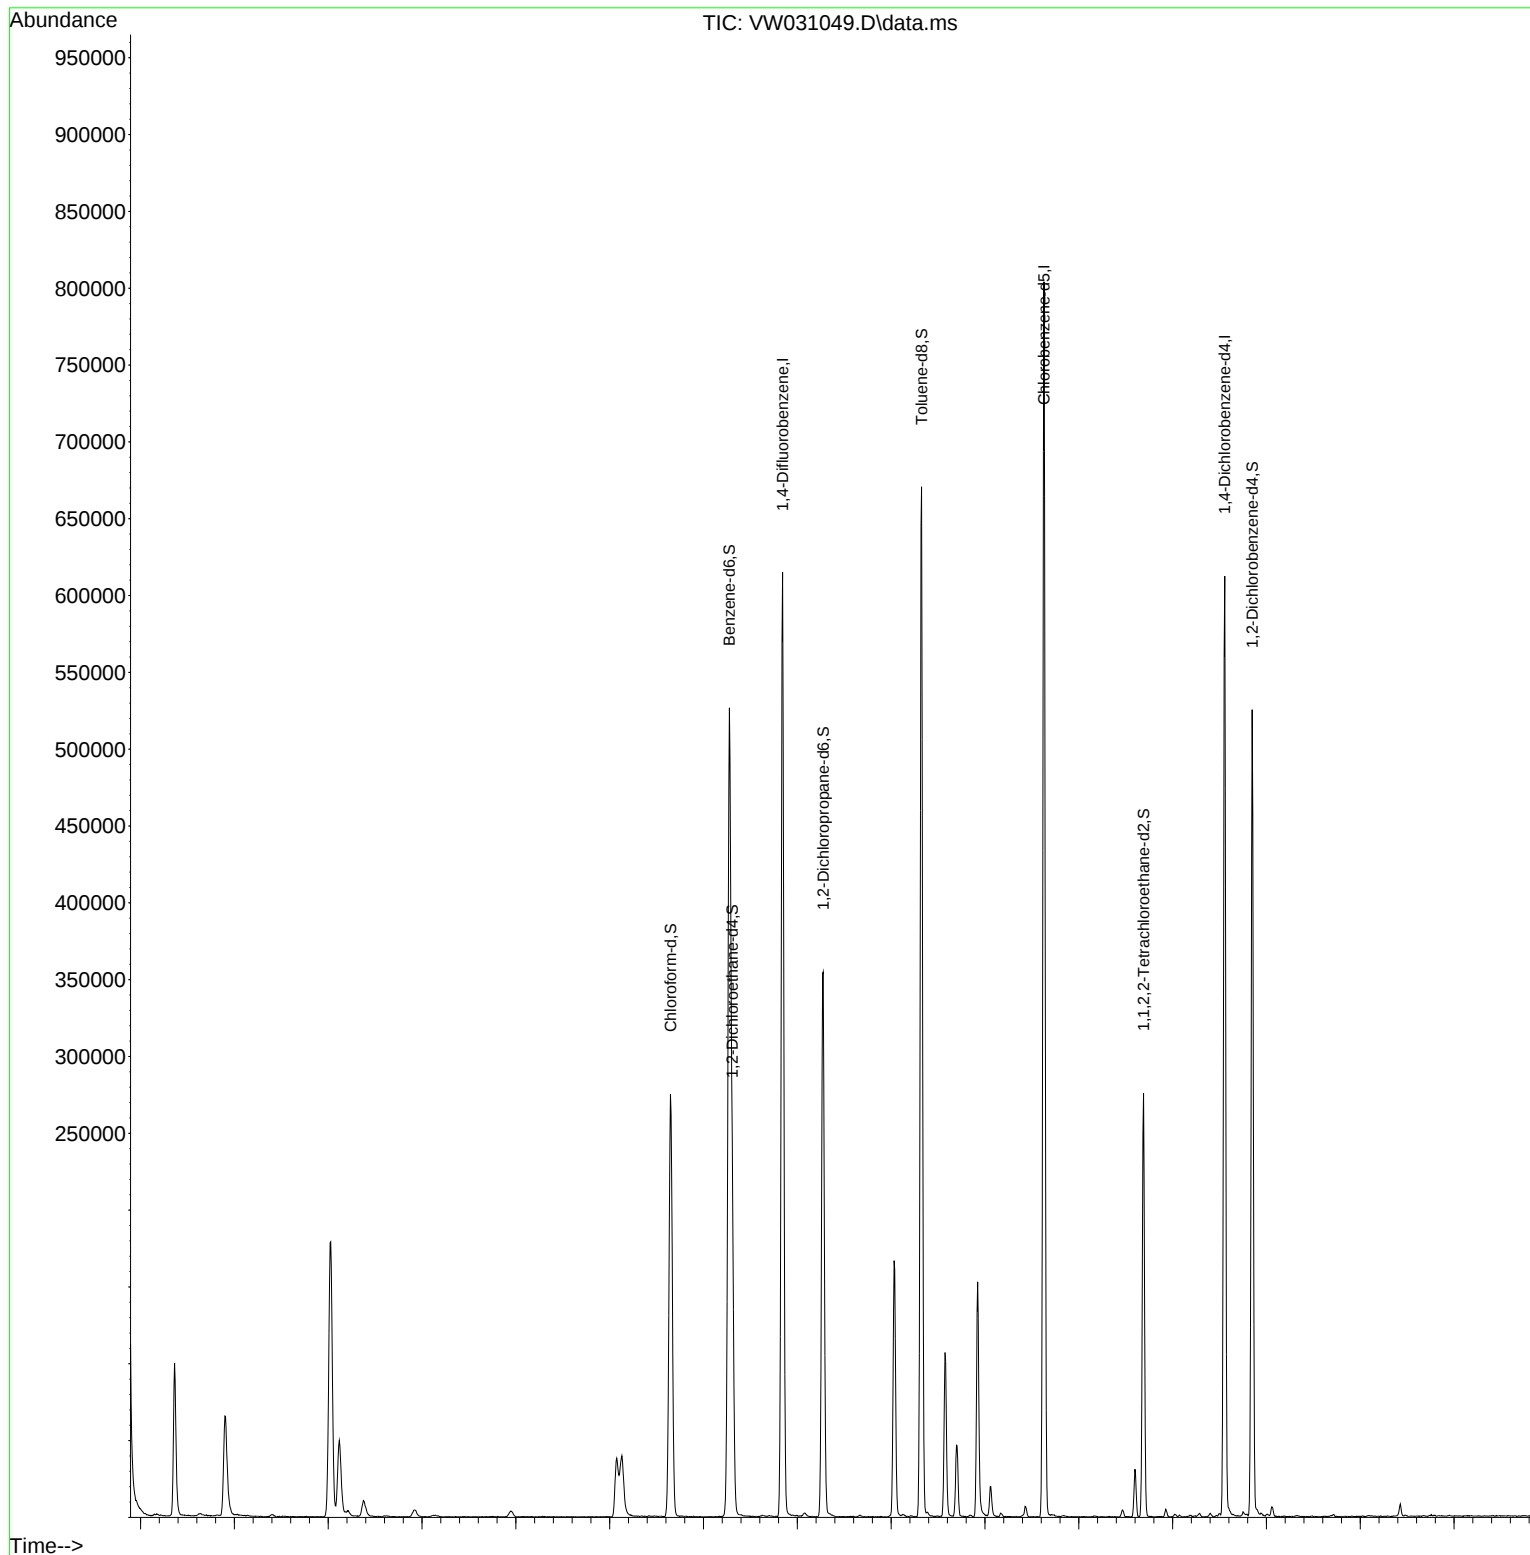

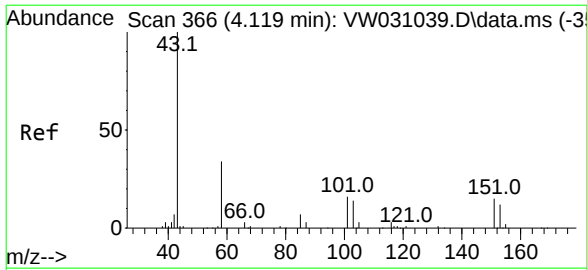

#13
 Acetone
 Concen: 48.488 ug/L
 RT: 4.118 min Scan# 36
 Delta R.T. -0.000 min
 Lab File: VW031049.D
 Acq: 18 Nov 2024 17:12

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Y8

Tgt Ion: 43 Resp: 84426
 Ion Ratio Lower Upper
 43 100
 58 32.8 0.0 62.6

