
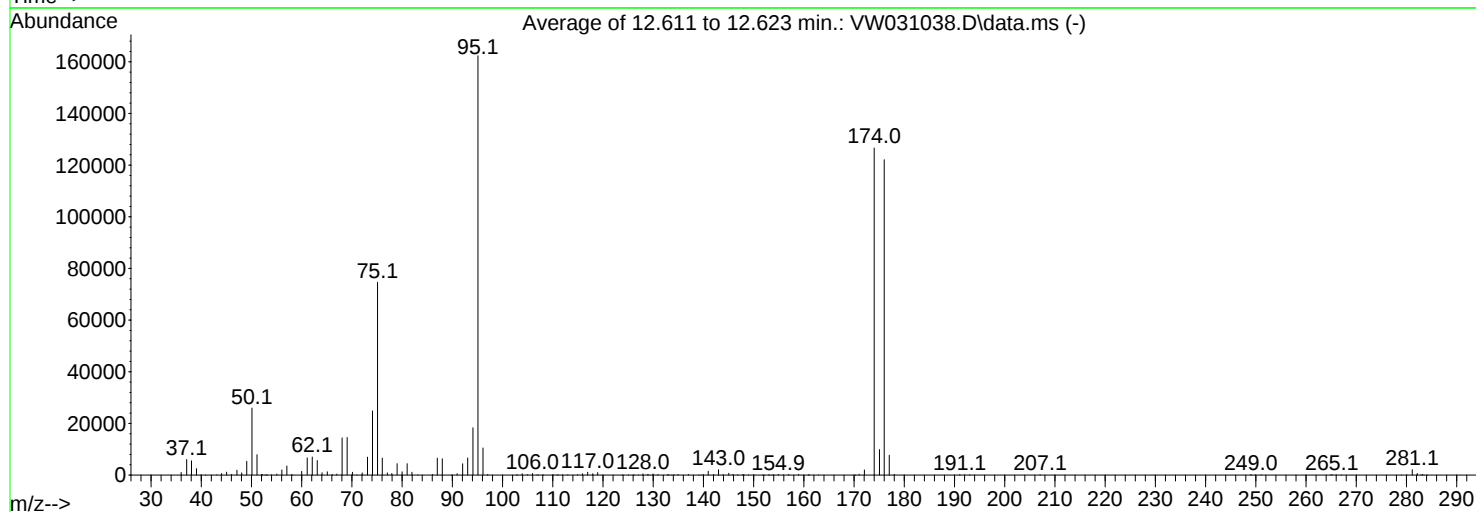


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111824\
Data File : VW031038.D
Acq On : 18 Nov 2024 08:42
Operator : SY/MD
Sample : BFB400
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB400

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Title : SFAM01.0
Last Update : Tue Nov 19 00:28:30 2024

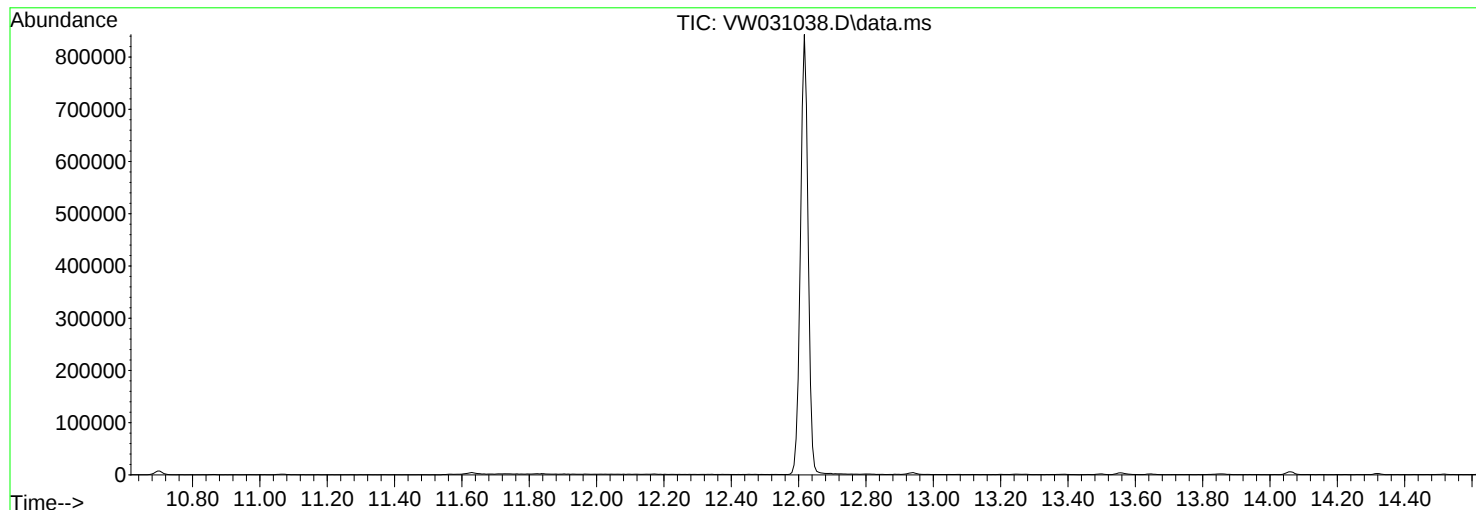

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	25957	PASS
75	95	30	80	46.0	74611	PASS
95	95	100	100	100.0	162347	PASS
96	95	5	9	6.5	10505	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.0	126627	PASS
175	174	5	9	7.8	9878	PASS
176	174	95	101	96.4	122123	PASS
177	176	5	9	6.3	7697	PASS

m/z	Abundance
35.90	247.0
38.00	95.0
39.90	238.0
44.10	183.0
57.20	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB400

m/z	Abundance
36.10	1302.0
37.10	6335.0
38.10	6330.0
39.10	2704.0
40.00	229.0
43.10	94.0
44.10	942.0
45.10	1128.0
46.10	291.0
47.00	1918.0
48.10	1004.0
49.10	5501.0
50.10	26664.0
51.10	8014.0
52.00	432.0
53.00	176.0
54.00	82.0
55.00	261.0
56.00	2025.0
57.00	3551.0
57.90	108.0
60.00	1518.0
61.10	6786.0
62.10	6830.0
63.10	5875.0
64.00	1071.0
65.10	1382.0
66.00	210.0
67.00	360.0
68.10	14678.0
69.10	14877.0
70.10	1173.0
71.00	58.0
72.10	986.0
73.10	7359.0
74.10	24320.0
75.10	73296.0
76.10	6722.0
77.10	773.0
78.00	467.0
79.00	4616.0
80.00	1332.0
81.00	4709.0
82.00	1158.0
83.10	95.0
86.10	102.0
87.00	6615.0
88.00	5870.0
91.00	569.0
92.00	4343.0
93.10	6168.0
94.10	17368.0
95.10	155264.0
96.10	10561.0
97.10	234.0
102.80	161.0
104.00	474.0
105.20	160.0
106.00	482.0
107.20	143.0
108.10	182.0
109.90	117.0
110.80	88.0
112.00	86.0
113.10	100.0
114.90	163.0
115.90	517.0
117.00	1143.0
118.00	386.0
118.90	1084.0
123.80	84.0
125.10	268.0
127.90	481.0
128.90	230.0
129.90	390.0
130.90	195.0
132.80	255.0
133.20	257.0
133.70	70.0
134.20	79.0
135.00	254.0
137.10	166.0
139.70	99.0
141.00	1377.0
142.10	207.0
143.00	2278.0
143.90	255.0
145.00	1040.0
145.90	303.0
146.80	115.0
148.10	264.0
149.10	81.0

Instrument :
MSVOA_W
ClientSampleId :
BFB400

150.00	102.0
152.10	51.0
153.00	156.0
154.00	141.0
154.90	219.0
156.90	227.0
159.00	193.0
160.90	236.0
162.90	97.0
170.90	421.0
172.00	2066.0
174.00	107216.0
175.00	8655.0
176.00	100256.0
177.00	6215.0
178.00	230.0
191.10	314.0
192.00	155.0
193.00	355.0
194.00	57.0
207.10	265.0
249.00	247.0
251.10	132.0
265.10	409.0
266.00	116.0
267.00	101.0
279.00	57.0
280.10	73.0
281.20	2741.0
282.10	890.0
283.20	608.0
284.20	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB400

m/z	Abundance
36.10	1464.0
37.10	6652.0
38.10	5887.0
39.10	2825.0
40.10	312.0
43.10	79.0
44.00	730.0
45.00	1332.0
45.90	168.0
47.10	2409.0
48.00	898.0
49.00	6112.0
50.10	29176.0
51.10	9049.0
52.20	416.0
52.90	168.0
54.00	128.0
55.00	491.0
56.10	2201.0
57.10	4046.0
58.00	166.0
60.00	1500.0
61.10	7333.0
62.10	8210.0
63.10	6559.0
64.10	968.0
65.10	1580.0
66.10	148.0
66.90	328.0
68.00	15961.0
69.00	16245.0
70.10	1174.0
71.00	79.0
72.00	826.0
73.10	7867.0
74.10	27760.0
75.10	83512.0
76.10	7447.0
77.00	992.0
78.00	708.0
79.00	4479.0
80.00	1298.0
81.00	5024.0
82.00	1238.0
83.20	150.0
86.00	260.0
87.00	7121.0
88.00	7067.0
89.80	54.0
91.00	583.0
92.10	4671.0
93.00	7669.0
94.10	21568.0
95.10	184384.0
96.10	11608.0
97.00	299.0
102.80	83.0
103.80	563.0
105.00	313.0
105.90	682.0
106.80	188.0
108.10	103.0
110.10	89.0
111.10	143.0
111.90	132.0
112.90	116.0
115.00	218.0
115.90	513.0
116.90	1297.0
117.90	698.0
119.00	1052.0
123.90	108.0
126.00	55.0
127.10	53.0
128.00	522.0
128.90	386.0
130.00	555.0
131.00	306.0
133.00	312.0
134.10	139.0
134.90	251.0
137.00	323.0
139.10	76.0
140.00	155.0
141.00	1880.0
142.10	199.0
143.00	2222.0
143.90	105.0
145.10	607.0
145.90	285.0
146.80	114.0
148.00	428.0

Instrument :
MSVOA_W
ClientSampleId :
BFB400

148.90	162.0
150.00	160.0
153.00	194.0
154.00	122.0
155.00	315.0
155.90	57.0
157.00	353.0
158.90	309.0
160.90	242.0
163.00	61.0
170.30	79.0
171.00	305.0
172.00	2058.0
174.00	144448.0
175.10	11560.0
176.00	131584.0
177.00	9434.0
178.00	266.0
190.90	162.0
193.10	169.0
207.10	101.0
249.00	201.0
249.90	61.0
250.90	77.0
265.20	243.0
266.00	57.0
281.10	2487.0
282.20	607.0
282.90	327.0

Instrument :
MSVOA_W
ClientSampleId :
BFB400

m/z	Abundance
36.00	1037.0
37.10	5086.0
38.10	4616.0
39.00	1958.0
40.00	224.0
40.90	51.0
43.10	50.0
44.10	657.0
45.10	976.0
46.10	217.0
47.20	1300.0
48.00	665.0
49.10	4418.0
50.10	22032.0
51.10	6644.0
52.20	261.0
52.70	91.0
53.20	65.0
55.10	429.0
56.10	1800.0
57.10	3115.0
58.20	131.0
60.00	1339.0
61.10	5878.0
62.10	5989.0
63.10	4470.0
64.10	704.0
65.00	888.0
66.20	131.0
67.10	463.0
68.10	12574.0
69.10	12598.0
70.10	922.0
71.00	71.0
72.00	693.0
73.10	5676.0
74.10	22440.0
75.10	67024.0
76.00	5596.0
77.00	839.0
77.90	710.0
79.00	4170.0
80.00	1216.0
81.00	3517.0
81.90	942.0
86.00	159.0
87.00	5984.0
88.00	6036.0
89.80	53.0
90.90	535.0
92.10	4181.0
93.10	6100.0
94.10	16051.0
95.10	147392.0
96.10	9345.0
97.00	234.0
103.00	182.0
103.90	513.0
104.90	170.0
106.00	654.0
106.90	140.0
108.10	62.0
110.10	119.0
110.90	130.0
113.00	163.0
114.90	118.0
115.90	554.0
117.00	840.0
118.00	474.0
118.90	766.0
123.90	79.0
126.20	67.0
127.90	437.0
129.10	314.0
130.00	416.0
131.00	136.0
132.90	102.0
134.10	61.0
135.00	218.0
136.90	249.0
139.10	83.0
140.00	120.0
140.90	1296.0
142.00	154.0
143.00	1784.0
143.90	54.0
145.10	505.0
145.90	334.0
146.90	121.0
147.80	357.0
149.10	97.0
150.10	135.0

Instrument :
MSVOA_W
ClientSampleId :
BFB400

151.80	78.0
153.20	139.0
153.70	79.0
154.00	82.0
154.80	352.0
155.90	86.0
157.10	190.0
159.00	298.0
161.10	102.0
171.10	247.0
172.10	1830.0
174.00	128216.0
175.00	9419.0
176.00	134528.0
177.00	7441.0
178.00	251.0
191.10	127.0
206.90	60.0
249.20	61.0
264.90	132.0
281.10	1076.0
282.10	369.0
283.10	109.0
283.50	75.0

Instrument :
MSVOA_W
ClientSampleId :
BFB400