

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW111918\
 Data File : VW006940.D
 Acq On : 19 Nov 2018 12:33
 Operator : SY/AP
 Sample : J5979-02
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETO65

Quant Time: Nov 20 06:27:05 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111418S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 20 06:18:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	129276	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	113362	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	43760	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	26265	22.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.52%
7) Chloroethane-d5	2.89	69	20563	24.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.64%
10) 1,1-Dichloroethene-d2	4.02	63	53735	17.53	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.12%
20) 2-Butanone-d5	7.09	46	19196	30.35	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	60.70%
24) Chloroform-d	7.65	84	70647	24.68	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.72%
26) 1,2-Dichloroethane-d4	8.31	65	41038	25.41	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.64%
29) Benzene-d6	8.27	84	143116	24.15	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.60%
33) 1,2-Dichloropropane-d6	9.27	67	43395	23.92	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.68%
37) Toluene-d8	10.32	98	142176	23.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.68%
38) trans-1,3-Dichloropropene-	10.58	79	16719	21.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.84%
39) 2-Hexanone-d5	10.93	63	14704	32.53	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	65.06%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	29827	19.00	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.00%
61) 1,2-Dichlorobenzene-d4	13.86	152	35449	21.39	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.56%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.14	43	6846	16.801	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW111918\
Data File : VW006940.D
Acq On : 19 Nov 2018 12:33
Operator : SY/AP
Sample : J5979-02
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETO65

Quant Time: Nov 20 06:27:05 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111418S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 20 06:18:45 2018
Response via : Initial Calibration

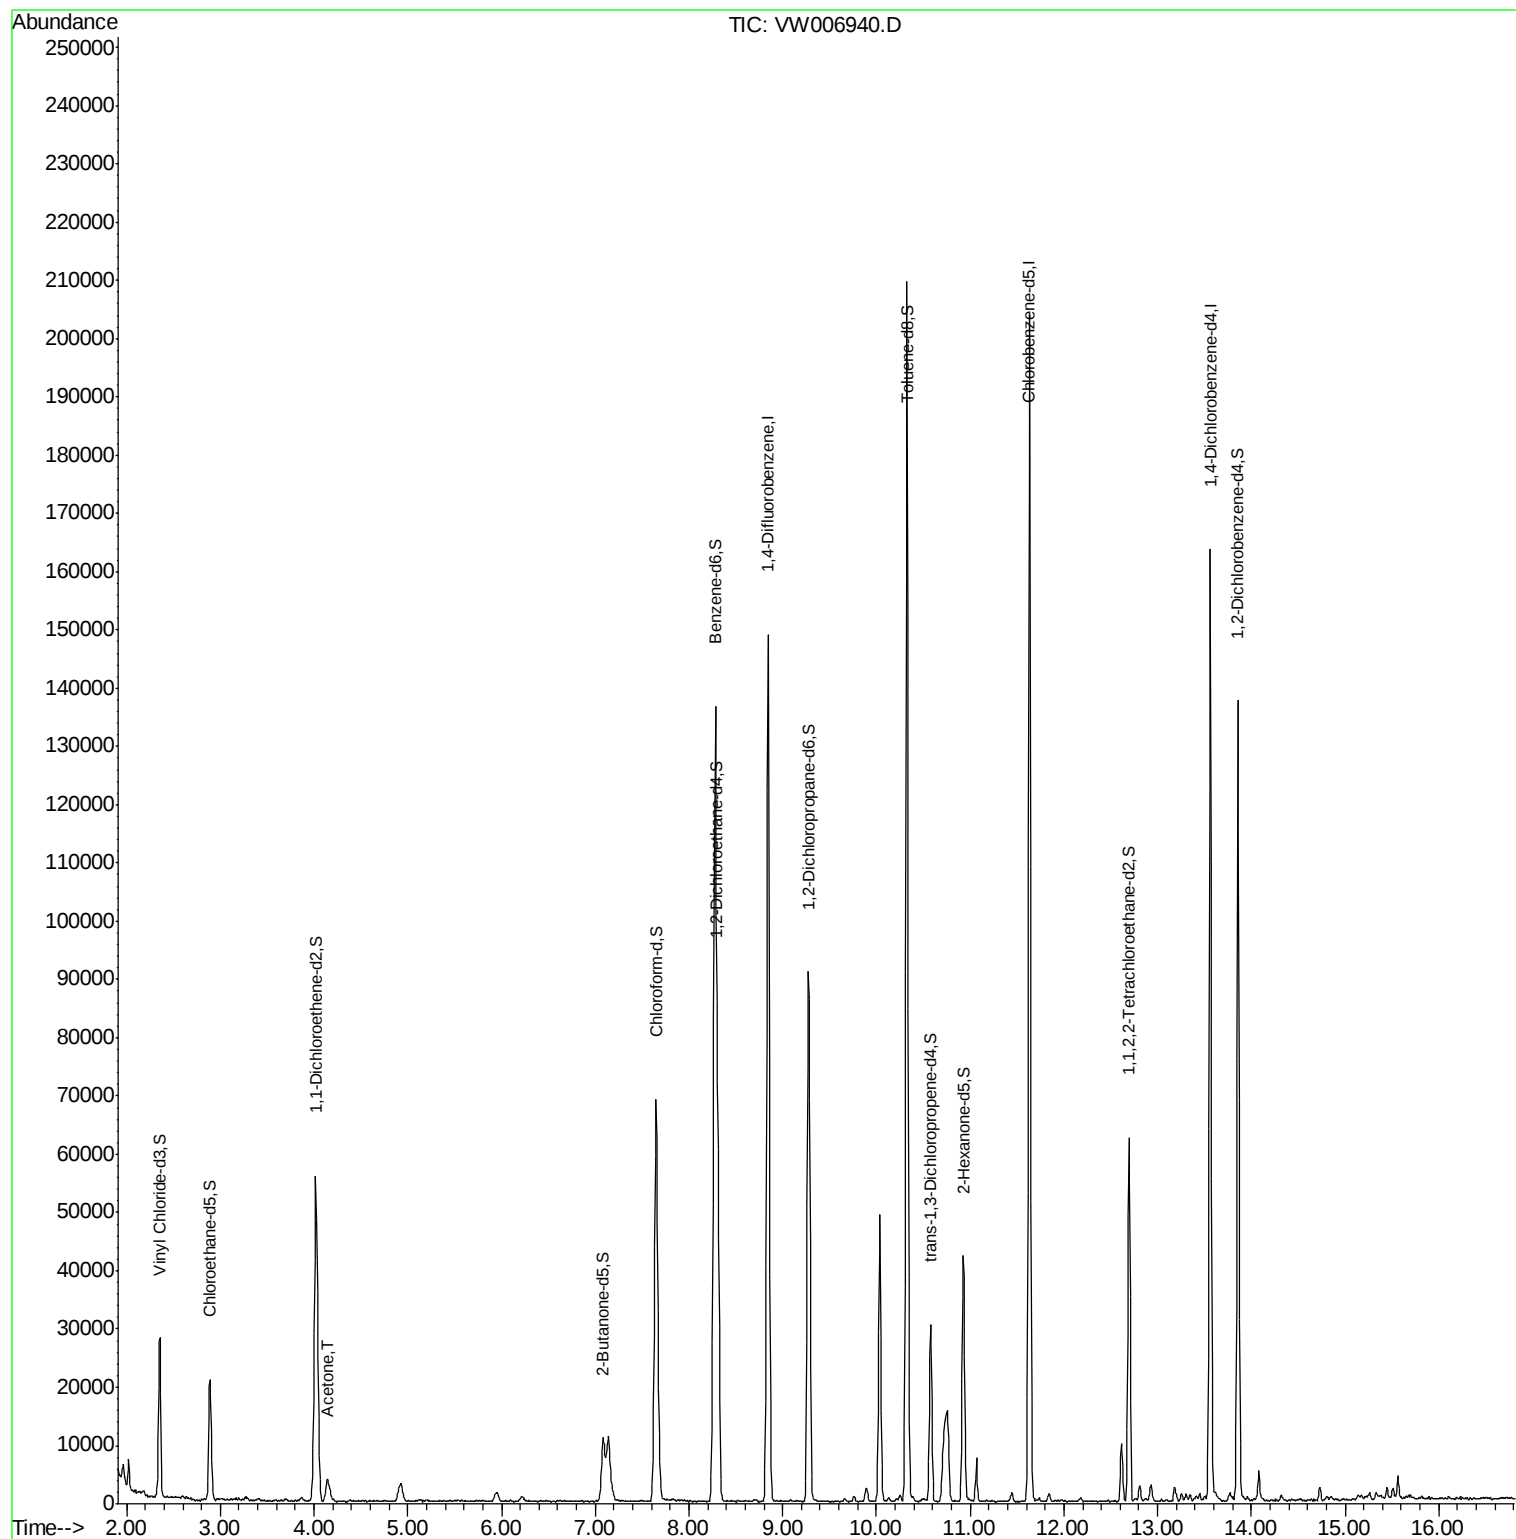

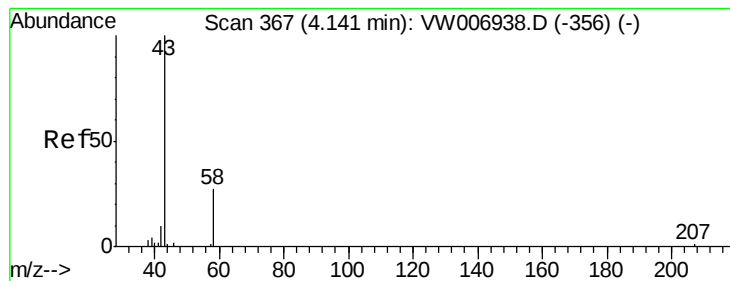

#13

Acetone

Concen: 16.801 ug/L

RT: 4.14 min Scan# 367

Delta R.T. -0.00 min

Lab File: VW006940.D

Acq: 19 Nov 2018 12:33

Instrument :

MSVOA_W

ClientSampleId :

ETO65

Tgt Ion: 43 Resp: 6846

Ion Ratio Lower Upper

43 100

58 29.9 0.0 65.6

