

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
 Data File : VW031055.D
 Acq On : 19 Nov 2024 12:32
 Operator : SY/MD
 Sample : VW1119SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 20 03:19:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 20 03:15:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	352547	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	345240	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	156177	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	75042	12.978	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	51.920%
7) Chloroethane-d5	2.899	69	69278	15.622	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.480%
11) 1,1-Dichloroethene-d2	4.021	65	37404	15.677	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.720%
21) 2-Butanone-d5	7.075	46	55617	58.450	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.900%
24) Chloroform-d	7.648	84	226494	21.793	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.160%
26) 1,2-Dichloroethane-d4	8.306	65	117668	22.771	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.080%
32) Benzene-d6	8.270	84	415696	19.382	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.520%
36) 1,2-Dichloropropane-d6	9.270	67	132586	20.970	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.880%
41) Toluene-d8	10.318	98	351960	18.295	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.160%
43) trans-1,3-Dichloroprop...	10.574	79	50088	19.544	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.160%
47) 2-Hexanone-d5	10.922	63	47644	58.143	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.280%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	119234	27.067	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.280%
66) 1,2-Dichlorobenzene-d4	13.848	152	141281	24.834	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.320%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3196	0.384	ug/L	Qvalue # 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
Data File : VW031055.D
Acq On : 19 Nov 2024 12:32
Operator : SY/MD
Sample : VW1119SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 20 03:19:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 20 03:15:02 2024
Response via : Initial Calibration

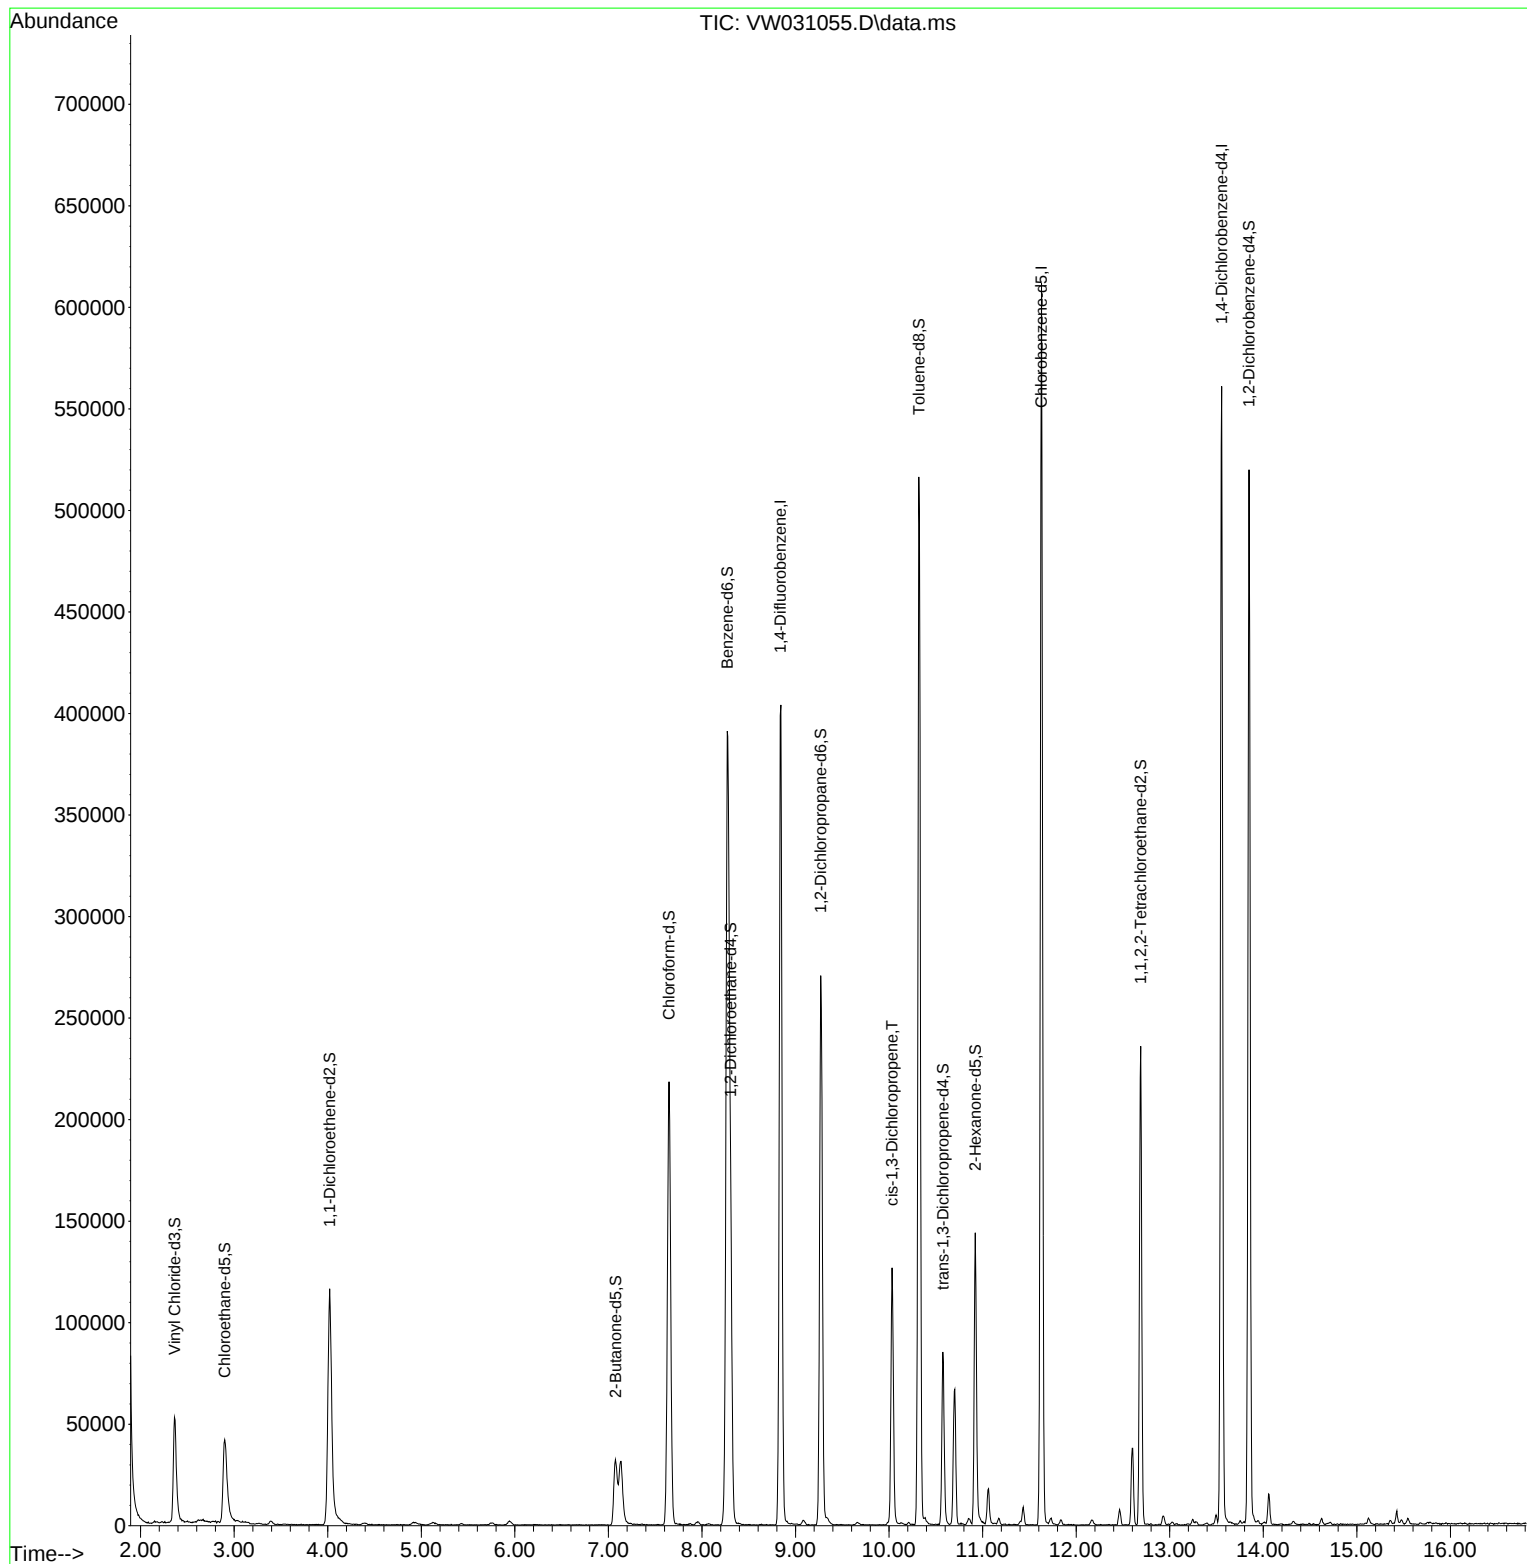

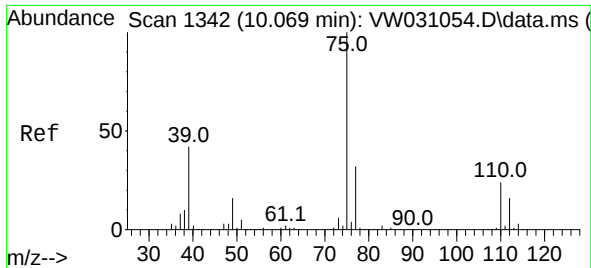

#39
 cis-1,3-Dichloropropene
 Concen: 0.384 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW031055.D
 Acq: 19 Nov 2024 12:32

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3196
 Ion Ratio Lower Upper
 75 100
 77 53.6 21.3 39.6#

