

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
 Data File : VW031062.D
 Acq On : 19 Nov 2024 16:37
 Operator : SY/MD
 Sample : P4895-01
 Misc : 5.29g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 20 03:21:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 20 03:15:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	374622	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	364150	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	159864	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	71972	11.714	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	46.840%
7) Chloroethane-d5	2.899	69	66793	14.174	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.680%
11) 1,1-Dichloroethene-d2	4.021	65	36788	14.511	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.040%
21) 2-Butanone-d5	7.082	46	44910	44.417	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.840%
24) Chloroform-d	7.648	84	217979	19.737	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.960%
26) 1,2-Dichloroethane-d4	8.301	65	108982	19.847	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.400%
32) Benzene-d6	8.270	84	396953	17.547	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	70.200%
36) 1,2-Dichloropropane-d6	9.270	67	128437	19.259	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	77.040%
41) Toluene-d8	10.319	98	346592	17.080	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	68.320%
43) trans-1,3-Dichloroprop...	10.575	79	46663	17.262	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.040%
47) 2-Hexanone-d5	10.922	63	36739	42.507	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.020%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	104934	22.584	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.320%
66) 1,2-Dichlorobenzene-d4	13.849	152	132060	22.678	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.720%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	3214	0.366	ug/L	# 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
Data File : VW031062.D
Acq On : 19 Nov 2024 16:37
Operator : SY/MD
Sample : P4895-01
Misc : 5.29g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 20 03:21:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 20 03:15:02 2024
Response via : Initial Calibration

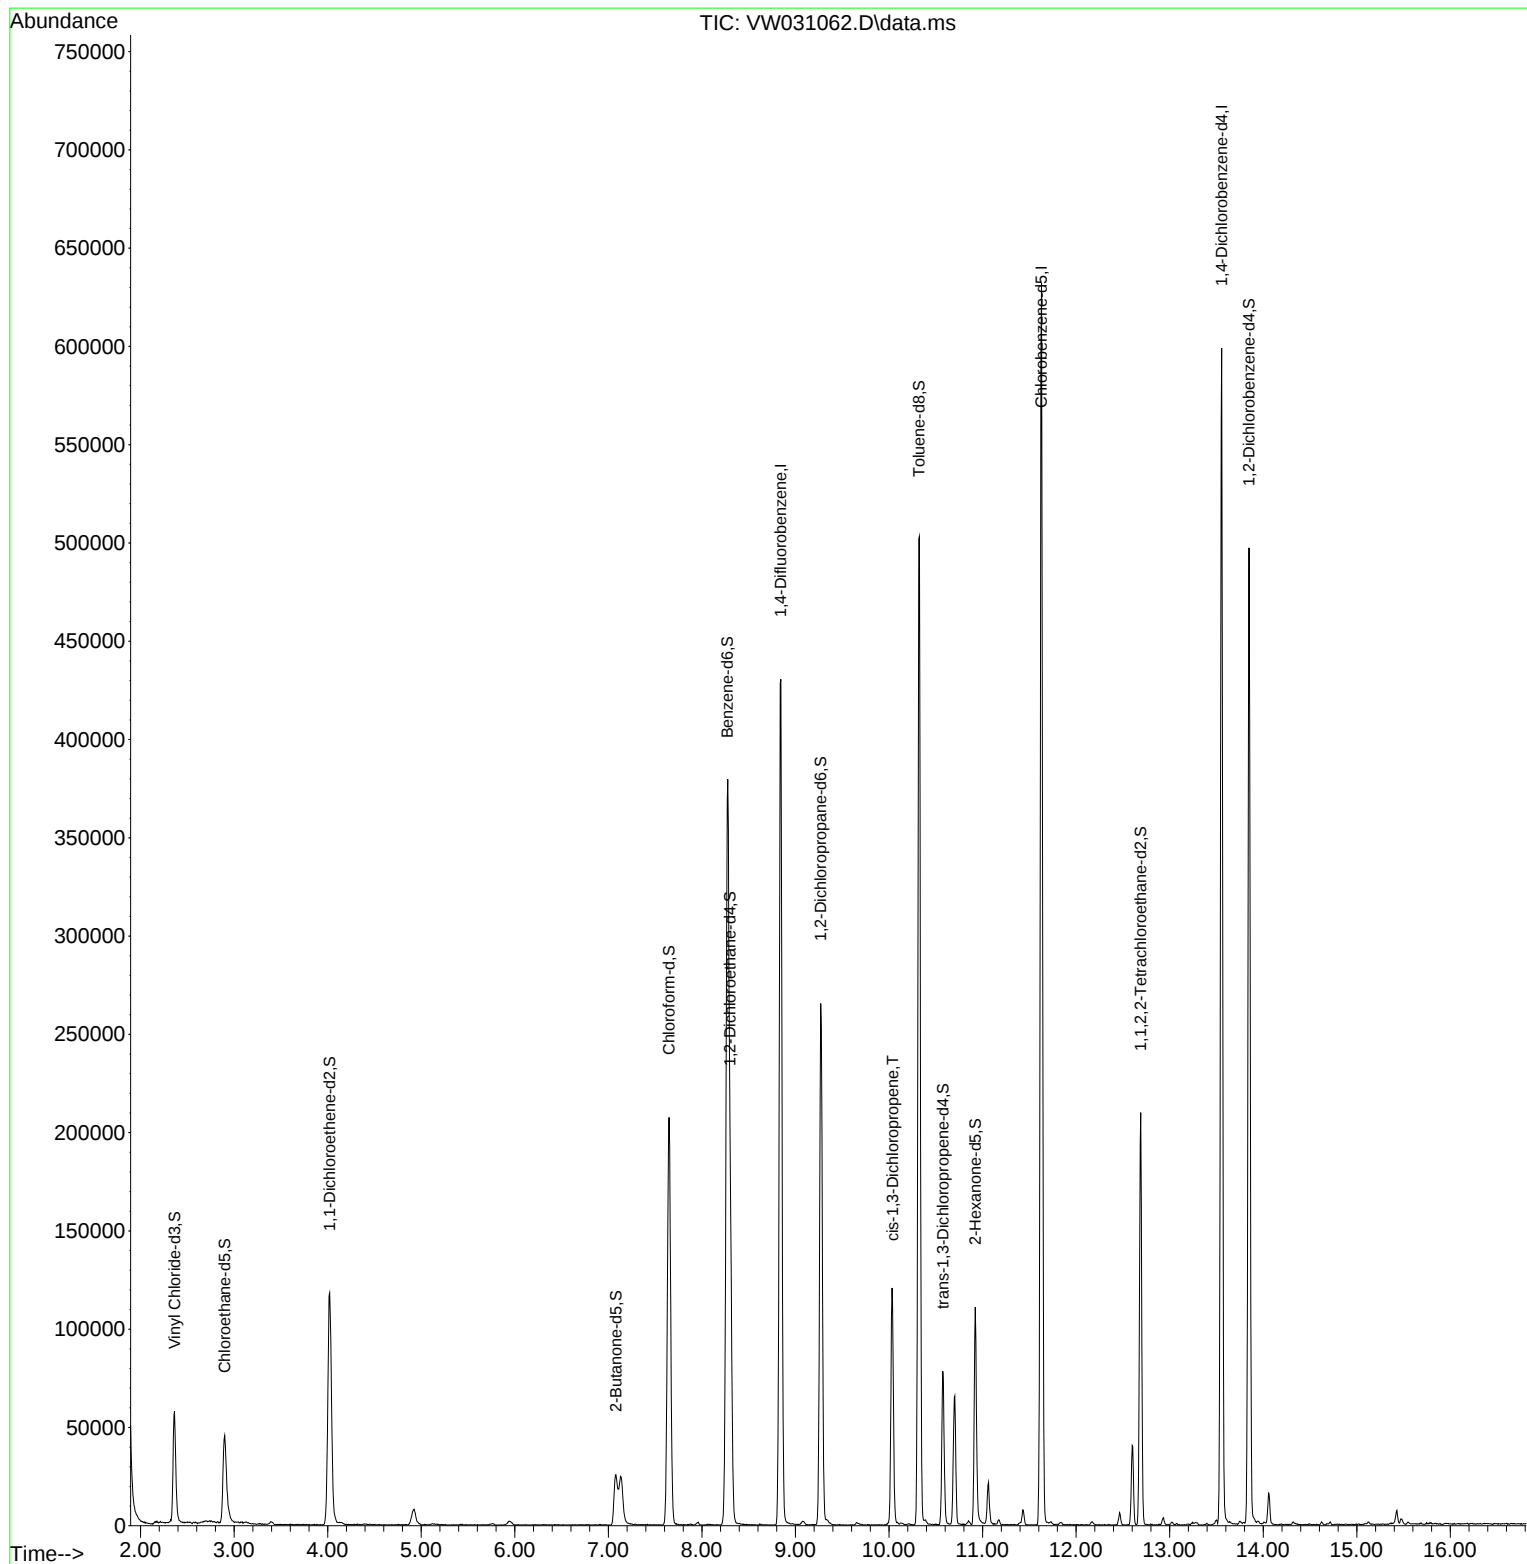

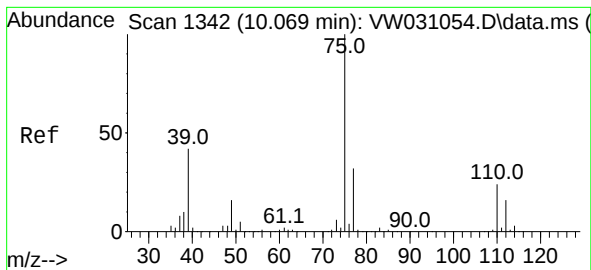

#39
 cis-1,3-Dichloropropene
 Concen: 0.366 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.030 min
 Lab File: VW031062.D
 Acq: 19 Nov 2024 16:37

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3214
 Ion Ratio Lower Upper
 75 100
 77 41.0 21.3 39.6#

