

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
 Data File : VW031056.D
 Acq On : 19 Nov 2024 13:29
 Operator : SY/MD
 Sample : P4895-02
 Misc : 6.14g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E2A12

Quant Time: Nov 20 03:20:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 20 03:15:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	487516	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	437677	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	167290	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	96789	12.105	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	48.440%
7) Chloroethane-d5	2.899	69	82007	13.373	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	53.480%
11) 1,1-Dichloroethene-d2	4.015	65	47371	14.358	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.440%
21) 2-Butanone-d5	7.075	46	73222	55.648	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.300%
24) Chloroform-d	7.648	84	255458	17.775	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.080%
26) 1,2-Dichloroethane-d4	8.301	65	139768	19.559	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.240%
32) Benzene-d6	8.276	84	477871	17.575	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	70.280%
36) 1,2-Dichloropropane-d6	9.270	67	152588	19.036	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	76.160%
41) Toluene-d8	10.319	98	405757	16.637	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	66.560%
43) trans-1,3-Dichloroprop...	10.575	79	57967	17.841	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.360%
47) 2-Hexanone-d5	10.922	63	59192	56.980	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.960%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	140495	25.158	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.640%
66) 1,2-Dichlorobenzene-d4	13.849	152	121681	19.968	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.880%
Target Compounds					Qvalue	
13) Acetone	4.119	43	86479	53.812	ug/L	94
22) 2-Butanone	7.179	43	5496	3.054	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
Data File : VW031056.D
Acq On : 19 Nov 2024 13:29
Operator : SY/MD
Sample : P4895-02
Misc : 6.14g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E2A12

Quant Time: Nov 20 03:20:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 20 03:15:02 2024
Response via : Initial Calibration

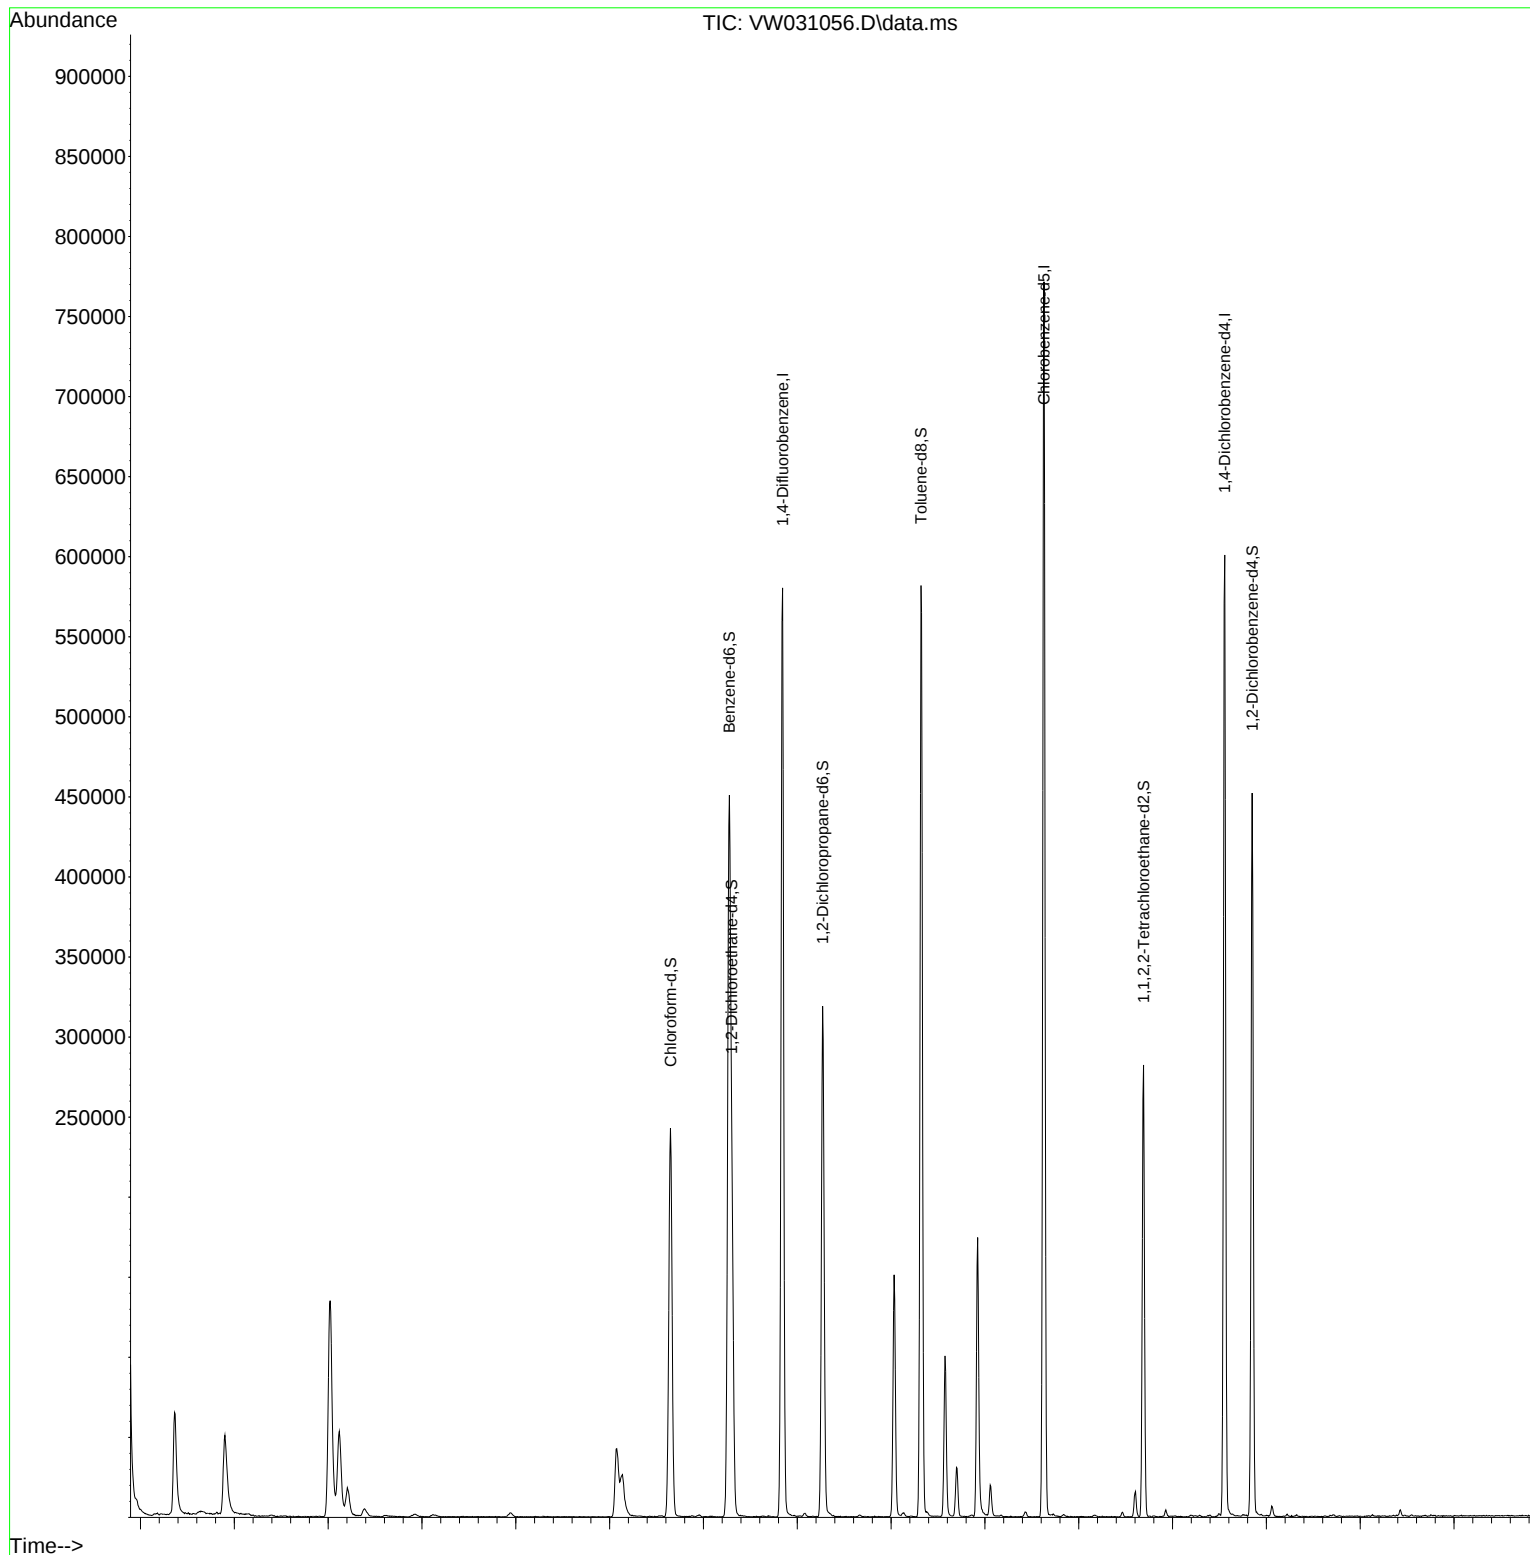

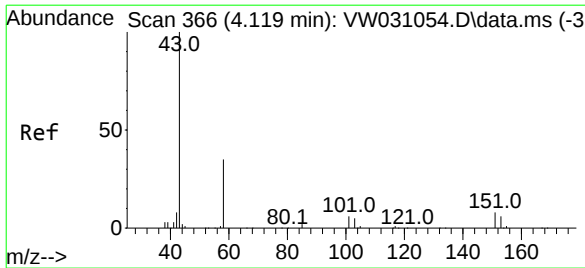

#13

Acetone

Concen: 53.812 ug/L

RT: 4.119 min Scan# 366

Delta R.T. -0.000 min

Lab File: VW031056.D

Acq: 19 Nov 2024 13:29

Instrument :

MSVOA_W

ClientSampleId :





E2A12

Tgt Ion: 43 Resp: 86479

Ion Ratio Lower Upper

43 100

58 34.8 0.0 62.6

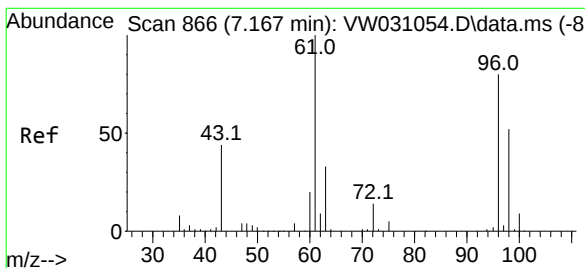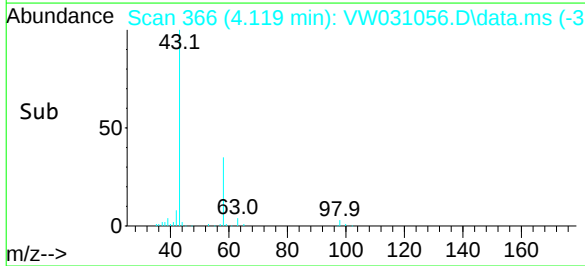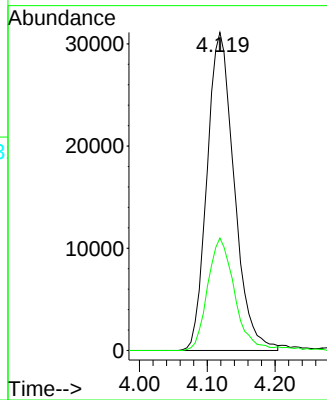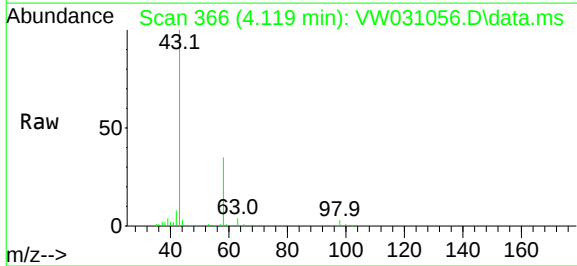

#22

2-Butanone

Concen: 3.054 ug/L

RT: 7.179 min Scan# 868

Delta R.T. 0.012 min

Lab File: VW031056.D

Acq: 19 Nov 2024 13:29

Tgt Ion: 43 Resp: 5496

Ion Ratio Lower Upper

43 100

72 28.8 14.5 43.6

