

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
 Data File : VW031058.D
 Acq On : 19 Nov 2024 15:02
 Operator : SY/MD
 Sample : P4872-18
 Misc : 5.51g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Y5

Quant Time: Nov 20 03:20:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 20 03:15:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	404255	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	372423	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	161677	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	74812	11.284	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	45.120%
7) Chloroethane-d5	2.899	69	63949	12.576	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.320%
11) 1,1-Dichloroethene-d2	4.021	65	36269	13.257	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.040%
21) 2-Butanone-d5	7.075	46	39422	36.131	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.260%
24) Chloroform-d	7.648	84	191891	16.102	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	64.400%
26) 1,2-Dichloroethane-d4	8.307	65	97146	16.395	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	65.560%#
32) Benzene-d6	8.276	84	347724	15.029	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	60.120%
36) 1,2-Dichloropropane-d6	9.270	67	114803	16.832	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	67.320%#
41) Toluene-d8	10.325	98	304945	14.694	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	58.760%
43) trans-1,3-Dichloroprop...	10.575	79	41045	14.846	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	59.400%
47) 2-Hexanone-d5	10.922	63	29569	33.451	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.900%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	90812	19.111	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.440%
66) 1,2-Dichlorobenzene-d4	13.848	152	111322	18.903	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.600%
Target Compounds					Qvalue	
13) Acetone	4.118	43	34909	26.196	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
Data File : VW031058.D
Acq On : 19 Nov 2024 15:02
Operator : SY/MD
Sample : P4872-18
Misc : 5.51g/10mL/MSVOA_W/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29Y5

Quant Time: Nov 20 03:20:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 20 03:15:02 2024
Response via : Initial Calibration

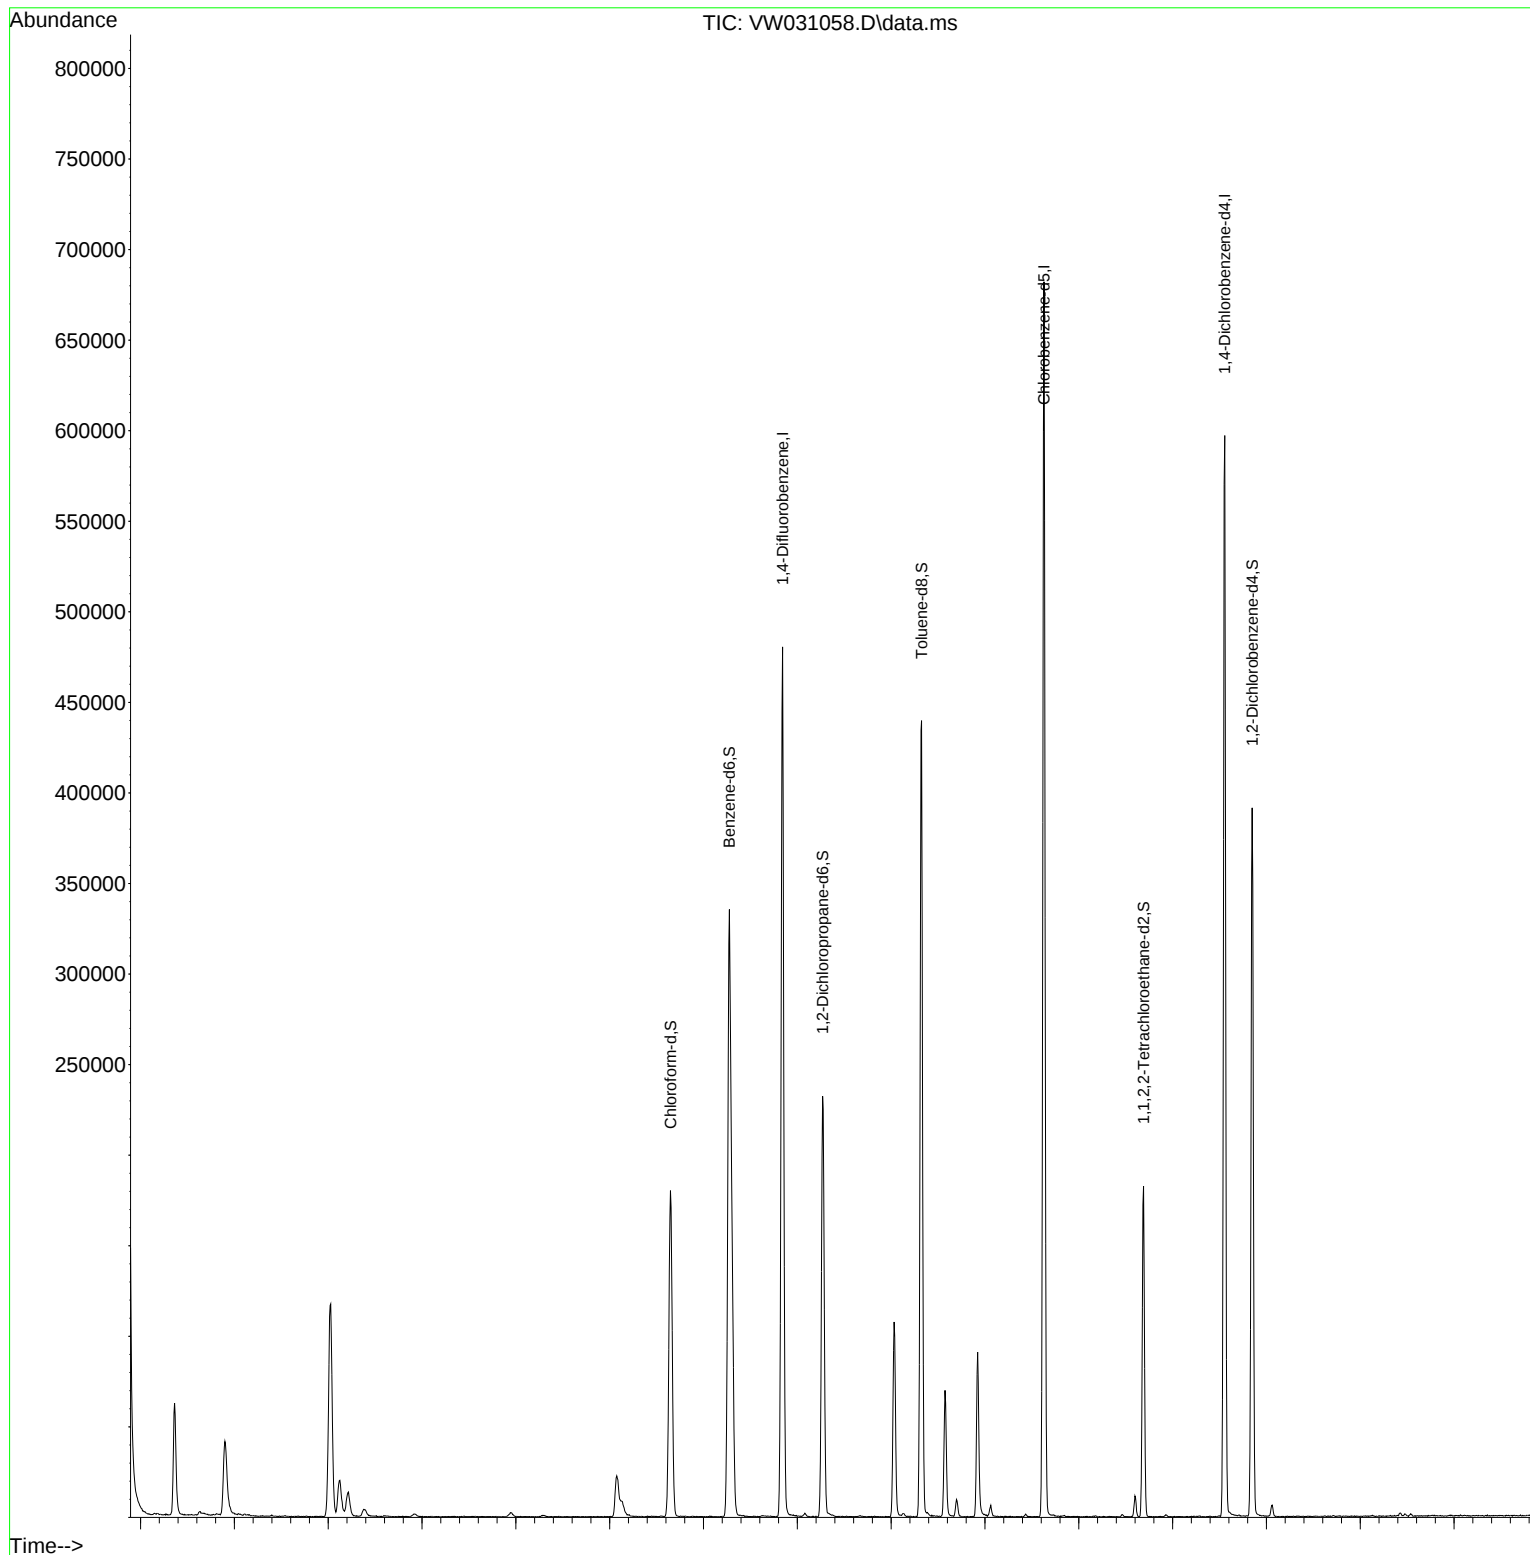

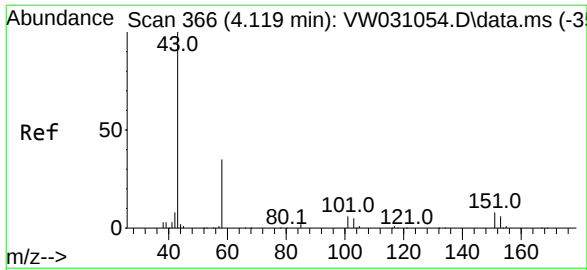

#13

Acetone

Concen: 26.196 ug/L

RT: 4.118 min Scan# 36

Delta R.T. -0.000 min

Lab File: VW031058.D


Acq: 19 Nov 2024 15:02

Instrument :

MSVOA_W

ClientSampleId :

E29Y5

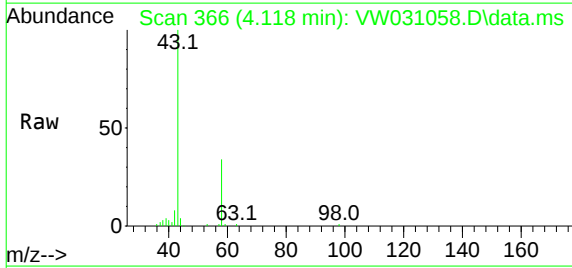

Tgt Ion: 43 Resp: 34909

Ion Ratio Lower Upper

43 100

58 33.8 0.0 62.6

