

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
 Data File : VW031060.D
 Acq On : 19 Nov 2024 15:49
 Operator : SY/MD
 Sample : P4872-20RE
 Misc : 6.76g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Y7RE

Quant Time: Nov 20 03:21:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 20 03:15:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	176206	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	153996	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	47949	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	44896	15.535	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.160%
7) Chloroethane-d5	2.893	69	39698	17.911	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.640%
11) 1,1-Dichloroethene-d2	4.021	65	20793	17.437	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.760%
21) 2-Butanone-d5	7.081	46	24318	51.133	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.260%
24) Chloroform-d	7.648	84	108095	20.809	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.240%
26) 1,2-Dichloroethane-d4	8.307	65	56216	21.766	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.080%
32) Benzene-d6	8.276	84	190419	19.904	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.600%
36) 1,2-Dichloropropane-d6	9.276	67	61937	21.961	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.840%
41) Toluene-d8	10.319	98	149389	17.409	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	69.640%
43) trans-1,3-Dichloroprop...	10.575	79	21023	18.390	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.560%
47) 2-Hexanone-d5	10.922	63	16429	44.948	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.900%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	53741	27.350	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	109.400%
66) 1,2-Dichlorobenzene-d4	13.842	152	41481	23.750	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.000%
Target Compounds					Qvalue	
13) Acetone	4.118	43	98716	169.951	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
Data File : VW031060.D
Acq On : 19 Nov 2024 15:49
Operator : SY/MD
Sample : P4872-20RE
Misc : 6.76g/10mL/MSVOA_W/SOIL/B
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29Y7RE

Quant Time: Nov 20 03:21:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 20 03:15:02 2024
Response via : Initial Calibration

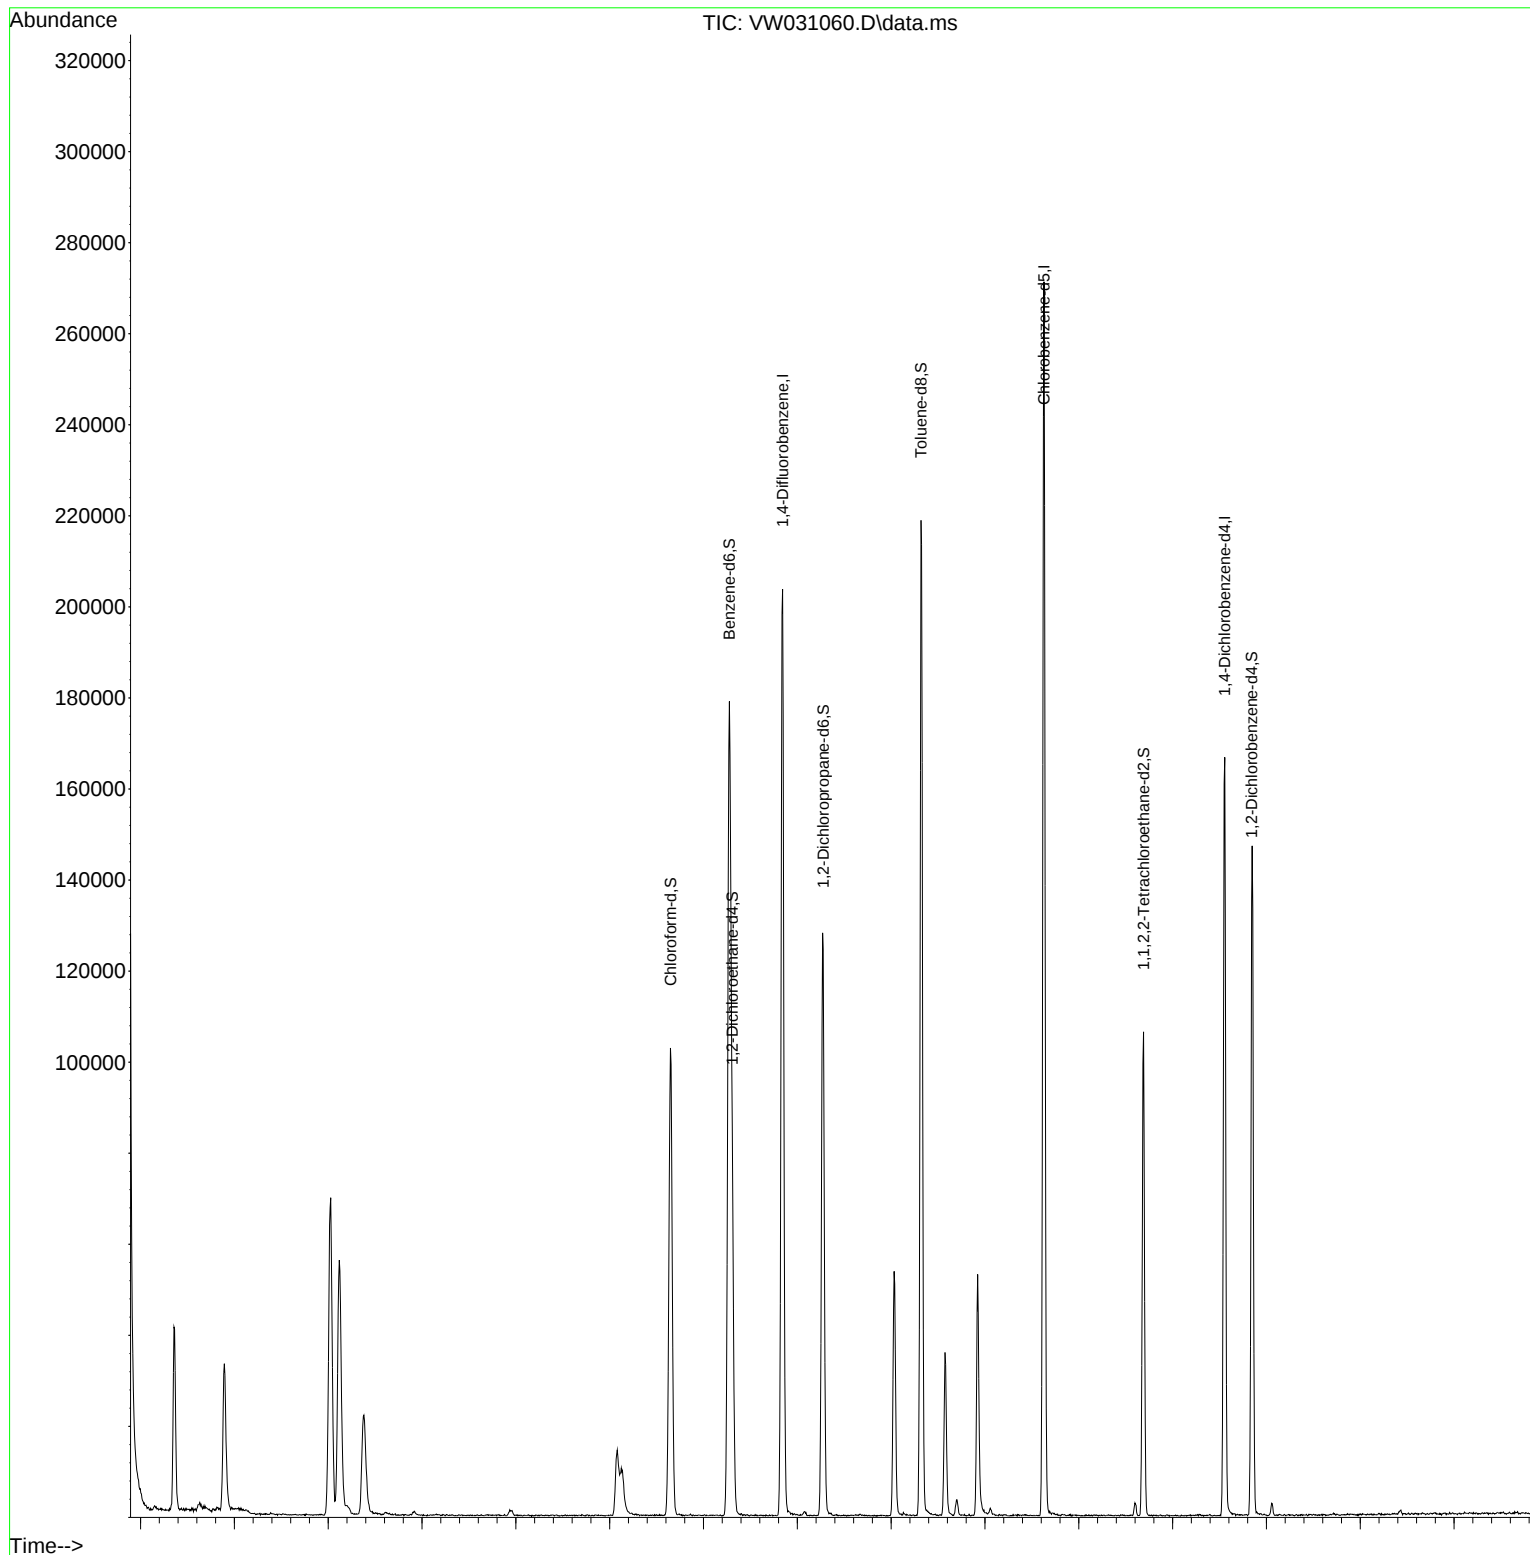

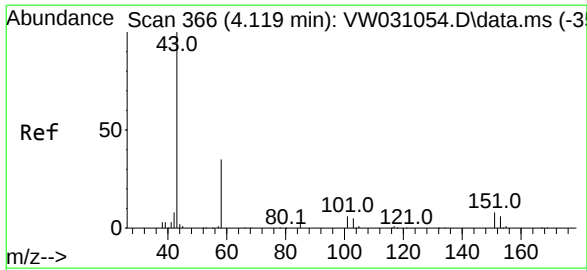

#13
 Acetone
 Concen: 169.951 ug/L
 RT: 4.118 min Scan# 36
 Delta R.T. -0.000 min
 Lab File: VW031060.D
 Acq: 19 Nov 2024 15:49

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Y7RE

Tgt Ion: 43 Resp: 98716
 Ion Ratio Lower Upper
 43 100
 58 33.2 0.0 62.6

