

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
 Data File : VW031061.D
 Acq On : 19 Nov 2024 16:13
 Operator : SY/MD
 Sample : P4872-23
 Misc : 5.01g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Z0

Quant Time: Nov 20 03:21:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 20 03:15:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	556079	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	486580	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	198202	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	112923	12.382	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	49.520%
7) Chloroethane-d5	2.899	69	98683	14.108	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.440%
11) 1,1-Dichloroethene-d2	4.027	65	53459	14.205	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.840%
21) 2-Butanone-d5	7.075	46	51683	34.436	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.880%
24) Chloroform-d	7.648	84	292852	17.864	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.440%
26) 1,2-Dichloroethane-d4	8.307	65	141416	17.350	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	69.400%#
32) Benzene-d6	8.276	84	543634	17.984	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.920%
36) 1,2-Dichloropropane-d6	9.270	67	172452	19.352	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	77.400%
41) Toluene-d8	10.325	98	462061	17.041	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	68.160%
43) trans-1,3-Dichloroprop...	10.574	79	58400	16.168	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	64.680%
47) 2-Hexanone-d5	10.922	63	40756	35.290	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.580%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	124078	19.985	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.960%
66) 1,2-Dichlorobenzene-d4	13.848	152	148922	20.627	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.520%
Target Compounds					Qvalue	
13) Acetone	4.118	43	63078	34.411	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
Data File : VW031061.D
Acq On : 19 Nov 2024 16:13
Operator : SY/MD
Sample : P4872-23
Misc : 5.01g/10mL/MSVOA_W/SOIL/B
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29Z0

Quant Time: Nov 20 03:21:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 20 03:15:02 2024
Response via : Initial Calibration

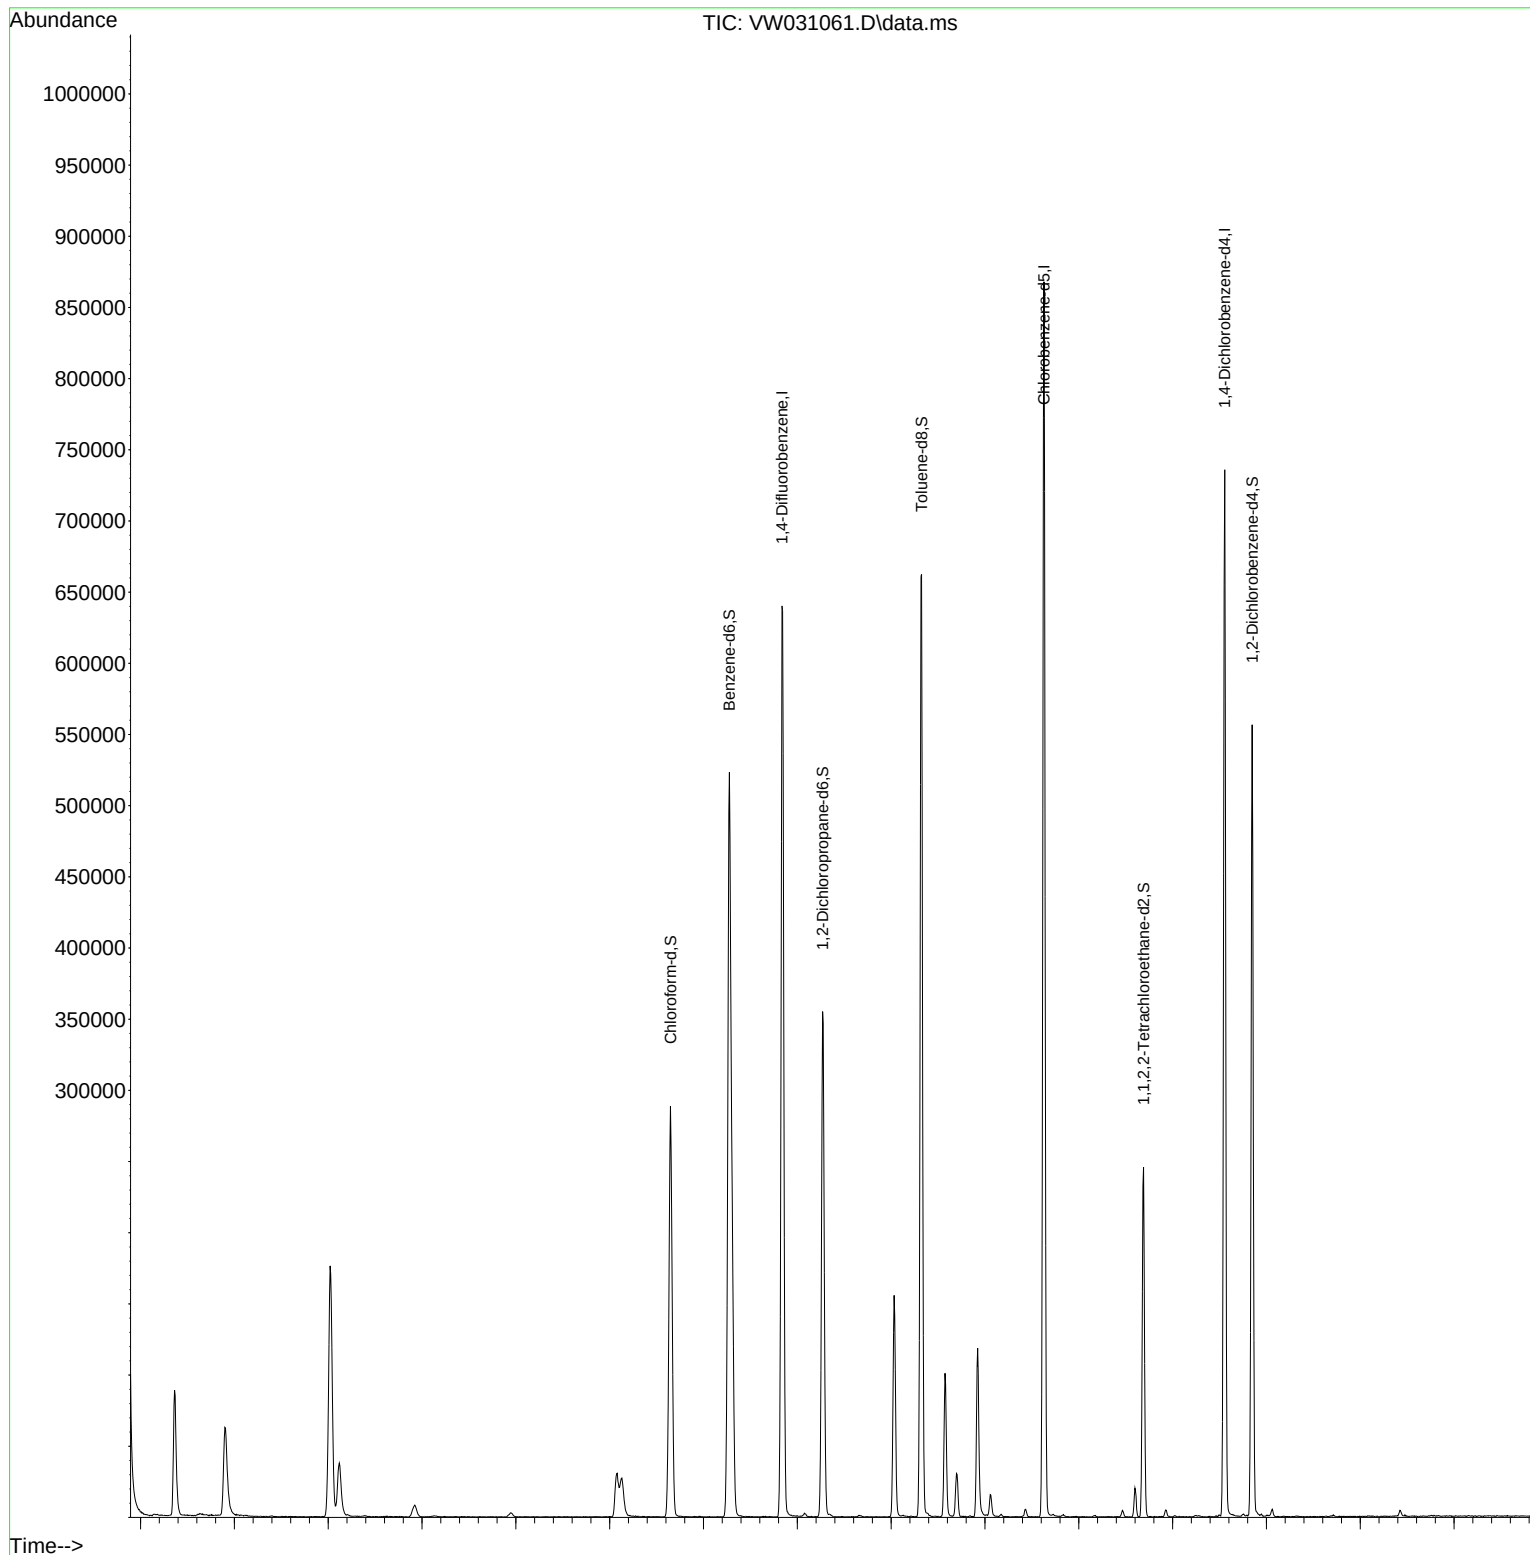

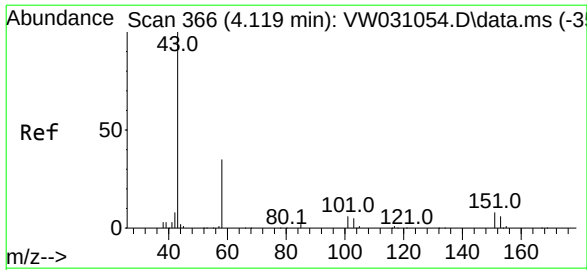

#13
 Acetone
 Concen: 34.411 ug/L
 RT: 4.118 min Scan# 36
 Delta R.T. -0.000 min
 Lab File: VW031061.D
 Acq: 19 Nov 2024 16:13

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Z0

Tgt Ion: 43 Resp: 63078
 Ion Ratio Lower Upper
 43 100
 58 34.2 0.0 62.6

