
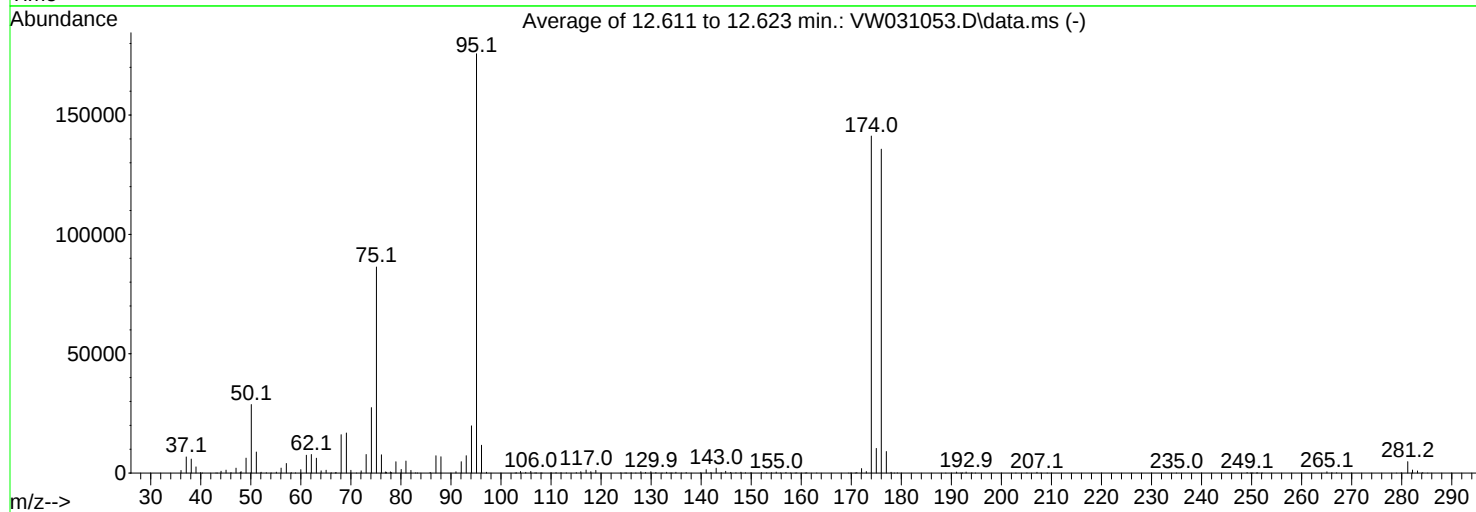


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111924\
Data File : VW031053.D
Acq On : 19 Nov 2024 10:28
Operator : SY/MD
Sample : BFB401
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB401

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Title : SFAM01.0
Last Update : Wed Nov 20 03:15:02 2024

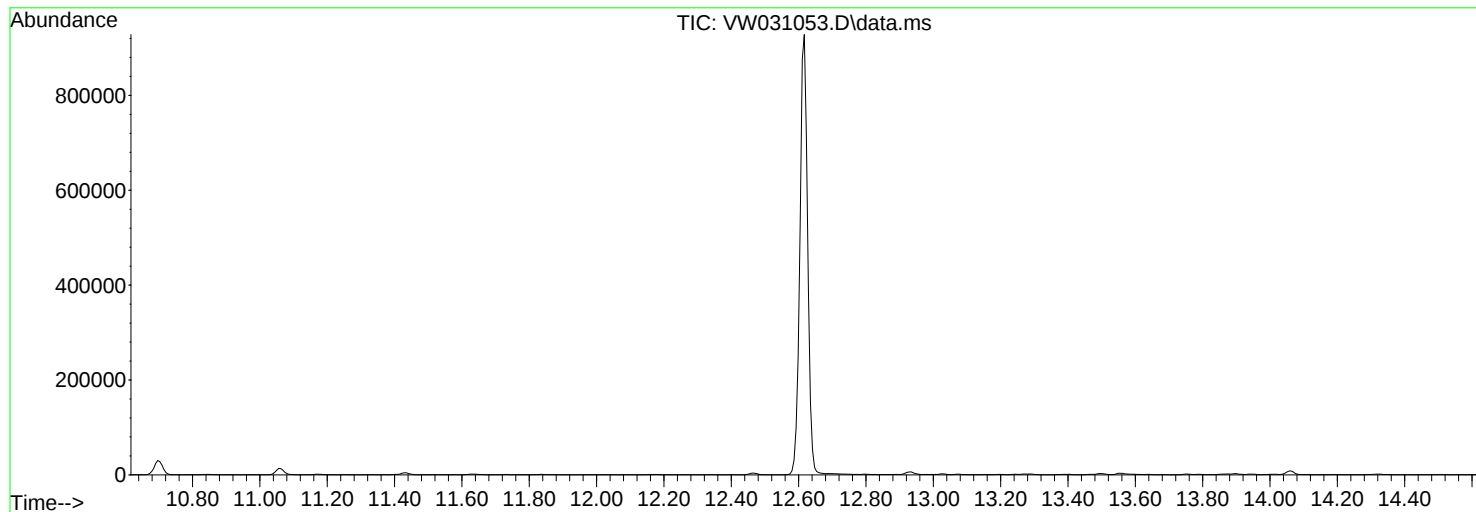

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	28733	PASS
75	95	30	80	49.1	86339	PASS
95	95	100	100	100.0	175701	PASS
96	95	5	9	6.6	11662	PASS
173	174	0.00	2	0.5	649	PASS
174	95	50	120	80.4	141205	PASS
175	174	5	9	7.3	10350	PASS
176	174	95	101	96.1	135717	PASS
177	176	5	9	6.7	9047	PASS

Scan 1751 (12.562 min): VW031053.D\data.ms
BFB401

m/z	Abundance
40.00	164.0
44.10	142.0

Instrument :
MSVOA_W
ClientSampleId :
BFB401

m/z	Abundance
36.10	1301.0
37.10	7706.0
38.10	6858.0
39.10	2776.0
39.90	208.0
40.30	179.0
43.00	107.0
44.00	1145.0
45.00	1448.0
46.00	209.0
47.00	2068.0
47.90	1022.0
49.10	6701.0
50.10	31472.0
51.10	9255.0
52.10	376.0
53.20	220.0
54.10	66.0
55.20	386.0
56.00	2184.0
57.10	4026.0
58.00	172.0
59.00	233.0
60.00	1677.0
61.10	7980.0
62.10	8895.0
63.10	6966.0
64.10	1120.0
65.00	1525.0
66.20	122.0
66.90	500.0
68.10	16864.0
69.10	18024.0
70.00	1303.0
72.00	1058.0
73.10	8645.0
74.10	30568.0
75.10	90544.0
76.10	8532.0
76.90	795.0
77.90	634.0
79.00	5336.0
80.10	1524.0
81.00	5328.0
82.00	1144.0
83.30	96.0
85.90	388.0
87.00	7862.0
88.00	6948.0
91.00	630.0
92.00	5255.0
93.10	8021.0
94.10	21104.0
95.10	187904.0
96.10	11986.0
97.10	406.0
103.10	245.0
103.90	729.0
105.00	211.0
106.00	739.0
107.10	149.0
108.00	115.0
110.00	145.0
111.10	178.0
112.10	208.0
113.10	97.0
115.00	241.0
115.90	544.0
117.00	1453.0
117.90	556.0
119.00	1180.0
123.90	80.0
124.80	247.0
126.00	164.0
126.90	62.0
128.00	584.0
129.00	333.0
130.00	541.0
130.90	238.0
133.10	570.0
134.20	180.0
135.00	362.0
137.00	223.0
139.90	101.0
141.00	1275.0
141.90	199.0
143.00	2318.0
143.90	155.0
144.90	1066.0
145.90	395.0
146.90	218.0
148.00	351.0

Instrument :
MSVOA_W
ClientSampleId :
BFB401

148.90	112.0
150.00	136.0
152.10	109.0
153.10	119.0
154.00	156.0
155.00	359.0
155.80	89.0
156.90	252.0
157.80	52.0
158.80	189.0
161.10	197.0
163.10	187.0
169.50	59.0
169.90	73.0
171.10	432.0
172.10	2002.0
173.00	1948.0
174.00	139008.0
175.00	9302.0
176.00	128560.0
177.00	8499.0
178.00	295.0
178.60	84.0
179.20	177.0
188.90	64.0
191.00	771.0
191.90	152.0
192.90	731.0
194.10	233.0
194.80	145.0
202.90	102.0
205.10	167.0
207.00	502.0
207.90	79.0
209.20	60.0
235.00	141.0
249.10	366.0
250.20	155.0
251.00	261.0
252.10	89.0
265.10	852.0
266.10	270.0
267.00	265.0
279.00	77.0
279.90	148.0
281.20	7400.0
282.20	2181.0
283.20	1309.0
284.20	329.0
285.20	66.0

Instrument :
MSVOA_W
ClientSampleId :
BFB401

m/z	Abundance
36.00	1264.0
37.10	7562.0
38.10	6338.0
39.00	2897.0
40.00	335.0
43.10	67.0
44.10	873.0
45.10	1411.0
46.10	186.0
47.00	2561.0
48.10	1125.0
49.00	7362.0
50.10	31112.0
51.10	10183.0
52.10	402.0
53.00	172.0
55.00	472.0
56.00	2332.0
57.10	4730.0
58.10	224.0
58.90	91.0
60.00	1658.0
61.10	8325.0
62.10	8484.0
63.10	6812.0
64.00	1173.0
65.10	1453.0
66.10	83.0
67.10	512.0
68.00	18136.0
69.10	18328.0
70.00	1278.0
71.10	75.0
72.10	1035.0
73.00	8648.0
74.10	30096.0
75.10	96864.0
76.10	8521.0
77.10	1013.0
77.90	924.0
79.00	5263.0
80.00	1760.0
81.00	5777.0
82.00	1354.0
82.90	142.0
85.90	252.0
87.00	7747.0
88.00	7801.0
91.00	699.0
92.10	5590.0
93.10	8237.0
94.10	22192.0
95.10	196736.0
96.10	13339.0
97.10	364.0
102.80	108.0
103.80	767.0
104.90	406.0
105.90	857.0
106.80	302.0
108.00	135.0
110.00	176.0
111.00	137.0
112.00	129.0
113.10	116.0
115.00	187.0
116.00	789.0
117.00	1272.0
118.00	682.0
119.00	1331.0
124.00	154.0
125.10	124.0
126.00	99.0
127.00	66.0
127.90	777.0
128.90	288.0
129.90	627.0
131.00	300.0
132.20	64.0
133.10	337.0
133.80	141.0
134.90	477.0
136.10	59.0
136.90	286.0
139.80	126.0
141.00	1663.0
142.00	273.0
143.00	2383.0
144.00	212.0
144.90	643.0
145.90	348.0
147.00	166.0

Instrument :
MSVOA_W
ClientSampleId :
BFB401

147.90	448.0
148.80	152.0
149.90	175.0
152.00	187.0
153.10	156.0
154.10	110.0
155.00	553.0
155.90	89.0
157.00	365.0
157.90	55.0
159.10	212.0
160.80	241.0
171.10	290.0
172.00	2186.0
174.00	152832.0
175.00	13027.0
176.00	147008.0
177.00	9602.0
178.00	351.0
179.20	128.0
191.10	327.0
192.20	167.0
193.00	476.0
194.10	69.0
205.10	69.0
207.10	346.0
209.10	67.0
249.10	273.0
249.80	70.0
250.30	77.0
251.20	331.0
252.10	74.0
265.00	560.0
266.00	181.0
267.10	87.0
281.20	4885.0
282.10	1130.0
283.10	1035.0
284.20	167.0

Instrument :
MSVOA_W
ClientSampleId :
BFB401

m/z	Abundance
36.00	769.0
37.10	5021.0
38.10	4410.0
39.10	2102.0
39.90	274.0
43.30	102.0
44.00	761.0
45.10	886.0
46.00	154.0
47.10	1589.0
48.00	710.0
49.10	4779.0
50.10	23616.0
51.10	7056.0
52.00	348.0
53.10	84.0
54.10	82.0
55.10	320.0
56.10	1787.0
57.10	3324.0
58.20	98.0
60.10	1014.0
61.10	6148.0
62.10	5951.0
63.10	4922.0
64.10	517.0
65.00	633.0
66.00	109.0
67.00	247.0
68.10	13254.0
69.10	14045.0
70.00	921.0
71.20	54.0
72.00	761.0
73.00	6068.0
74.10	21656.0
75.10	71608.0
76.10	5929.0
76.90	678.0
78.10	634.0
79.00	3651.0
80.10	1329.0
81.00	4065.0
82.00	878.0
83.00	138.0
85.80	244.0
87.00	6167.0
88.00	5773.0
91.10	379.0
92.00	3468.0
93.00	5594.0
94.10	16096.0
95.10	142464.0
96.10	9662.0
97.10	293.0
102.90	161.0
103.10	157.0
104.00	492.0
105.00	279.0
106.00	553.0
107.00	176.0
108.20	75.0
110.00	96.0
110.90	216.0
111.90	123.0
113.00	83.0
115.10	218.0
116.00	462.0
117.00	1140.0
118.00	550.0
118.90	854.0
124.00	81.0
126.00	74.0
127.90	425.0
128.80	262.0
130.00	627.0
130.90	203.0
133.00	146.0
134.10	62.0
135.00	225.0
137.10	236.0
141.00	1422.0
141.90	194.0
143.00	1400.0
144.10	155.0
145.00	510.0
145.90	199.0
146.90	87.0
148.00	351.0
148.90	182.0
150.00	178.0
152.00	129.0

Instrument :
MSVOA_W
ClientSampleId :
BFB401

153.10	67.0
154.10	123.0
155.00	394.0
156.90	330.0
159.10	153.0
161.10	315.0
170.80	215.0
172.10	1521.0
174.00	131776.0
175.00	8722.0
176.00	131584.0
177.00	9039.0
177.90	383.0
191.10	178.0
192.20	60.0
193.00	151.0
207.20	226.0
249.00	180.0
251.10	55.0
265.10	206.0
267.00	66.0
281.10	2111.0
282.20	586.0
283.20	359.0
284.10	108.0

Instrument :
MSVOA_W
ClientSampleId :
BFB401