

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112018\
 Data File : VW006965.D
 Acq On : 20 Nov 2018 01:14
 Operator : SY/AP
 Sample : J5977-13
 Misc : 5.04G/5ML/MSVOA W/SOIL
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DUP-01

Quant Time: Nov 20 06:30:30 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W111718S.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 17 04:45:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	99098	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	152479	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	132885	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	57633	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	47467	42.98	ug/l	0.00
Spiked Amount	50.000		Recovery	=	85.96%	
35) Dibromofluoromethane	7.89	113	43907	49.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.36%	
50) Toluene-d8	10.32	98	175517	45.75	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.50%	
62) 4-Bromofluorobenzene	12.62	95	61390	41.03	ug/l	0.00
Spiked Amount	50.000		Recovery	=	82.06%	
Target Compounds						
16) Acetone	4.15	43	2235	13.231	ug/l	95
20) Methylene Chloride	4.93	84	5258	1.228	ug/l	88
86) p-Isopropyltoluene	13.51	119	6466	1.554	ug/l	89
95) Naphthalene	15.37	128	14170	6.608	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW112018\
Data File : VW006965.D
Acq On : 20 Nov 2018 01:14
Operator : SY/AP
Sample : J5977-13
Misc : 5.04G/5ML/MSVOA W/SOIL
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DUP-01

Quant Time: Nov 20 06:30:30 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W111718S.M
Quant Title : SW846 8260
QLast Update : Sat Nov 17 04:45:18 2018
Response via : Initial Calibration

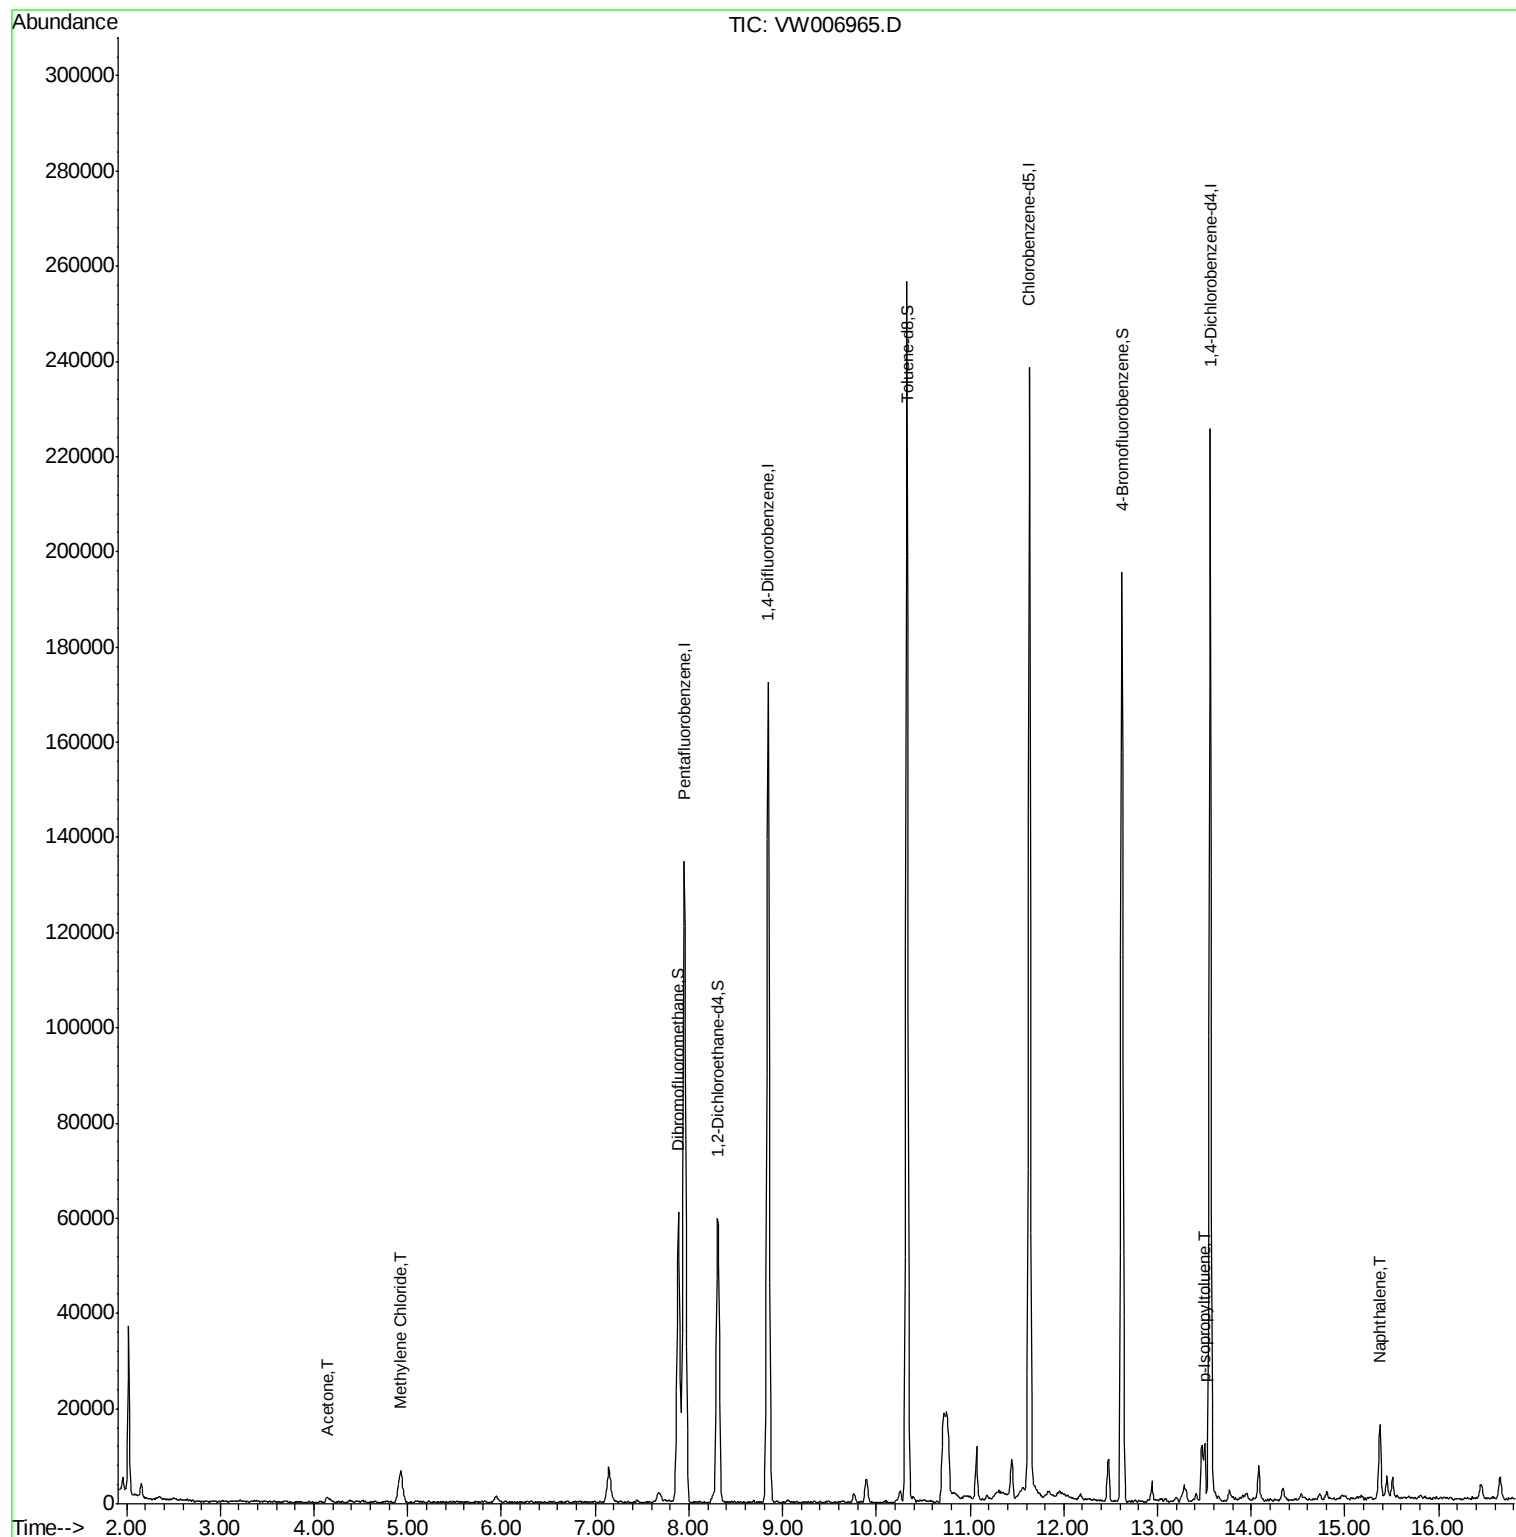

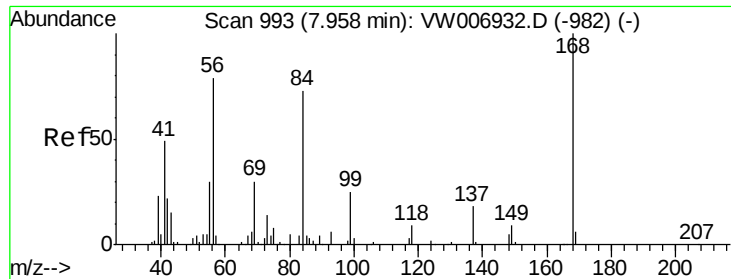

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. -0.01 min

Lab File: VW006965.D

Acq: 20 Nov 2018 01:14

Instrument :

MSVOA_W

ClientSampled :


DUP-01

Tot Ion:168 Resp: 99098

Ion Ratio Lower Upper




168 100

99 60.0 49.3 73.9

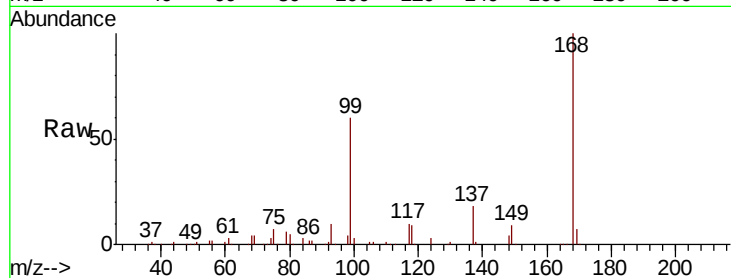

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

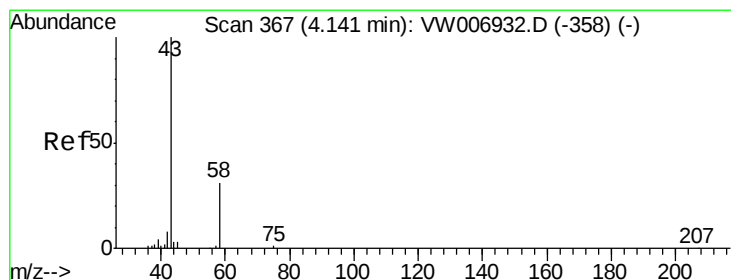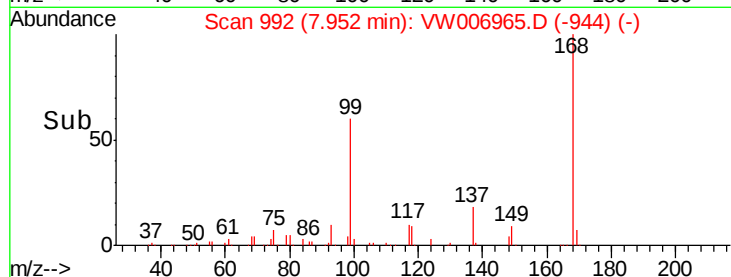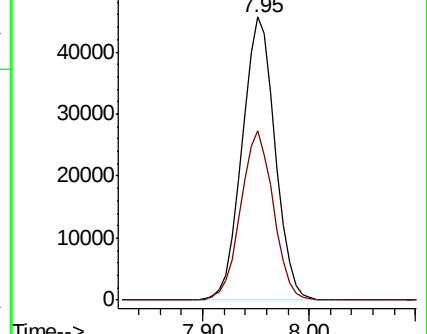

#16

Acetone

Concen: 13.231 ug/l

RT: 4.15 min Scan# 368

Delta R.T. 0.01 min

Lab File: VW006965.D


Acq: 20 Nov 2018 01:14

Tgt Ion: 43 Resp: 2235

Ion Ratio Lower Upper



43 100


58 27.5 24.2 36.4

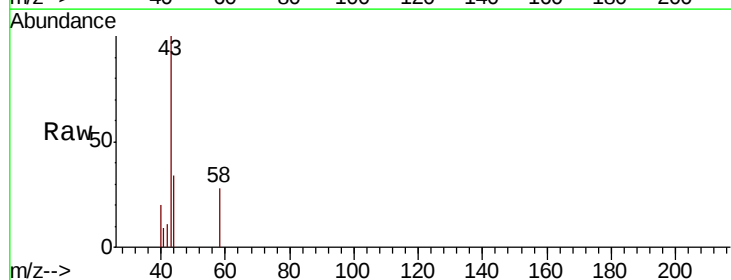

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

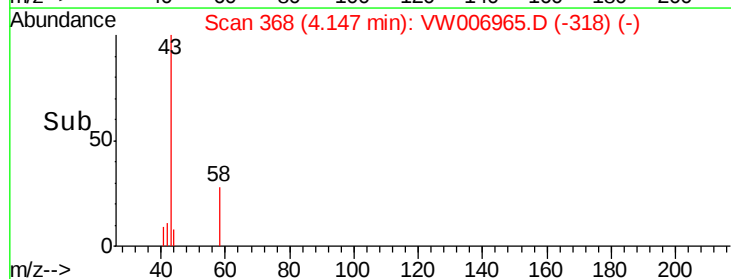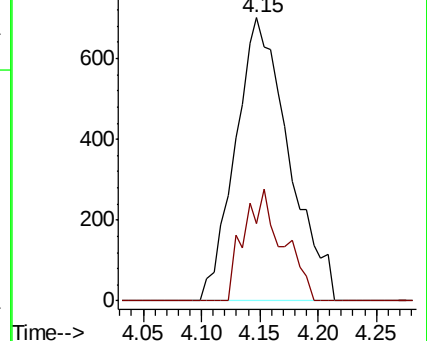

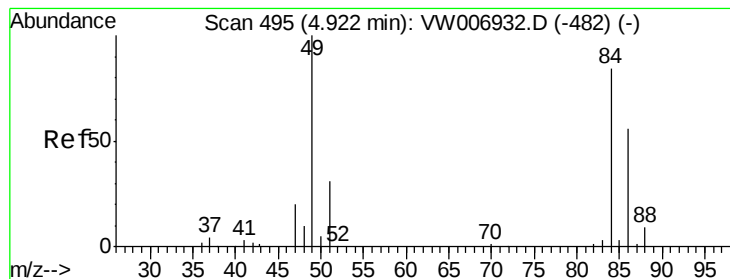

#20

Methvlene Chloride

Concen: 1.228 ug/l

RT: 4.93 min Scan# 496

Delta R.T. 0.01 min

Lab File: VW006965.D

Acq: 20 Nov 2018 01:14

Instrument :

MSVOA_W

ClientSampled :

DUP-01

Tot Ion: 84 Resp: 5258



Ion Ratio Lower Upper

84 100

49 97.1 95.4 143.2

51 34.4 29.5 44.3

86 65.4 53.4 80.2

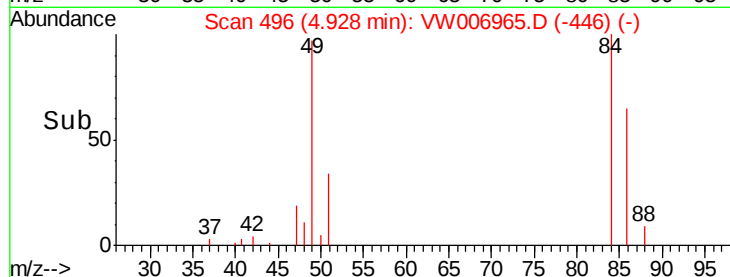
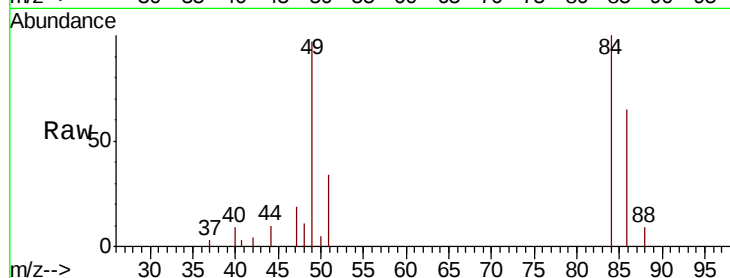


Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW

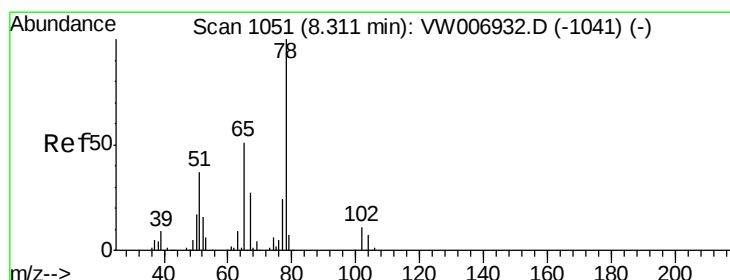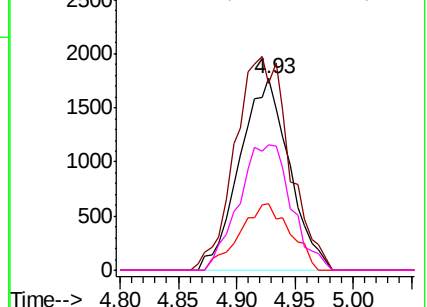

#33

1,2-Dichloroethane-d4

Concen: 42.980 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.01 min

Lab File: VW006965.D



Acq: 20 Nov 2018 01:14

Tgt Ion: 65 Resp: 47467

Ion Ratio Lower Upper


65 100


67 52.8 0.0 104.0

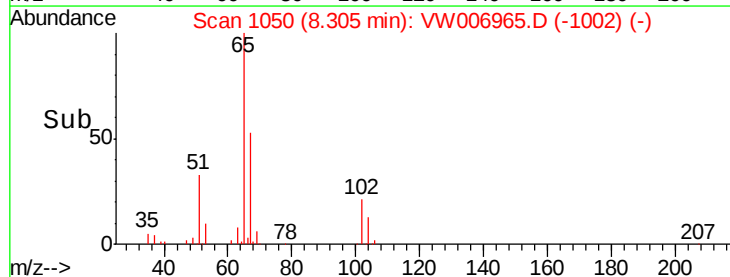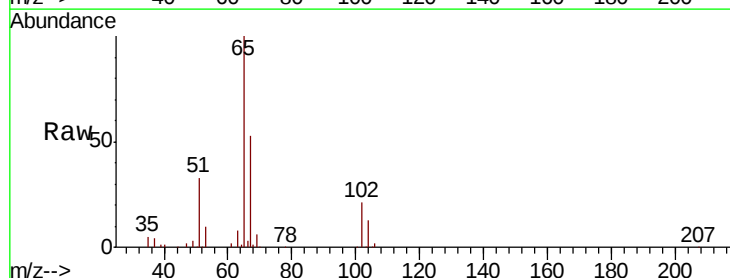

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

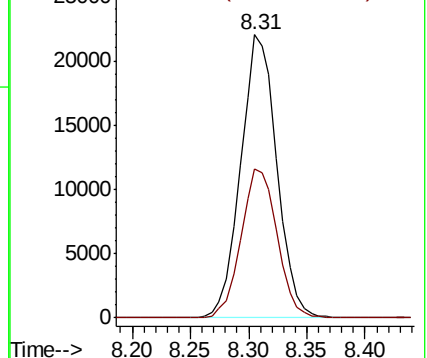


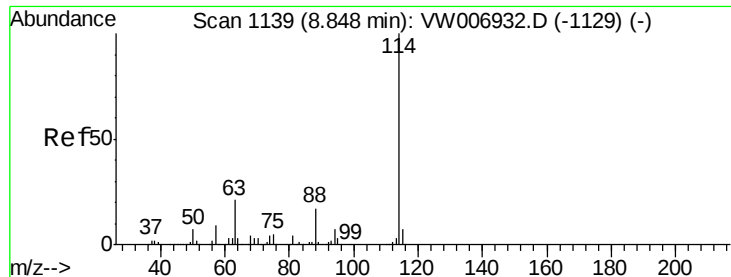




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.85 min Scan# 1139
 Delta R.T. 0.00 min
 Lab File: VW006965.D
 Acq: 20 Nov 2018 01:14

Instrument :
 MSVOA_W
 ClientSampled :
 DUP-01

Tot Ion:114 Resp: 152479
 Ion Ratio Lower Upper
 114 100
 63 20.7 0.0 42.2
 88 15.5 0.0 33.4

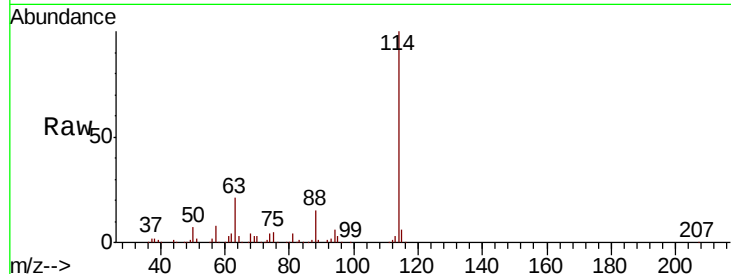


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

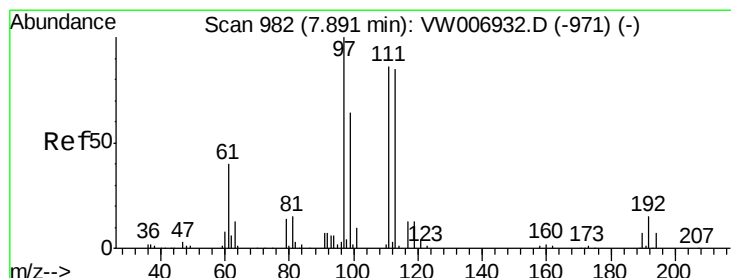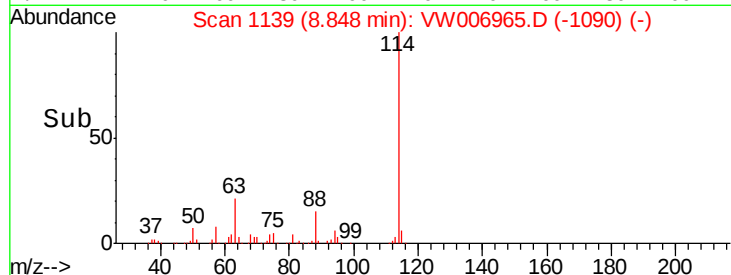
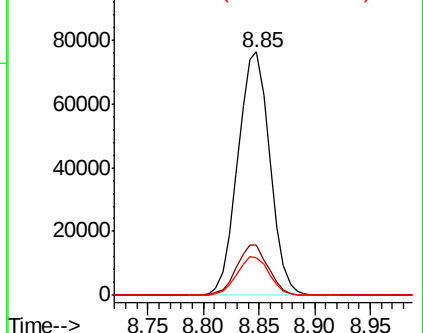



#35
 Dibromofluoromethane
 Concen: 49.178 ug/l
 RT: 7.89 min Scan# 982
 Delta R.T. 0.00 min
 Lab File: VW006965.D
 Acq: 20 Nov 2018 01:14

Tgt Ion:113 Resp: 43907
 Ion Ratio Lower Upper
 113 100
 111 104.0 81.7 122.5
 192 18.6 13.9 20.9

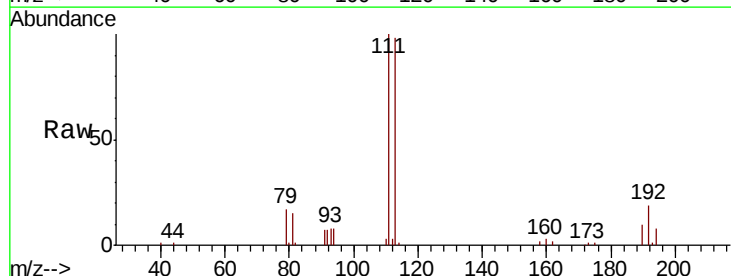

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

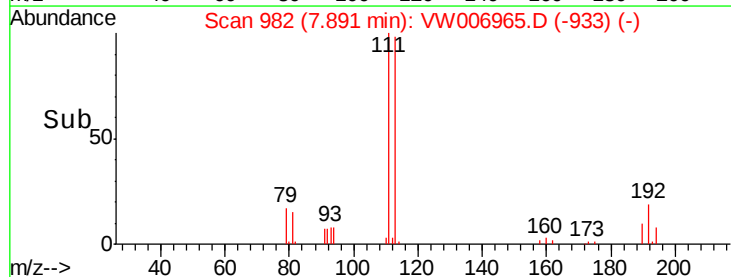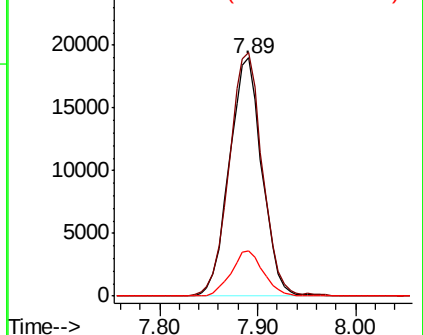

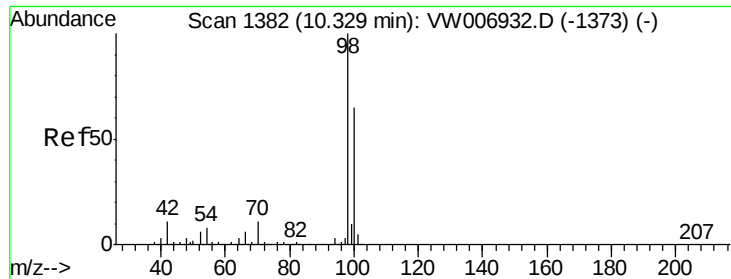

#50

Toluene-d8

Concen: 45.746 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.01 min

Lab File: VW006965.D

Acq: 20 Nov 2018 01:14

Instrument :

MSVOA_W

ClientSampled :


DUP-01

Tot Ion: 98 Resp: 175517

Ion Ratio Lower Upper




98 100

100 65.1 52.3 78.5

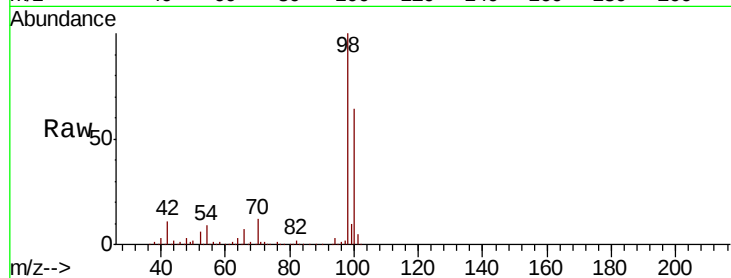

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

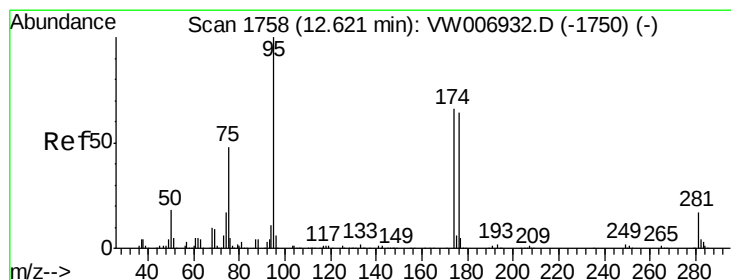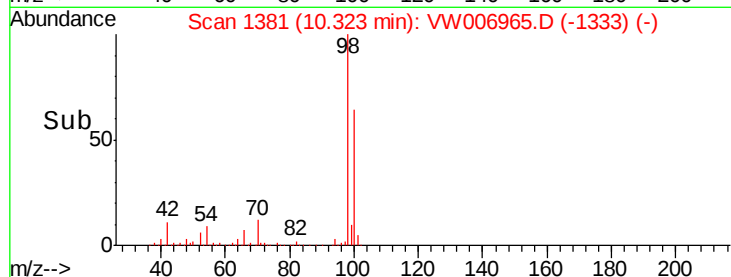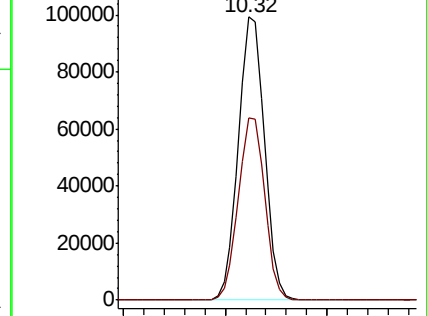

#62

4-Bromofluorobenzene

Concen: 41.035 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.00 min

Lab File: VW006965.D

Acq: 20 Nov 2018 01:14


Tgt Ion: 95 Resp: 61390

Ion Ratio Lower Upper

95 100

174 74.3 0.0 138.4



176 70.7 0.0 133.4

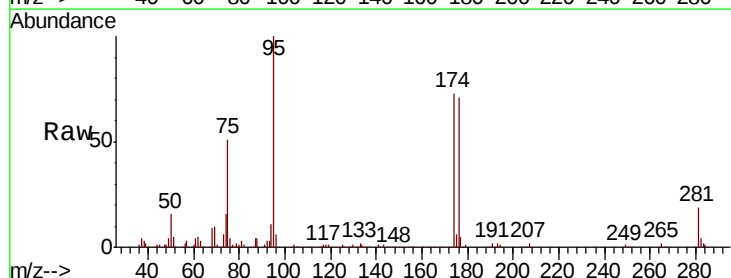


Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



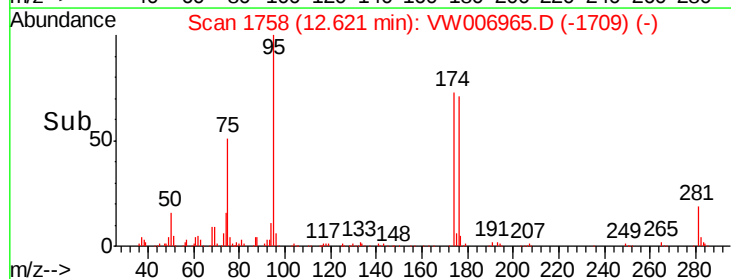
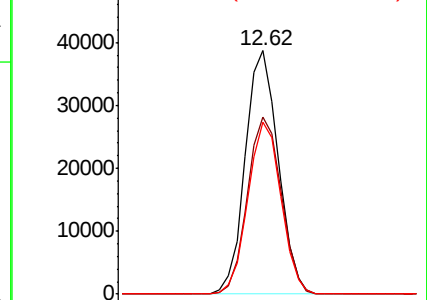


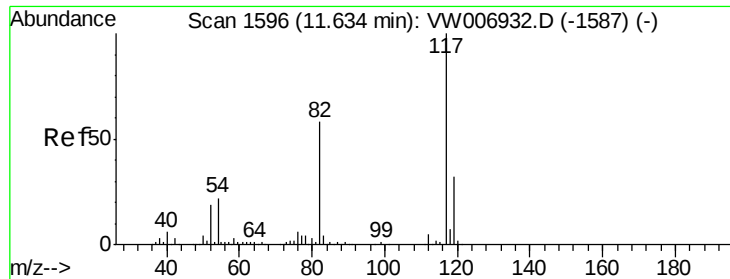

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW006965.D
Acq: 20 Nov 2018 01:14




Instrument :
MSVOA_W
ClientSampleID :
DUP-01


Tot Ion:117 Resp: 132885
Ion Ratio Lower Upper
117 100
82 56.2 46.2 69.2
119 31.8 25.5 38.3

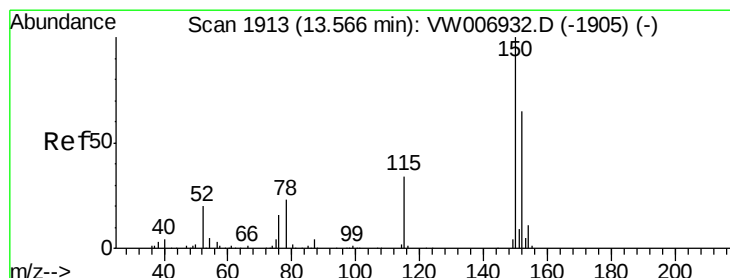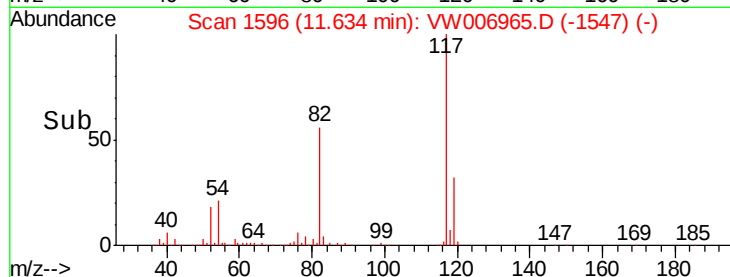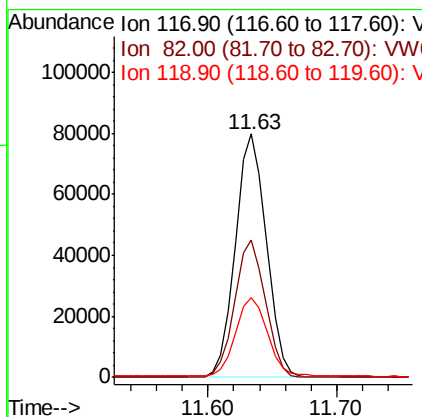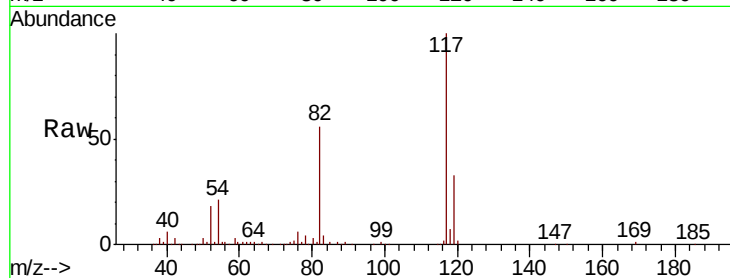

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.01 min
Lab File: VW006965.D
Acq: 20 Nov 2018 01:14

Tgt Ion:152 Resp: 57633
Ion Ratio Lower Upper
152 100
115 61.0 31.6 94.7
150 157.3 0.0 350.0


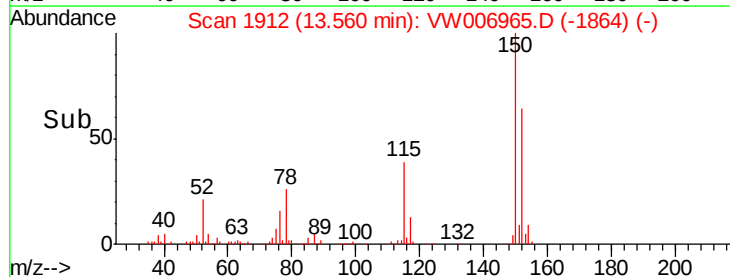
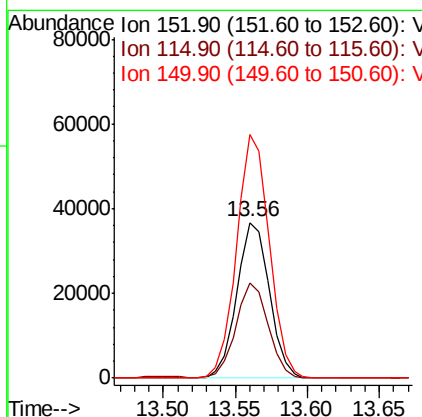
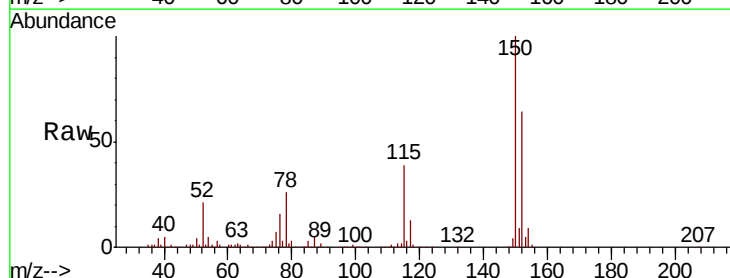


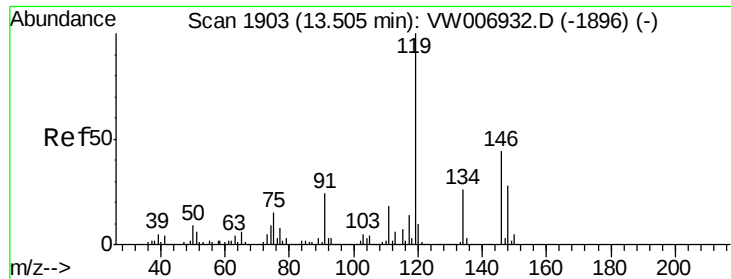

#86
 p-Isopropyltoluene
 Concen: 1.554 ug/l
 RT: 13.51 min Scan# 1903
 Delta R.T. 0.00 min
 Lab File: VW006965.D
 Acq: 20 Nov 2018 01:14

Instrument :
 MSVOA_W
 ClientSampleId :
 DUP-01

Tot Ion:119 Resp: 6466
 Ion Ratio Lower Upper
 119 100
 134 25.8 12.7 38.1
 91 35.2 12.4 37.2

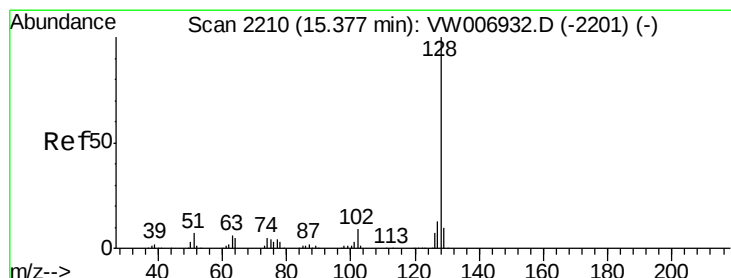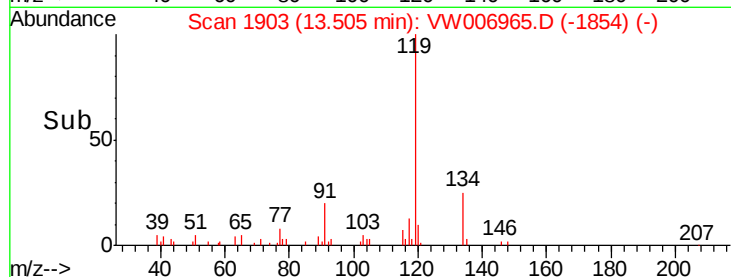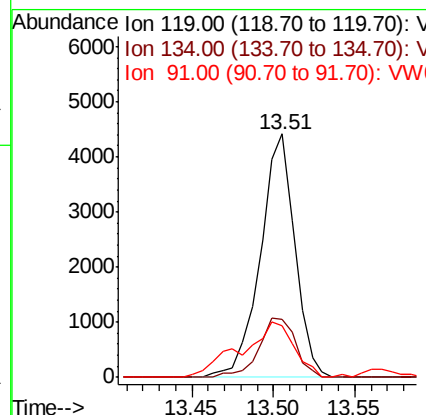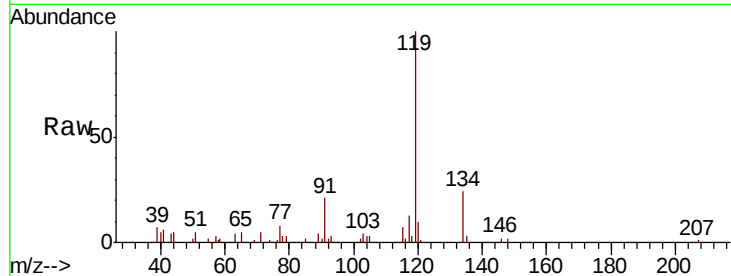

#95
 Naphthalene
 Concen: 6.608 ug/l
 RT: 15.37 min Scan# 2209
 Delta R.T. -0.01 min
 Lab File: VW006965.D
 Acq: 20 Nov 2018 01:14

Tgt Ion:128 Resp: 14170
 Ion Ratio Lower Upper
 128 100
 127 14.2 10.6 15.8
 129 11.6 8.5 12.7

