


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW112018\
 Data File : VW006947.D
 Acq On : 19 Nov 2018 16:36
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W111718S.M
 Title : SW846 8260
 Last Update : Sat Nov 17 04:45:18 2018

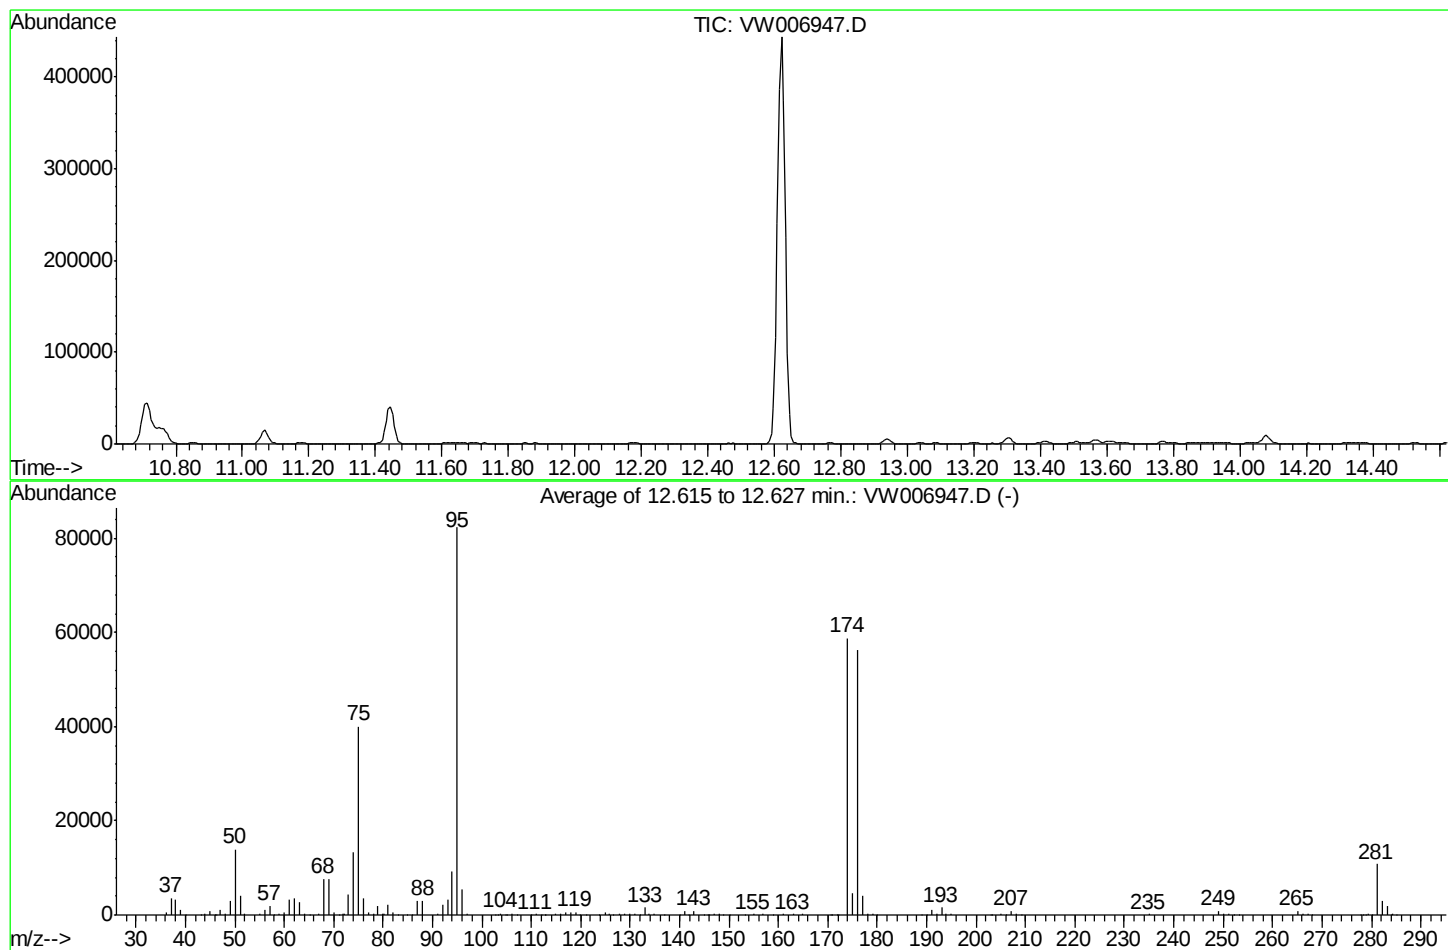

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	13975	PASS
75	95	30	60	48.6	39968	PASS
95	95	100	100	100.0	82301	PASS
96	95	5	9	6.7	5502	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.5	58829	PASS
175	174	5	9	7.9	4630	PASS
176	174	95	101	95.6	56264	PASS
177	176	5	9	7.1	4000	PASS