
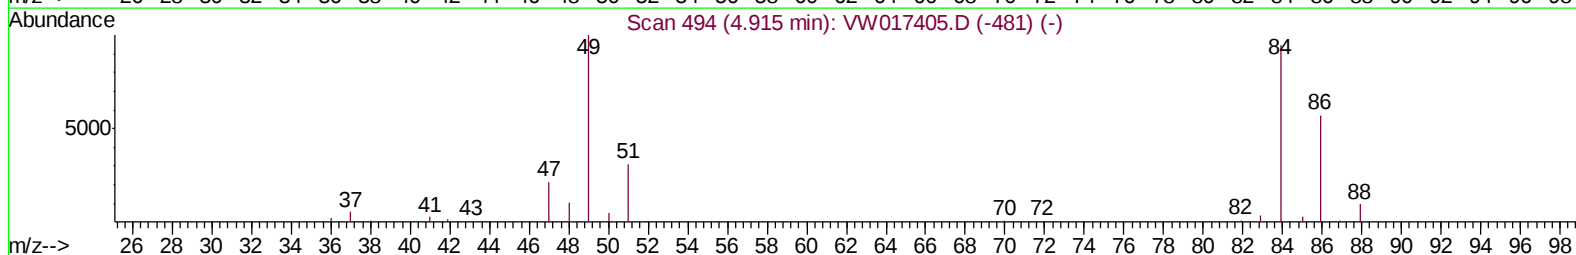
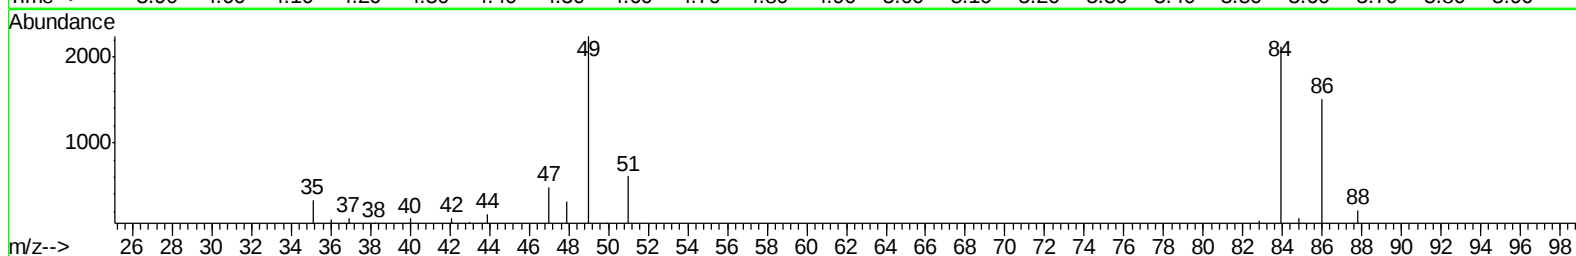


Data File : VW017406.D
Acq On : 20 Nov 2020 10:54
Operator : SY/VA
Sample : VW1120SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 00:31:45 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 21 00:30:34 2020
Response via : Initial Calibration

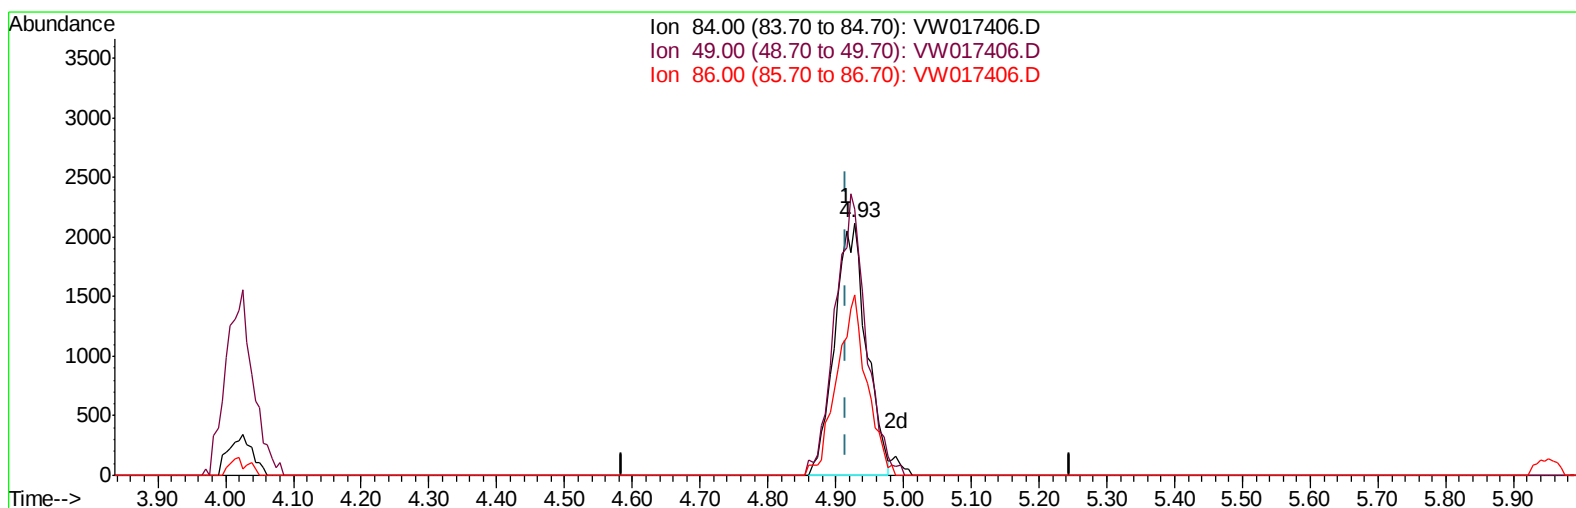

TIC: VW017406.D

(16) Methylene chloride (T)

4.928min (+0.012) 1.21ug/L m

response 6894

Ion	Exp%	Act%
84.00	100	100
49.00	102.20	105.52
86.00	61.10	71.27
0.00	0.00	0.00