
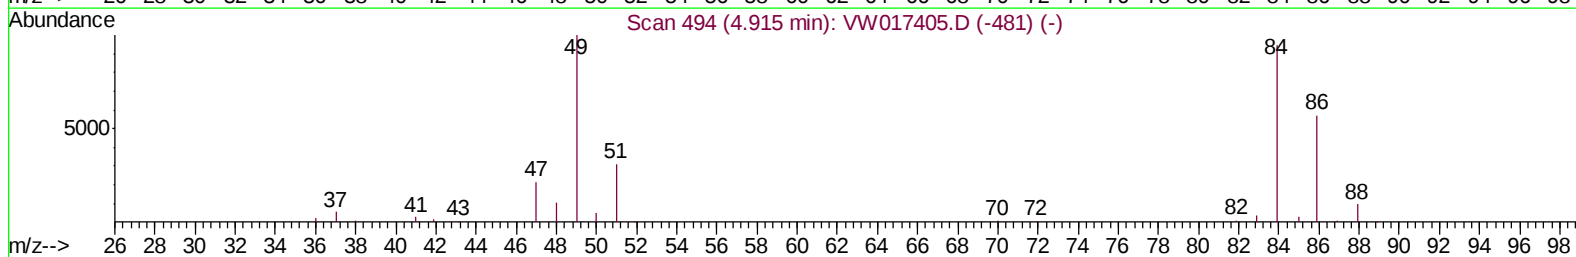
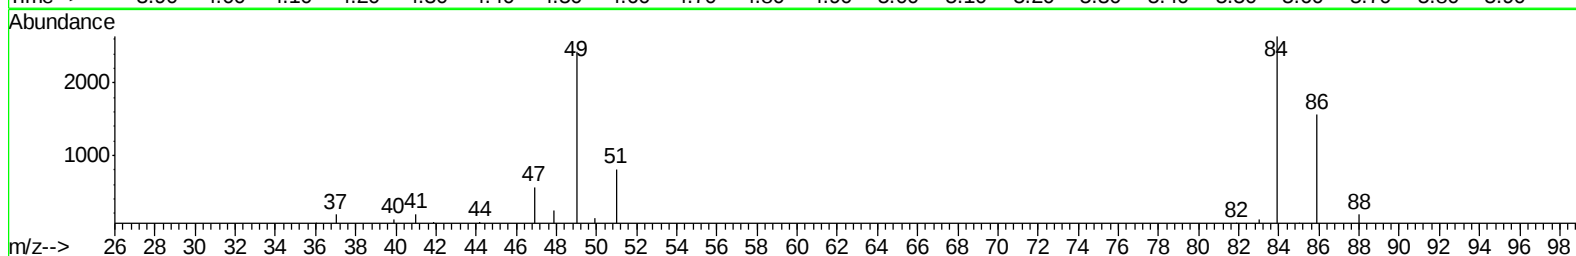


Data File : VW017423.D
Acq On : 20 Nov 2020 17:32
Operator : SY/VA
Sample : VIBLK12
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 00:33:56 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 21 00:30:34 2020
Response via : Initial Calibration

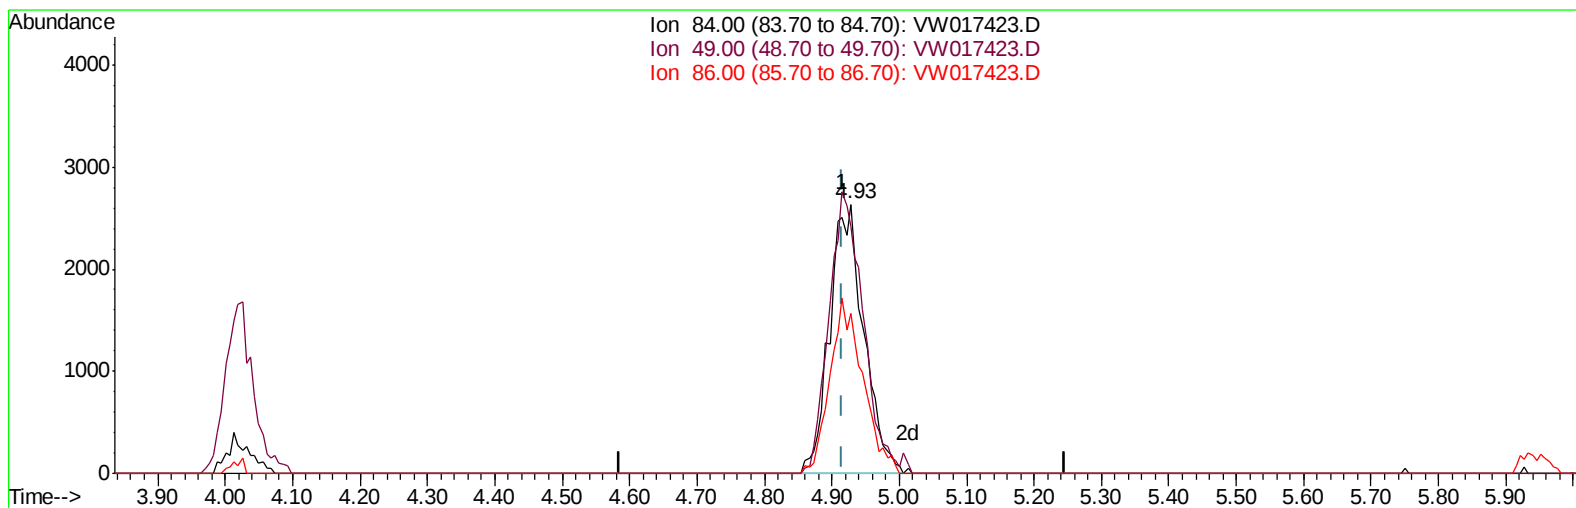

TIC: VW017423.D

(16) Methylene chloride (T)

4.928min (+0.012) 1.51ug/L m

response 9239

Ion	Exp%	Act%
84.00	100	100
49.00	102.20	91.93
86.00	61.10	59.19
0.00	0.00	0.00