
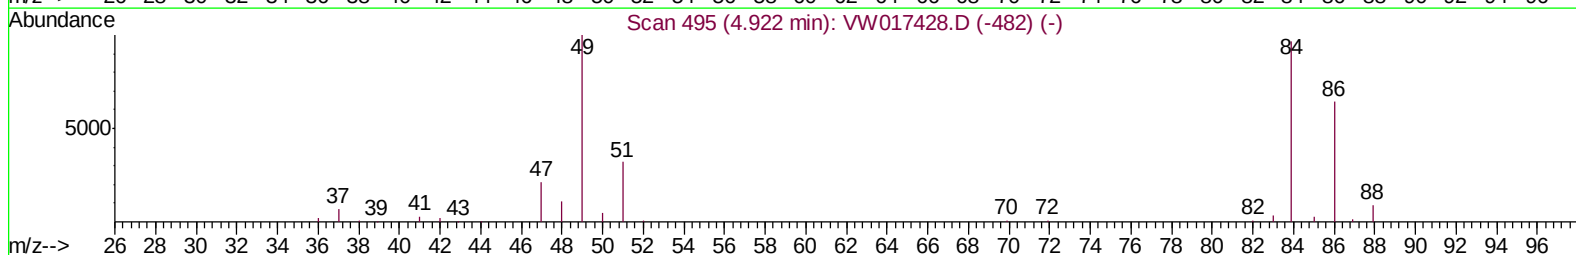
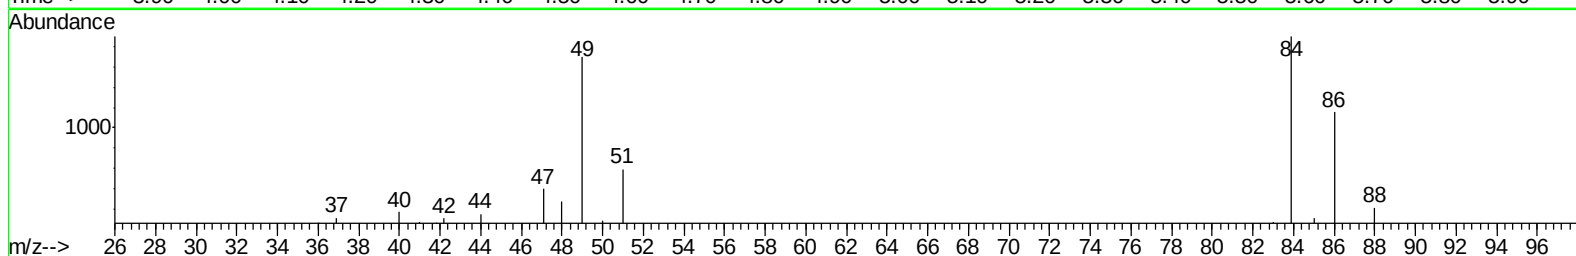


Data File : VW017443.D
Acq On : 21 Nov 2020 02:10
Operator : SY/VA
Sample : L4860-09
Misc : 5.87G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 02:43:13 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 21 02:27:17 2020
Response via : Initial Calibration

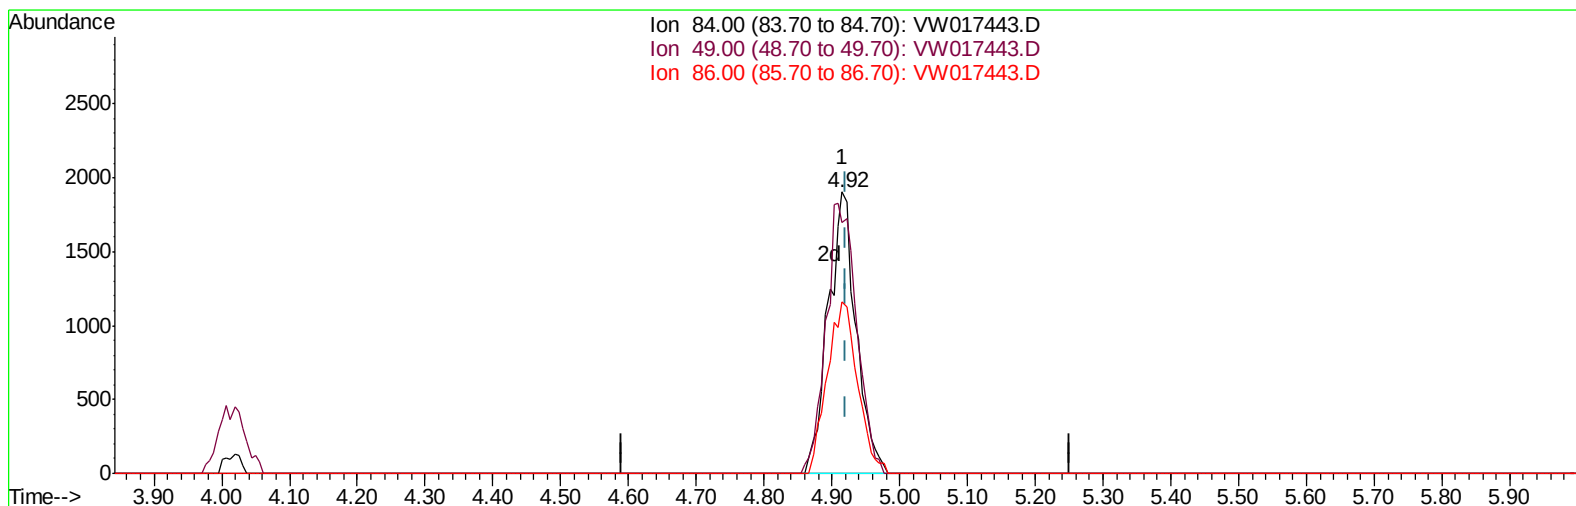

TIC: VW017443.D

(16) Methylene chloride (T)

4.915min (-0.007) 2.63ug/L m

response 5405

Ion	Exp%	Act%
84.00	100	100
49.00	102.20	89.08
86.00	61.10	60.73
0.00	0.00	0.00