

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW112020\
Quantitation Report (Qedit)


Data File : VW017413.D
Acq On : 20 Nov 2020 13:38
Operator : SY/VA
Sample : L4819-03
Misc : 5.39G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AZ3

Quant Time: Nov 21 00:32:39 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 21 00:30:34 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
11/23/2020 12:52:00 PM

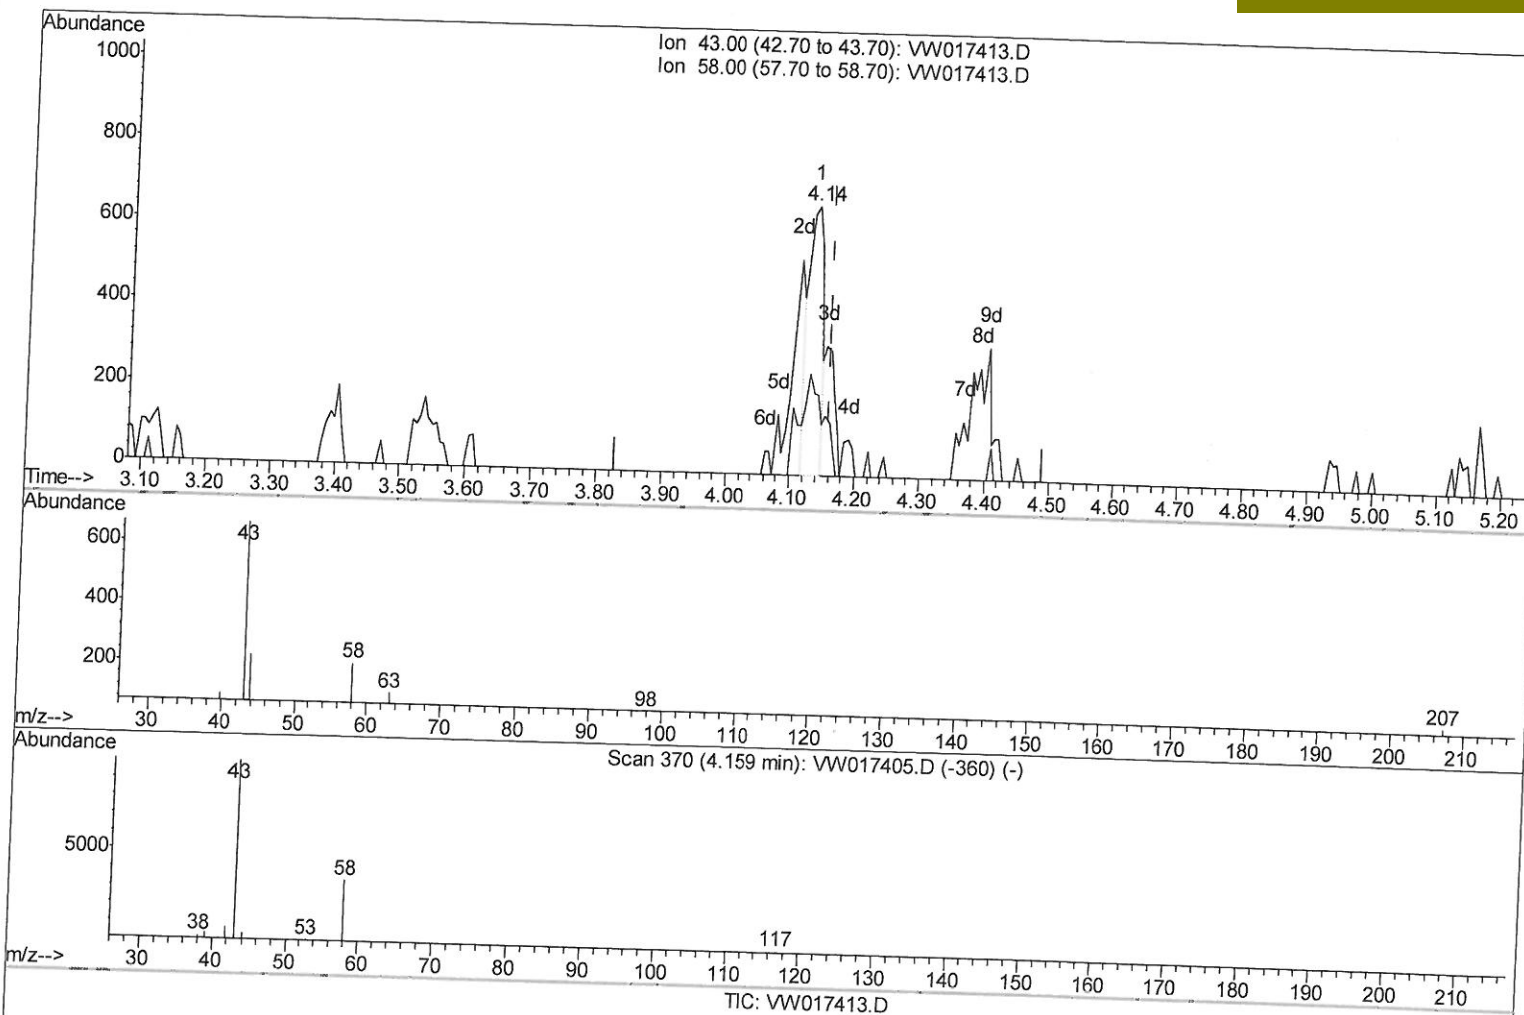

(13) Acetone (T)

4.135min (-0.024) 2.20ug/L

response 982

Ion	Exp%	Act%
43.00	100	100
58.00	33.50	22.61
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW112020\
Quantitation Report (Qedit)


Data File : VW017413.D
Acq On : 20 Nov 2020 13:38
Operator : SY/VA
Sample : L4819-03
Misc : 5.39G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
C0AZ3

Quant Time: Nov 21 00:32:39 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 21 00:30:34 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
11/23/2020 12:52:00 PM

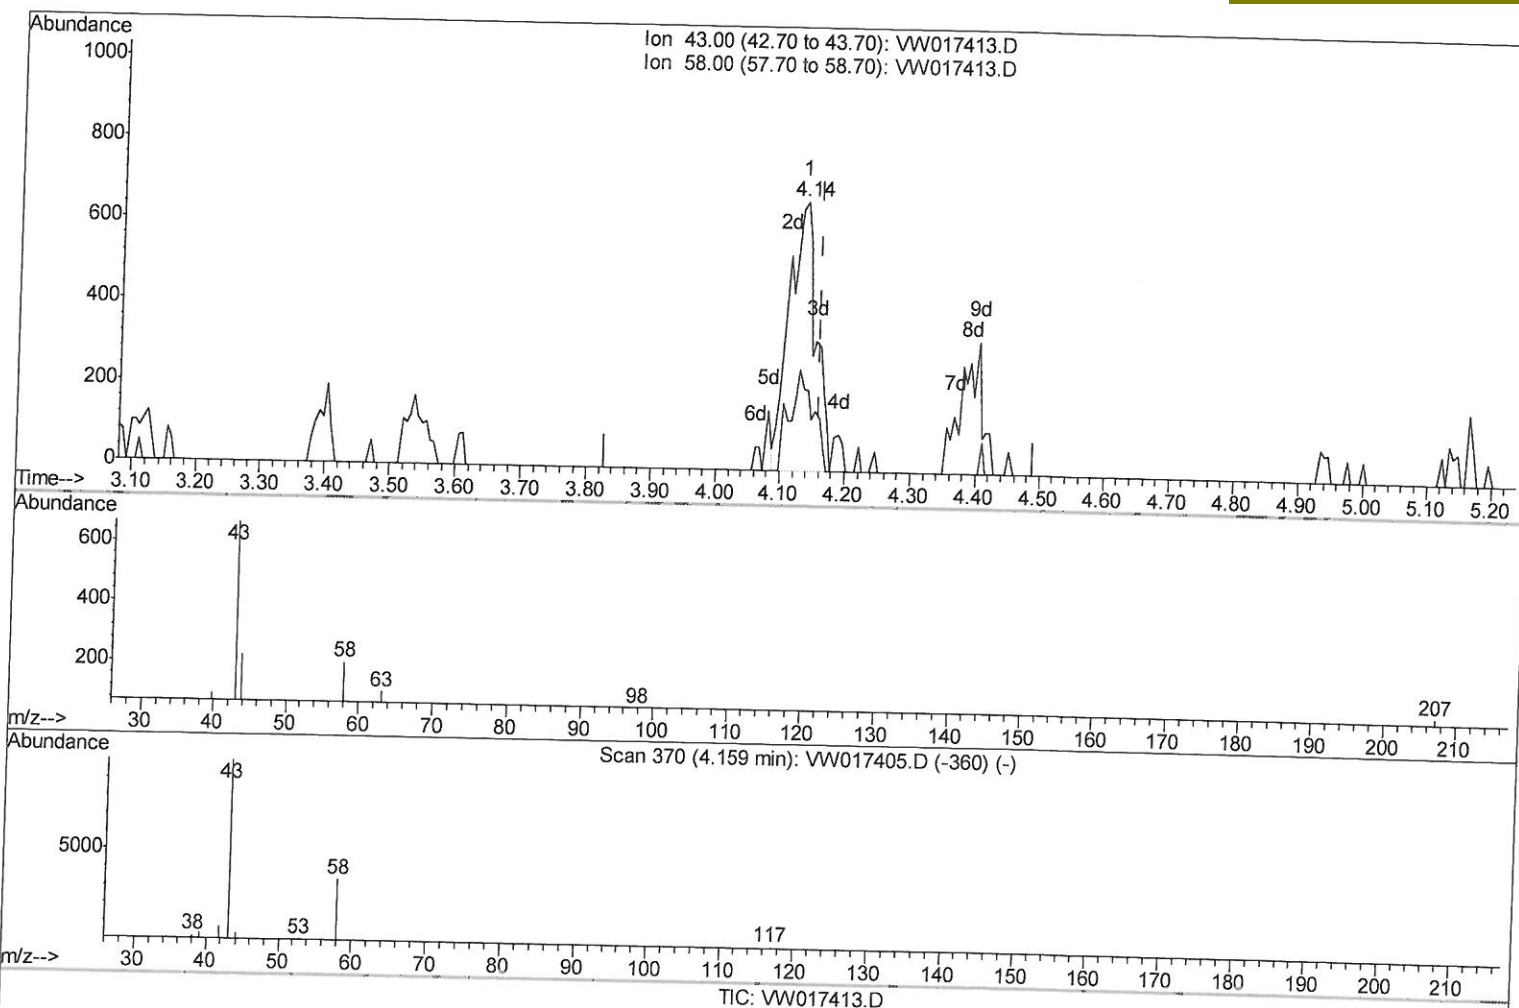

(13) Acetone (T)

4.135min (-0.024) 4.29ug/L m

response 1915

Ion	Exp%	Act%
43.00	100	100
58.00	33.50	11.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW112020\
 Quantitation Report (QT Reviewed)

Data File : VW017413.D
 Acq On : 20 Nov 2020 13:38
 Operator : SY/VA
 Sample : L4819-03
 Misc : 5.39G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 C0AZ3

Quant Time: Nov 21 01:09:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 21 00:30:34 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 11/23/2020 12:52:00 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	251733	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	221122	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	86024	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	92040	24.70	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	98.80%		
7) Chloroethane-d5	2.89	69	76245	25.76	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	103.04%		
10) 1,1-Dichloroethene-d2	4.03	63	117402	18.01	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	72.04%		
20) 2-Butanone-d5	7.08	46	31217	51.00	ug/L	-0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.00%		
24) Chloroform-d	7.65	84	166484	25.17	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	100.68%		
26) 1,2-Dichloroethane-d4	8.31	65	85177	26.66	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	106.64%		
29) Benzene-d6	8.27	84	322473	25.87	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	103.48%		
33) 1,2-Dichloropropane-d6	9.28	67	89129	26.84	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	107.36%		
37) Toluene-d8	10.32	98	289468	24.67	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	98.68%		
38) trans-1,3-Dichloropropene-	10.58	79	34854	24.11	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	96.44%		
39) 2-Hexanone-d5	10.93	63	22008	49.42	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	98.84%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	68798	27.34	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	109.36%		
61) 1,2-Dichlorobenzene-d4	13.85	152	81628	25.70	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	102.80%		

Target Compounds

13) Acetone	4.14	43	1915m	4.288	ug/L	Qvalue
16) Methylene chloride	4.92	84	11714	2.720	ug/L	4125/2052 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW112020\
 Quantitation Report (QT Reviewed)
 Data File : VW017413.D
 Acq On : 20 Nov 2020 13:38
 Operator : SY/VA
 Sample : L4819-03
 Misc : 5.39G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 C0AZ3

Quant Time: Nov 21 01:09:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 21 00:30:34 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 11/23/2020 12:52:00 PM

