

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112020\
 Data File : VW017436.D
 Acq On : 20 Nov 2020 23:25
 Operator : SY/VA
 Sample : L4819-15
 Misc : 6.21G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BB3

Manual Integrations
 APPROVED

MMDadoda
 11/23/2020 12:52:27 PM

Quant Time: Nov 21 03:29:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 21 02:27:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	246950	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	229280	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	109698	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.34	65	68100	18.63	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.52%
7) Chloroethane-d5	2.89	69	60003	20.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.64%
10) 1,1-Dichloroethene-d2	4.01	63	100741	15.75	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.00%
20) 2-Butanone-d5	7.07	46	35151	58.54	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.08%
24) Chloroform-d	7.65	84	151844	23.41	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.64%
26) 1,2-Dichloroethane-d4	8.30	65	84290	26.89	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.56%
29) Benzene-d6	8.27	84	294550	22.79	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.16%
33) 1,2-Dichloropropane-d6	9.27	67	84246	24.47	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.88%
37) Toluene-d8	10.32	98	279351	22.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.84%
38) trans-1,3-Dichloropropene-	10.58	79	34816	23.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.88%
39) 2-Hexanone-d5	10.93	63	27247	59.01	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.02%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	74566	28.58	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.32%
61) 1,2-Dichlorobenzene-d4	13.85	152	100810	24.89	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.56%

Target Compounds					Ovalue
13) Acetone	4.13	43	1330m	3.036	ug/L
16) Methylene chloride	4.92	84	13903	3.291	ug/L
43) 4-Methyl-2-pentanone	10.21	43	1123	0.772	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW112020\
Data File : VW017436.D
Acq On : 20 Nov 2020 23:25
Operator : SY/VA
Sample : L4819-15
Misc : 6.21G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0BB3

Manual Integrations
APPROVED

MMDadoda
11/23/2020 12:52:27 PM

Quant Time: Nov 21 03:29:25 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 21 02:27:17 2020
Response via : Initial Calibration

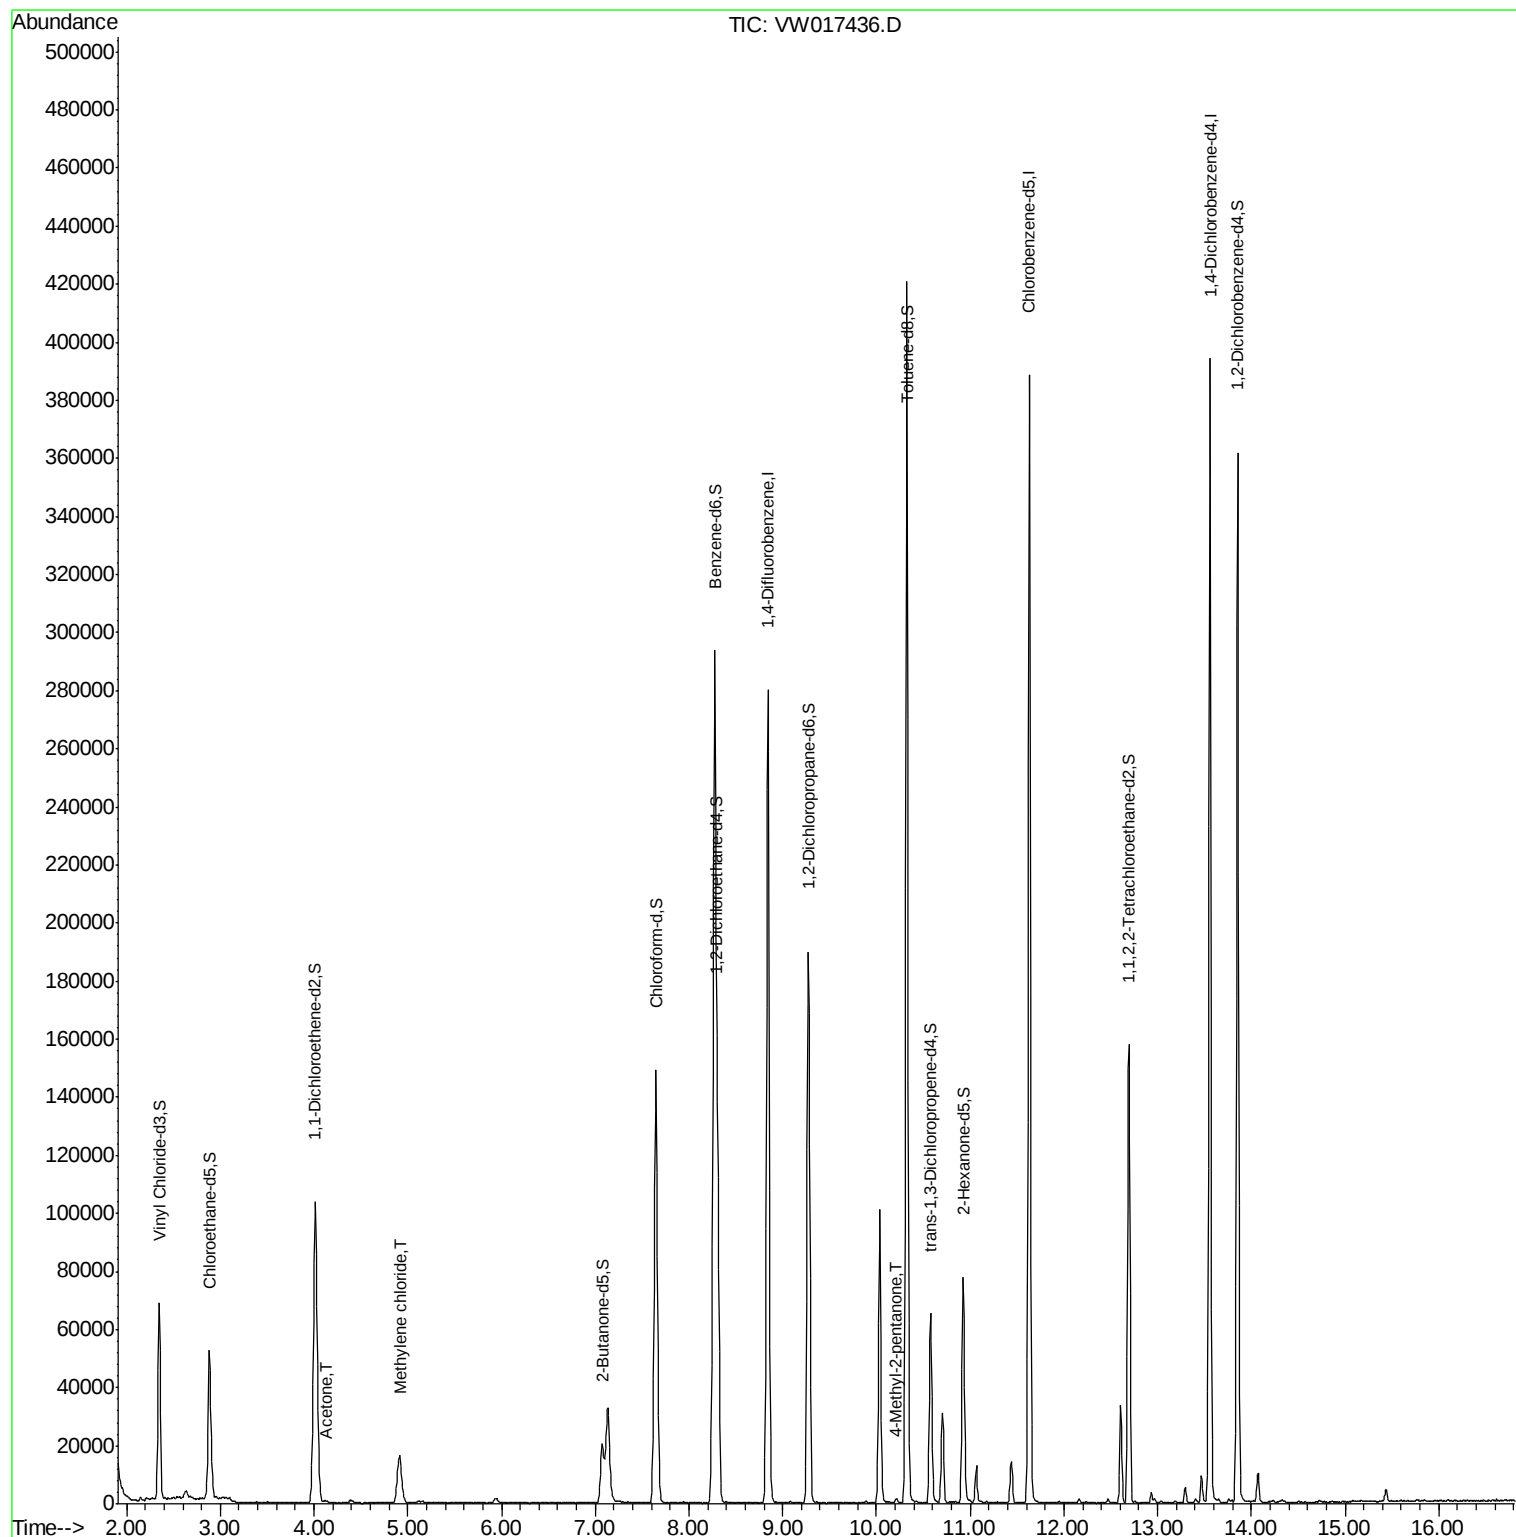

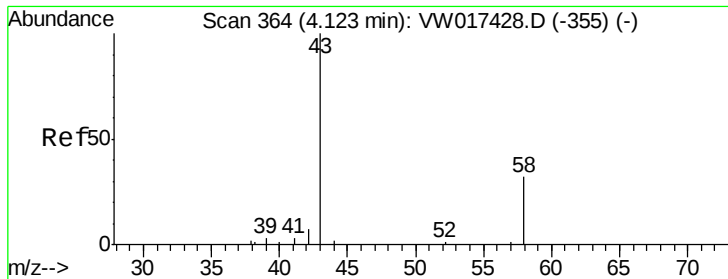

#13

Acetone

Concen: 3.036 ug/L m

RT: 4.13 min Scan# 365

Delta R.T. 0.01 min

Lab File: VW017436.D

Acq: 20 Nov 2020 23:25

Instrument :

MSVOA_W

ClientSampled :

C0BB3

Tot Ion: 43 Resp: 1330

Ion Ratio Lower Upper

43 100





58 14.5 0.0 67.0

Manual Integrations

APPROVED

MMDadoda

11/23/2020 12:52:27 PM

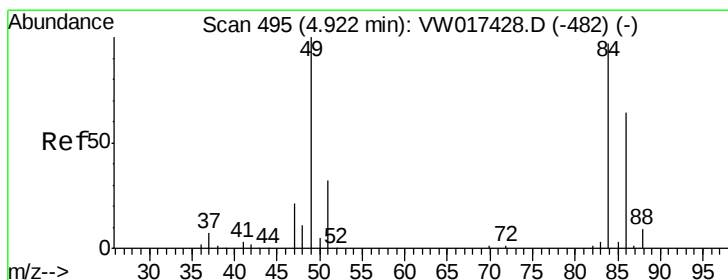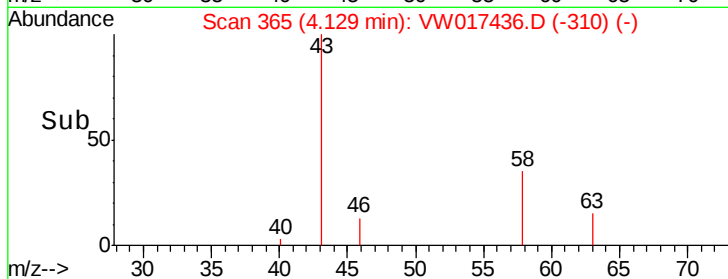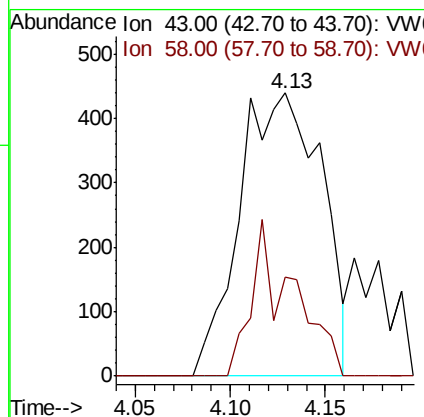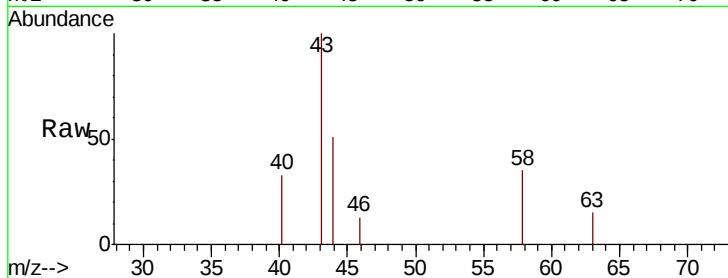

#16

Methylene chloride

Concen: 3.291 ug/L

RT: 4.92 min Scan# 494

Delta R.T. -0.01 min

Lab File: VW017436.D

Acq: 20 Nov 2020 23:25




Tgt Ion: 84 Resp: 13903


Ion Ratio Lower Upper

84 100

49 107.0 71.5 132.9

86 62.4 42.8 79.4

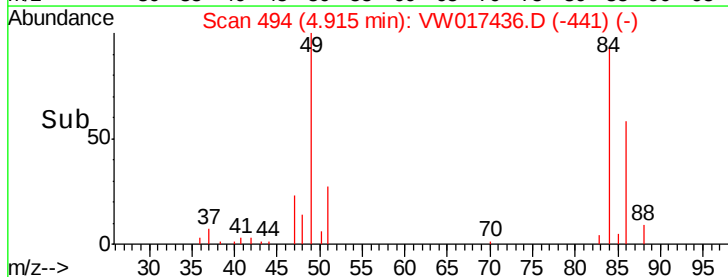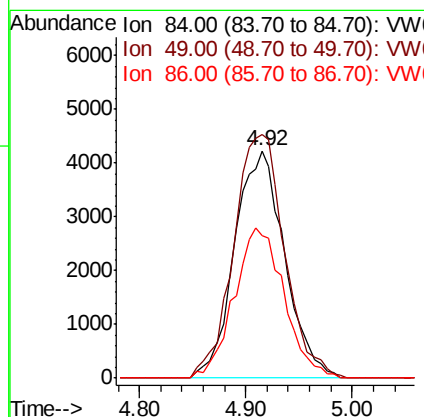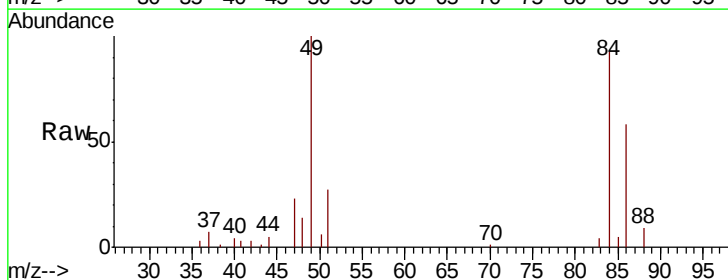

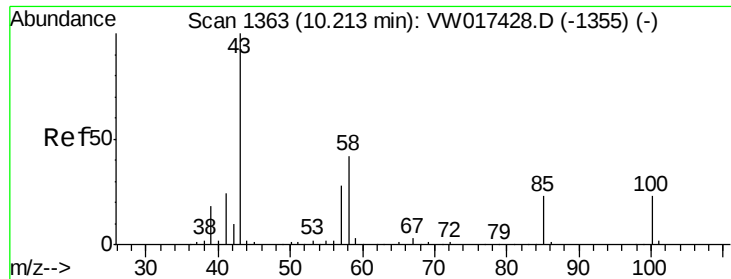

#43
 4-Methyl-2-pentanone
 Concen: 0.772 ug/L
 RT: 10.21 min Scan# 1363
 Delta R.T. -0.00 min
 Lab File: VW017436.D
 Acq: 20 Nov 2020 23:25

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BB3

Tot Ion	Ratio	Lower	Upper
43	100		
58	35.4	33.4	50.2
100	16.7	16.3	24.5

Manual Integrations
 APPROVED

MMDadoda
 11/23/2020 12:52:27 PM

