

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112124\
 Data File : VW031078.D
 Acq On : 21 Nov 2024 10:38
 Operator : SY/MD
 Sample : P4872-13
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 22 00:08:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112024SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 22 00:06:47 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.837	114	403371	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	374203	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	171458	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.363	65	132451	26.935	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.760%	
7) Chloroethane-d5		2.899	69	101643	26.189	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.760%	
11) 1,1-Dichloroethene-d2		4.015	65	60693	24.979	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	99.920%	
21) 2-Butanone-d5		7.075	46	52560	46.422	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.840%	
24) Chloroform-d		7.648	84	273814	24.989	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.960%	
26) 1,2-Dichloroethane-d4		8.301	65	138498	25.870	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.480%	
32) Benzene-d6		8.276	84	544774	25.707	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.840%	
36) 1,2-Dichloropropane-d6		9.270	67	163947	26.237	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.960%	
41) Toluene-d8		10.319	98	501079	25.955	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.800%	
43) trans-1,3-Dichloroprop...		10.575	79	63791	24.522	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.080%	
47) 2-Hexanone-d5		10.922	63	41001	45.655	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.320%	
56) 1,1,2,2-Tetrachloroeth...		12.690	84	117719	24.735	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.920%	
66) 1,2-Dichlorobenzene-d4		13.848	152	163981	27.365	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.440%	
Target Compounds							
39) cis-1,3-Dichloropropene		10.032	75	4240	0.471	ug/L	Qvalue # 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112124\
Data File : VW031078.D
Acq On : 21 Nov 2024 10:38
Operator : SY/MD
Sample : P4872-13
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 22 00:08:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112024SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 22 00:06:47 2024
Response via : Initial Calibration

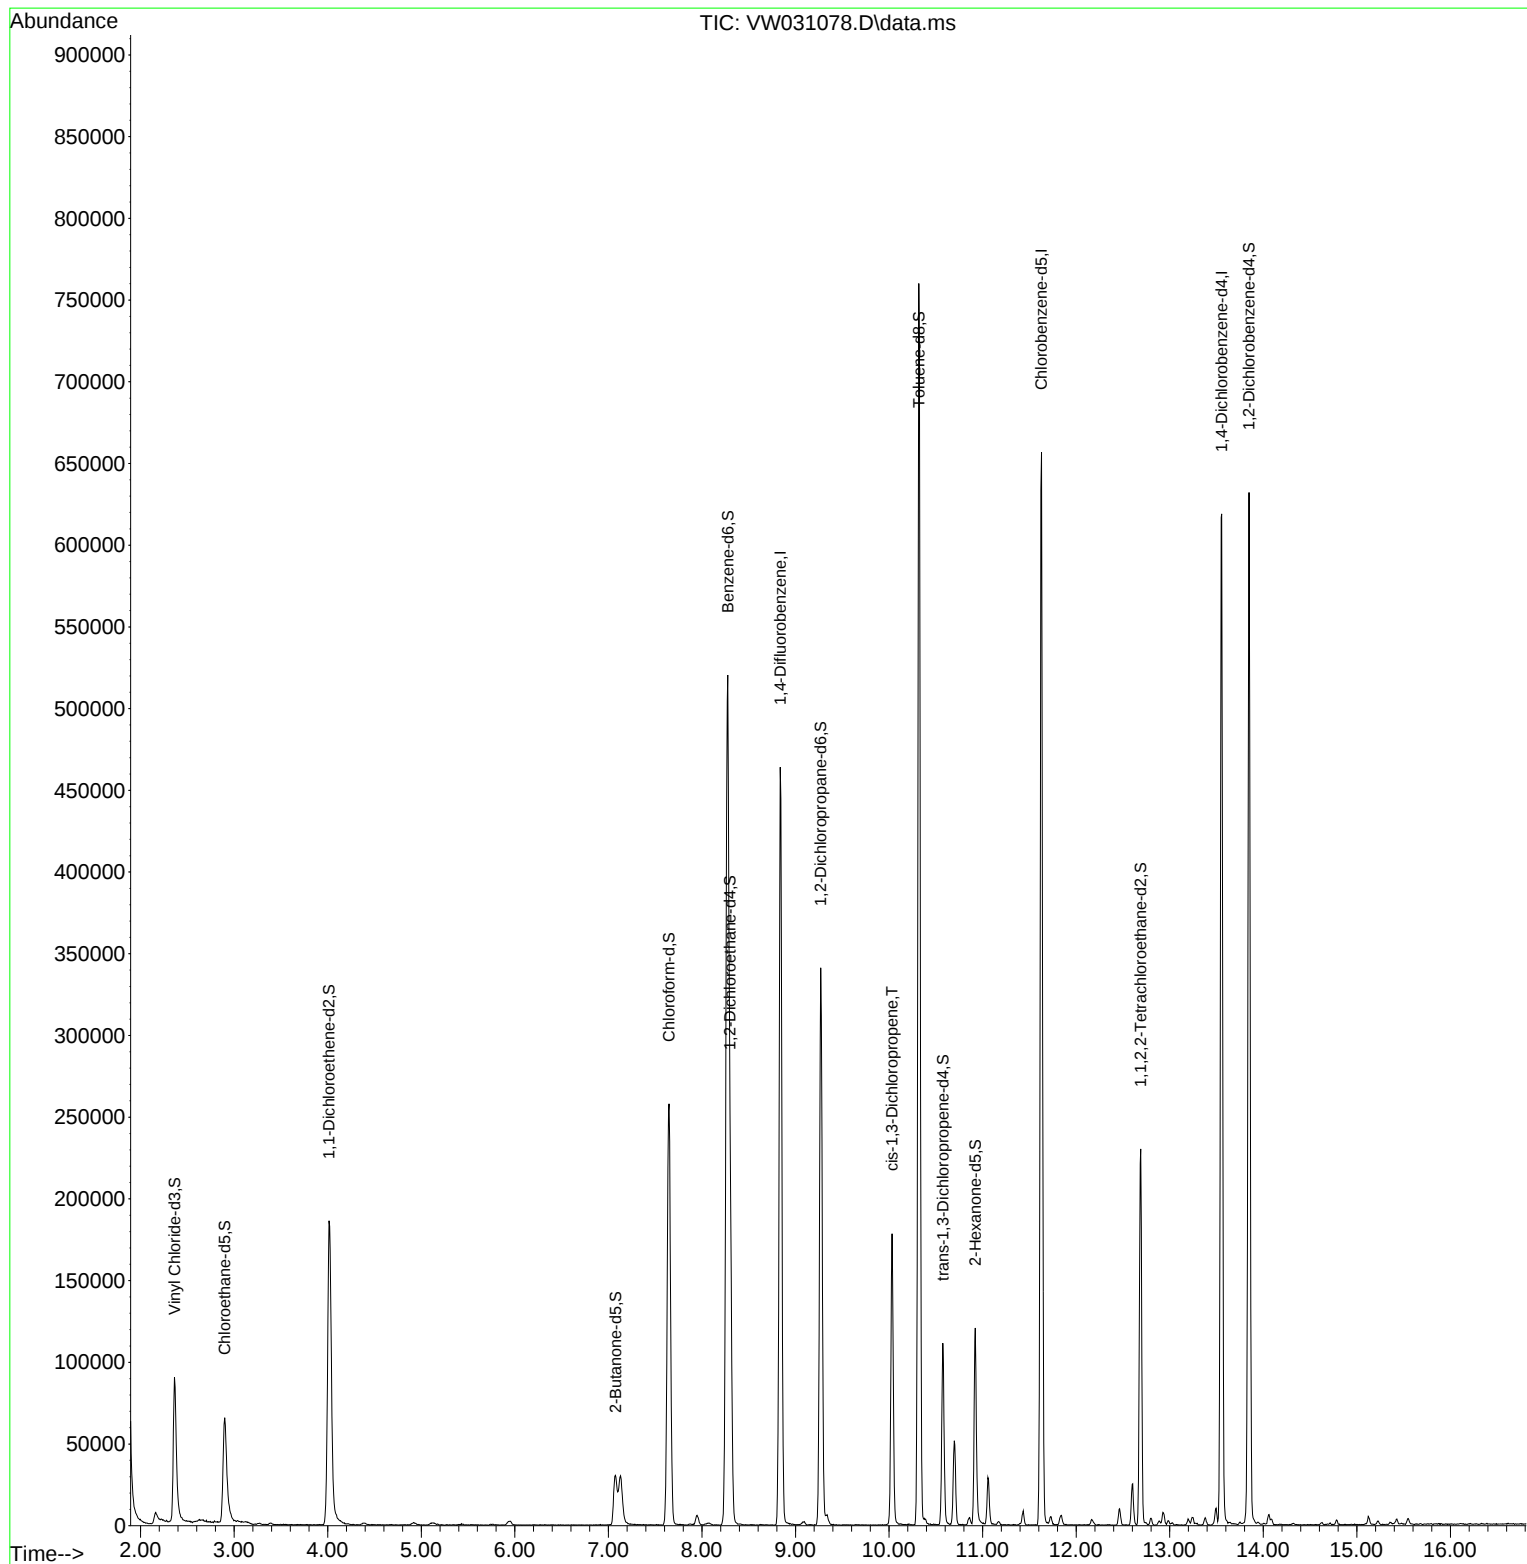

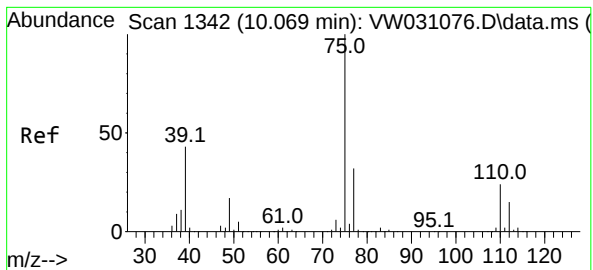

#39
cis-1,3-Dichloropropene
Concen: 0.471 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.037 min
Lab File: VW031078.D
Acq: 21 Nov 2024 10:38

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 4240
Ion Ratio Lower Upper
75 100
77 54.1 21.6 40.2#

