
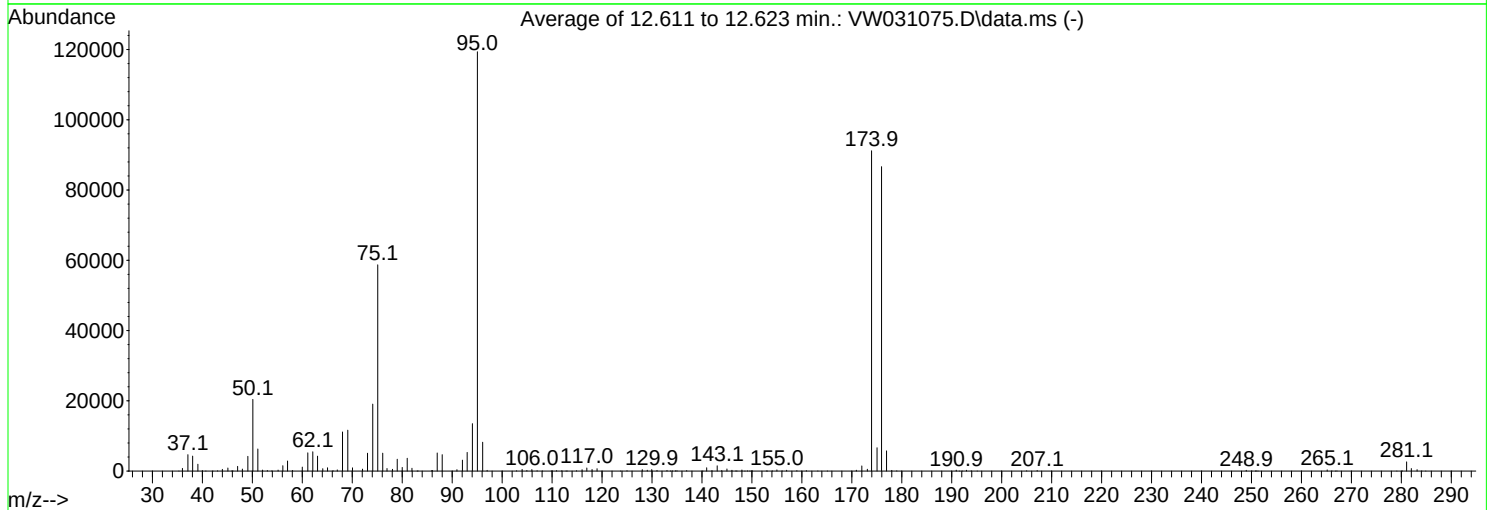


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112124\
Data File : VW031075.D
Acq On : 21 Nov 2024 08:00
Operator : SY/MD
Sample : BFB403
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB403

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112024SMA.M
Title : SFAM01.0
Last Update : Fri Nov 22 22:09:34 2024

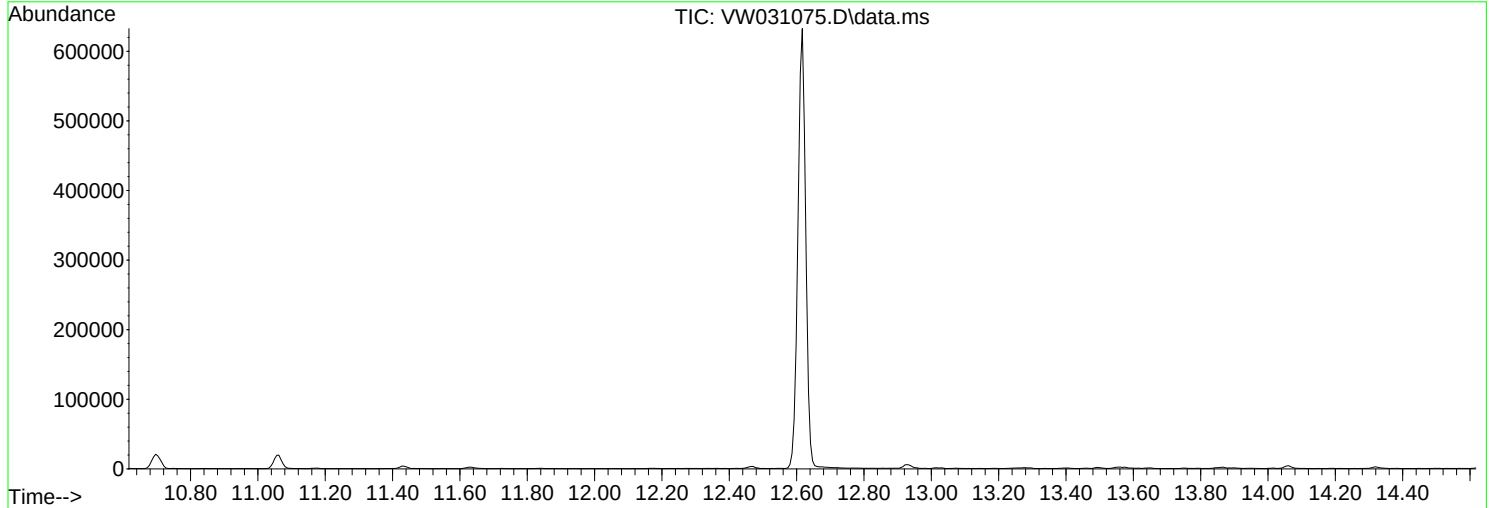

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	20405	PASS
75	95	30	80	49.2	58715	PASS
95	95	100	100	100.0	119371	PASS
96	95	5	9	6.9	8212	PASS
173	174	0.00	2	0.6	527	PASS
174	95	50	120	76.4	91187	PASS
175	174	5	9	7.3	6637	PASS
176	174	95	101	95.0	86659	PASS
177	176	5	9	6.6	5752	PASS

m/z	Abundance
35.90	211.0
37.80	75.0
40.00	183.0
43.90	180.0

Instrument :
MSVOA_W
ClientSampleId :
BFB403

m/z	Abundance
35.30	59.0
36.10	1137.0
37.10	4945.0
38.00	4414.0
39.10	2140.0
40.00	358.0
42.10	53.0
43.10	120.0
44.10	687.0
45.10	1079.0
45.90	150.0
47.10	1399.0
48.00	600.0
49.10	4298.0
50.10	21440.0
51.10	6598.0
52.00	377.0
53.00	181.0
53.90	57.0
55.20	268.0
56.10	1608.0
57.00	2922.0
58.10	188.0
60.00	1128.0
61.10	5246.0
62.10	6064.0
63.10	4503.0
64.10	770.0
65.10	1160.0
66.20	125.0
67.00	366.0
68.00	11591.0
69.10	12151.0
70.10	917.0
72.10	641.0
73.00	5566.0
74.10	20224.0
75.10	60952.0
76.10	5589.0
77.00	751.0
78.00	466.0
79.00	3475.0
80.00	1072.0
81.00	4190.0
82.00	839.0
83.00	99.0
85.90	362.0
87.00	5387.0
88.00	4563.0
91.00	401.0
92.10	3257.0
93.00	5493.0
94.10	14363.0
95.10	122560.0
96.10	8519.0
97.00	243.0
102.90	106.0
104.00	520.0
104.90	232.0
105.90	505.0
107.00	110.0
108.10	58.0
110.10	102.0
110.90	175.0
112.00	95.0
112.80	82.0
114.90	132.0
116.10	425.0
117.00	1004.0
118.00	570.0
119.00	881.0
125.00	229.0
128.00	492.0
129.00	230.0
130.00	361.0
131.10	185.0
133.10	340.0
133.70	138.0
134.10	112.0
135.00	134.0
137.00	159.0
140.90	856.0
142.10	184.0
143.10	1685.0
144.00	133.0
145.00	772.0
146.00	295.0
146.80	101.0
148.00	349.0
149.20	82.0
149.90	124.0
152.90	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB403

154.10	69.0
155.00	340.0
157.00	217.0
159.00	110.0
163.20	63.0
165.10	107.0
170.80	183.0
172.00	1449.0
173.10	1582.0
173.90	78112.0
175.00	5830.0
176.00	83728.0
177.00	5812.0
178.00	213.0
179.00	116.0
190.90	373.0
192.20	64.0
192.90	427.0
193.90	165.0
195.10	88.0
205.00	166.0
207.10	192.0
248.90	304.0
250.10	58.0
250.80	78.0
251.30	91.0
265.10	642.0
266.10	111.0
267.10	163.0
279.10	53.0
280.20	123.0
281.00	4218.0
282.00	1038.0
283.20	662.0
284.10	97.0
284.90	51.0

Instrument :
MSVOA_W
ClientSampleId :
BFB403

m/z	Abundance
36.00	1047.0
37.10	5181.0
38.10	4893.0
39.10	2198.0
40.00	228.0
43.00	112.0
44.00	786.0
45.10	950.0
46.10	160.0
47.00	1407.0
47.90	617.0
49.10	4957.0
50.10	22600.0
51.10	7180.0
52.10	298.0
53.10	202.0
53.90	58.0
55.10	380.0
56.10	1651.0
57.10	3314.0
58.00	189.0
60.00	1333.0
61.10	5794.0
62.10	5882.0
63.10	4874.0
64.10	811.0
65.00	1011.0
66.10	123.0
67.00	455.0
68.00	12471.0
69.10	13567.0
70.00	1106.0
72.00	673.0
73.10	5873.0
74.10	21232.0
75.10	66480.0
76.10	5582.0
76.90	780.0
78.10	554.0
79.00	3739.0
80.00	1162.0
81.00	3797.0
82.00	930.0
83.20	89.0
86.10	290.0
87.00	5420.0
88.00	5087.0
90.90	499.0
92.00	3439.0
93.00	5923.0
94.00	15035.0
95.10	132480.0
96.10	8919.0
97.00	263.0
102.90	137.0
104.00	505.0
105.00	174.0
106.00	519.0
107.00	120.0
109.80	55.0
110.90	113.0
112.00	108.0
113.00	61.0
115.00	115.0
116.00	500.0
116.90	993.0
117.90	495.0
119.00	704.0
123.70	57.0
125.00	97.0
128.00	429.0
129.10	324.0
130.00	524.0
130.90	298.0
132.90	243.0
134.70	237.0
136.90	133.0
141.00	1178.0
141.90	194.0
143.00	1811.0
144.00	131.0
145.00	594.0
145.90	237.0
147.00	126.0
147.90	309.0
148.60	53.0
149.10	62.0
149.60	105.0
150.10	65.0
152.90	118.0
154.10	66.0
155.00	304.0

Instrument :
MSVOA_W
ClientSampleId :
BFB403

156.00	118.0
157.00	264.0
159.00	120.0
160.90	228.0
163.20	56.0
170.90	307.0
172.00	1702.0
174.00	106736.0
175.10	7105.0
175.90	98392.0
176.90	5516.0
177.90	196.0
179.00	117.0
190.90	335.0
193.00	209.0
205.00	112.0
207.10	330.0
249.00	253.0
251.00	161.0
265.20	287.0
266.80	60.0
281.10	2524.0
282.00	700.0
283.10	390.0

Instrument :
MSVOA_W
ClientSampleId :
BFB403

m/z	Abundance
36.00	763.0
37.10	3911.0
38.10	3475.0
39.10	1544.0
40.10	240.0
40.70	101.0
44.00	560.0
45.10	619.0
46.10	107.0
47.00	1234.0
48.10	533.0
49.10	3350.0
50.10	17176.0
51.10	5101.0
52.10	177.0
52.90	121.0
55.10	232.0
56.10	1340.0
57.00	2359.0
58.10	132.0
60.00	922.0
61.10	4532.0
62.10	4517.0
63.00	3374.0
64.00	489.0
65.00	649.0
66.20	59.0
67.00	194.0
68.10	9361.0
69.10	9210.0
70.00	769.0
72.10	388.0
73.00	3820.0
74.10	15744.0
75.10	48712.0
76.10	4112.0
76.90	692.0
78.00	520.0
79.00	2914.0
80.00	890.0
81.00	2970.0
81.90	676.0
83.10	86.0
86.00	186.0
87.00	4643.0
88.00	4384.0
90.90	335.0
92.10	2661.0
93.00	4536.0
94.10	11106.0
95.00	103072.0
96.10	7197.0
97.00	94.0
102.90	67.0
104.00	437.0
104.90	129.0
106.00	317.0
107.00	108.0
109.90	77.0
110.80	91.0
111.80	58.0
113.00	70.0
114.80	106.0
115.90	256.0
117.00	619.0
118.10	283.0
119.00	481.0
125.00	57.0
128.10	312.0
129.00	201.0
129.90	424.0
131.00	96.0
135.00	186.0
136.90	171.0
140.20	65.0
141.00	809.0
143.10	1026.0
143.90	108.0
144.90	426.0
146.10	154.0
146.80	72.0
148.10	270.0
149.00	66.0
150.10	96.0
153.10	71.0
155.00	366.0
156.10	67.0
156.90	227.0
159.00	186.0
160.90	165.0
171.00	235.0
172.00	1242.0

Instrument :
MSVOA_W
ClientSampleId :
BFB403

174.00	88712.0
175.00	6977.0
176.00	77856.0
177.00	5927.0
178.10	175.0
190.80	94.0
191.60	56.0
193.10	79.0
249.10	102.0
250.90	55.0
265.20	106.0
281.20	1130.0
281.90	421.0
283.10	172.0

Instrument :
MSVOA_W
ClientSampleId :
BFB403