

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112222\
 Data File : VW025117.D
 Acq On : 22 Nov 2022 12:57
 Operator : SY/VA
 Sample : N5658-07
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Nov 23 04:06:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 23 04:05:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	485608	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	427717	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	192442	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	128629	21.556	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.240%
7) Chloroethane-d5	2.891	69	77919	19.978	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.920%
11) 1,1-Dichloroethene-d2	4.019	63	214087	16.669	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.680%
21) 2-Butanone-d5	7.080	46	58917	47.516	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.040%
24) Chloroform-d	7.653	84	279828	22.330	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.320%
26) 1,2-Dichloroethane-d4	8.305	65	143900	23.251	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.000%
32) Benzene-d6	8.281	84	599805	23.261	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.040%
36) 1,2-Dichloropropane-d6	9.274	67	175047	23.476	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.920%
41) Toluene-d8	10.323	98	547272	23.373	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.480%
43) trans-1,3-Dichloroprop...	10.579	79	68360	22.721	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.880%
47) 2-Hexanone-d5	10.926	63	44935	47.444	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.880%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	113755	22.965	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	155769	23.744	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.960%
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	9.274	63	18969	2.857	ug/L	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112222\
Data File : VW025117.D
Acq On : 22 Nov 2022 12:57
Operator : SY/VA
Sample : N5658-07
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Nov 23 04:06:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 23 04:05:02 2022
Response via : Initial Calibration

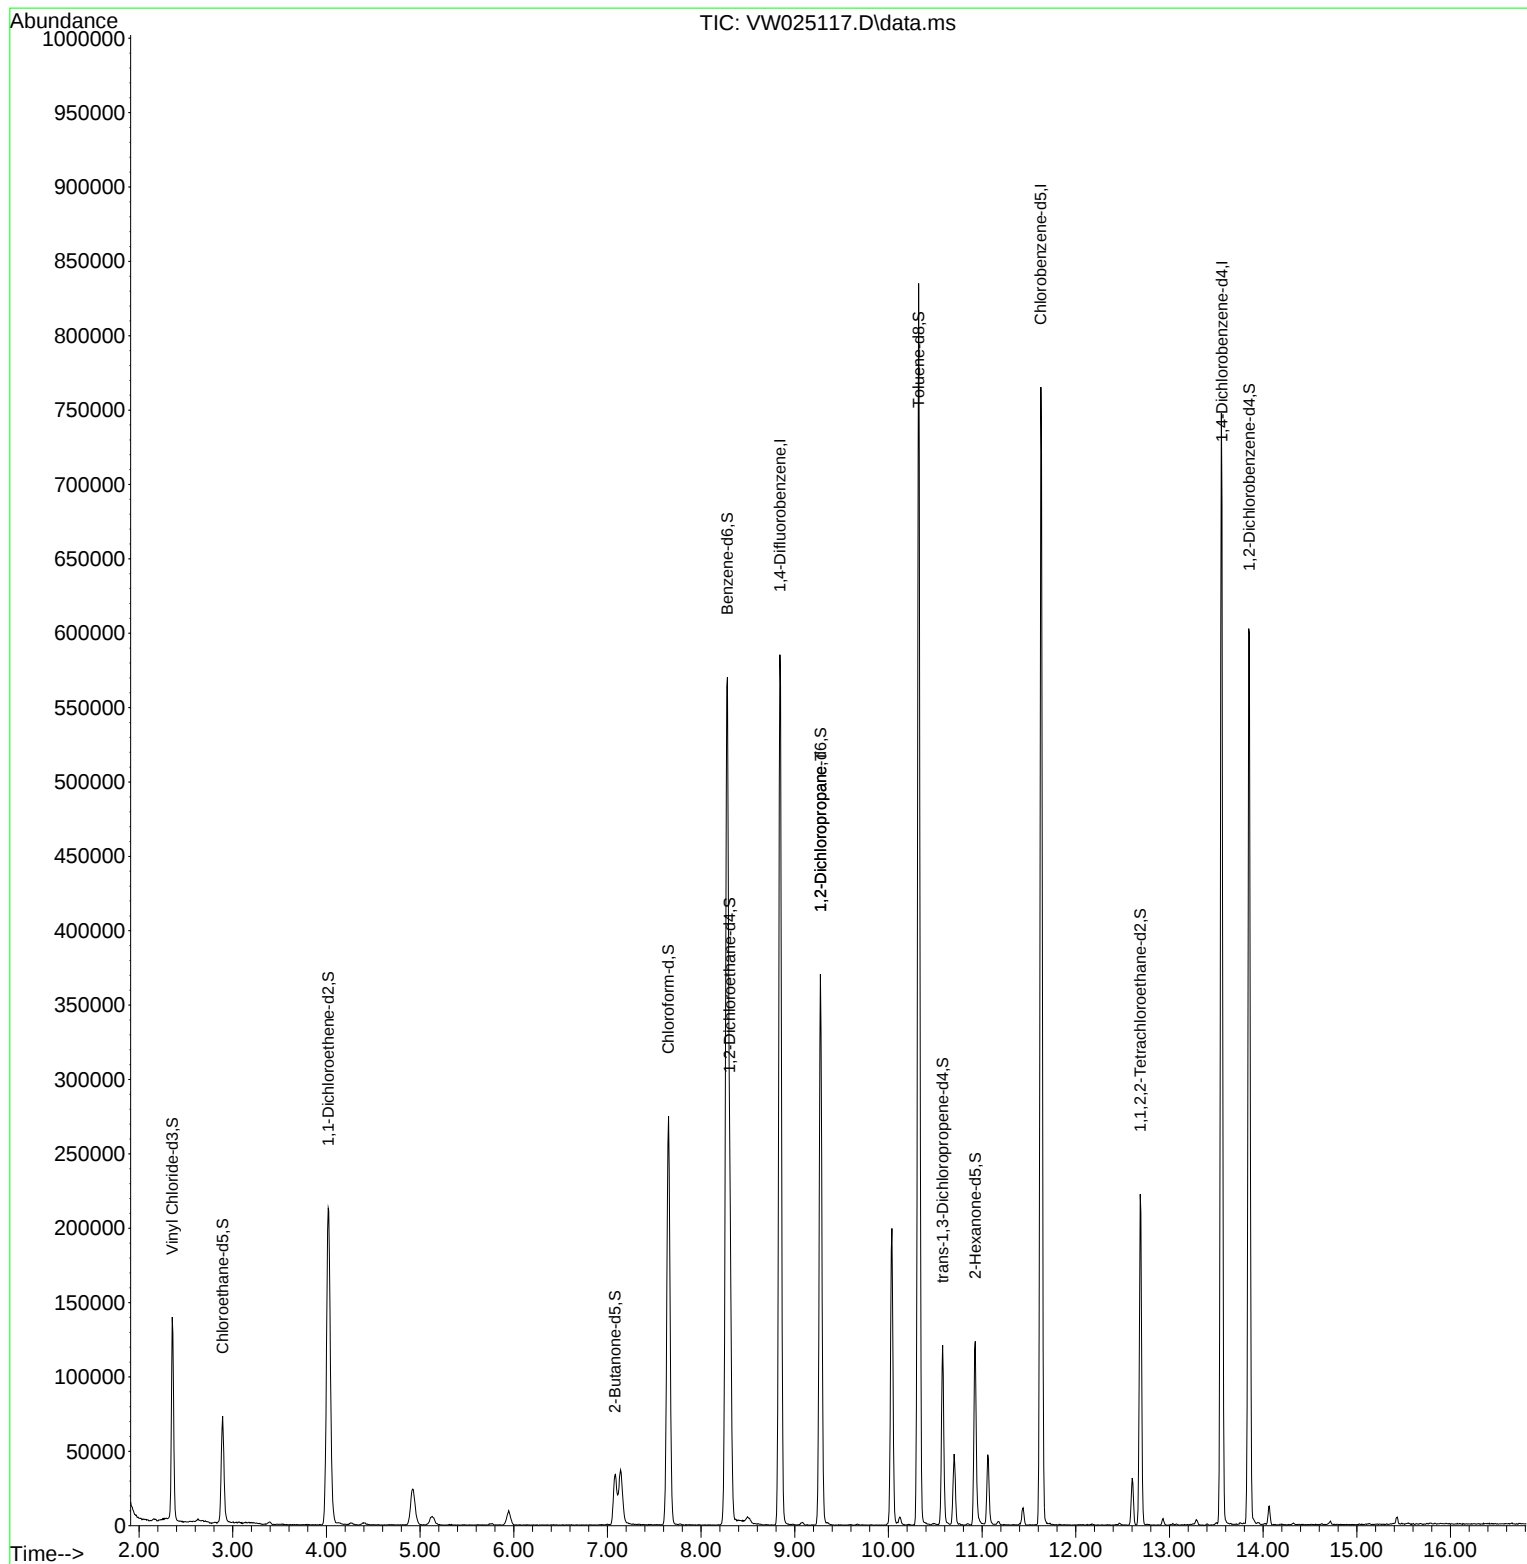

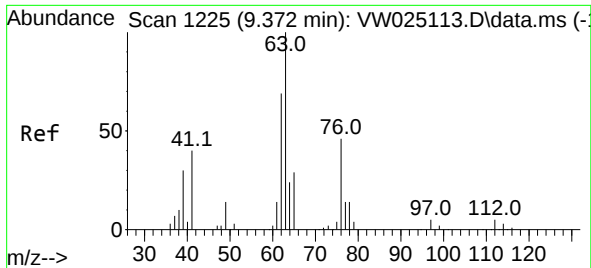

#37

1,2-Dichloropropane

Concen: 2.857 ug/L

RT: 9.274 min Scan# 11

Delta R.T. -0.097 min

Lab File: VW025117.D

Acq: 22 Nov 2022 12:57

Instrument :

MSVOA_W

ClientSampleId :

VHBLK001

Tgt Ion: 63 Resp: 18969

Ion Ratio Lower Upper

63 100

112 0.2 3.4 5.2#

