

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112222\
 Data File : VW025118.D
 Acq On : 22 Nov 2022 13:21
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK591

Quant Time: Nov 23 04:06:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 23 04:05:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	526173	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	467925	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	205820	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	134130	20.745	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.960%		
7) Chloroethane-d5	2.891	69	80065	18.945	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.800%		
11) 1,1-Dichloroethene-d2	4.019	63	222317	15.975	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	63.920%		
21) 2-Butanone-d5	7.080	46	72684	54.100	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	108.200%		
24) Chloroform-d	7.653	84	306991	22.609	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	90.440%		
26) 1,2-Dichloroethane-d4	8.305	65	159897	23.844	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	95.360%		
32) Benzene-d6	8.274	84	648006	22.971	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	91.880%		
36) 1,2-Dichloropropane-d6	9.274	67	190152	23.310	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	93.240%		
41) Toluene-d8	10.323	98	580411	22.658	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	90.640%		
43) trans-1,3-Dichloroprop...	10.579	79	75265	22.866	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	91.480%		
47) 2-Hexanone-d5	10.926	63	56634	54.658	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	109.320%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	132893	24.524	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	98.080%		
66) 1,2-Dichlorobenzene-d4	13.853	152	169122	24.104	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.400%		
Target Compounds					Qvalue	
34) Trichloroethene	8.841	95	16546	2.091	ug/L	# 8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112222\
Data File : VW025118.D
Acq On : 22 Nov 2022 13:21
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK591

Quant Time: Nov 23 04:06:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 23 04:05:02 2022
Response via : Initial Calibration

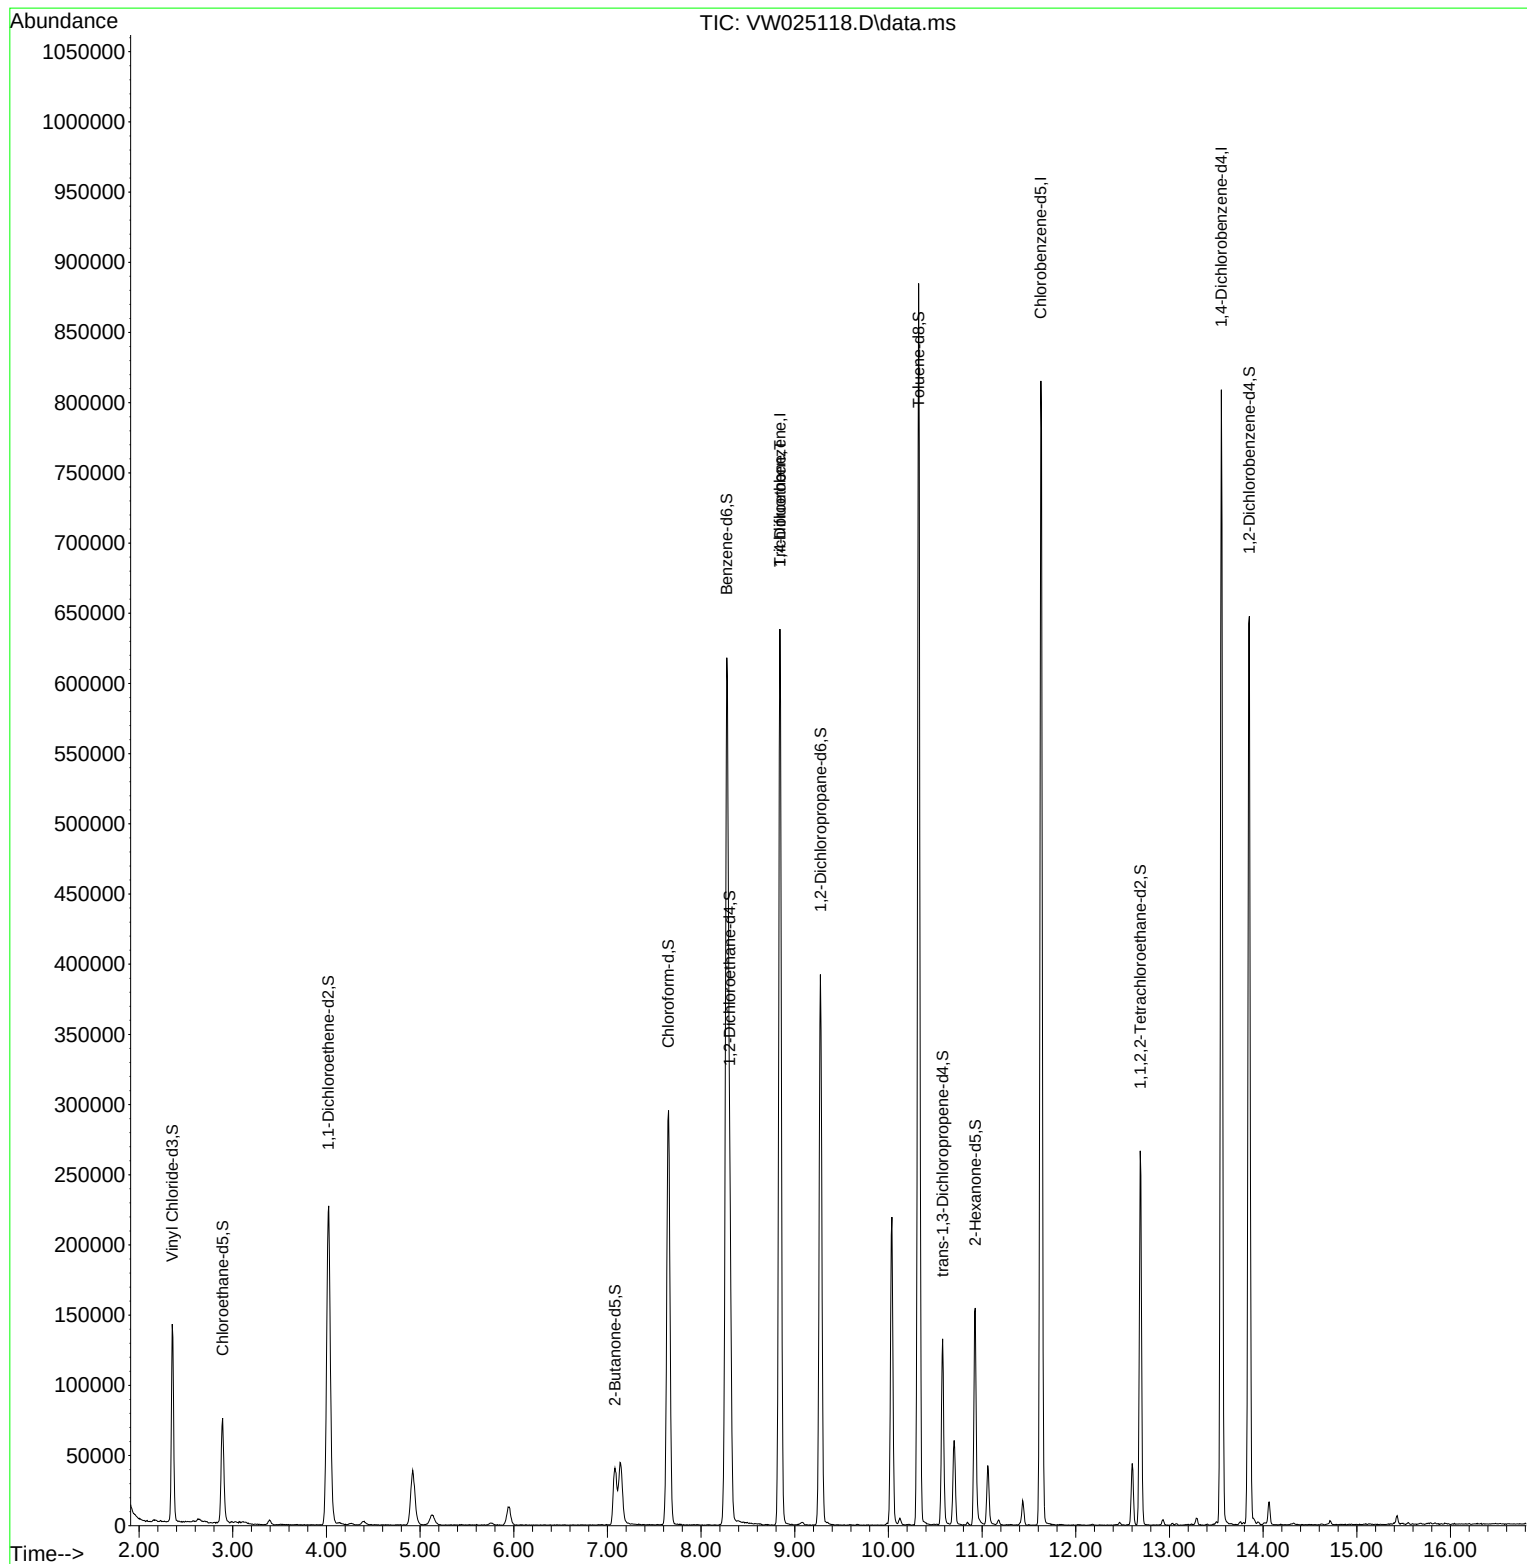

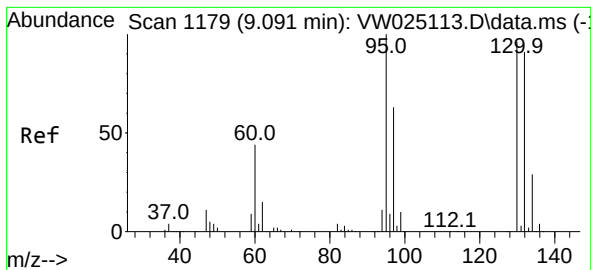

#34

Trichloroethene

Concen: 2.091 ug/L

RT: 8.841 min Scan# 11

Delta R.T. -0.250 min

Lab File: VW025118.D


Acq: 22 Nov 2022 13:21

Instrument :

MSVOA_W

ClientSampleId :

VIBLK591

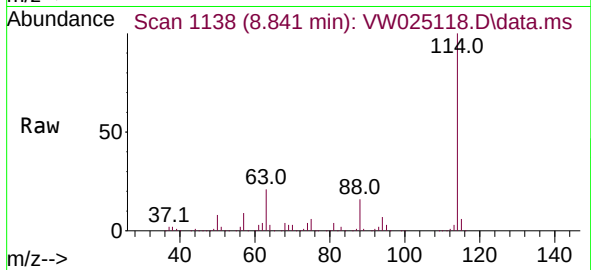

Tgt Ion: 95 Resp: 16546

Ion Ratio Lower Upper

95 100

97 0.0 44.3 82.3#

132 0.0 63.0 117.0#

130 0.0 63.4 117.8#

