

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112224\
 Data File : VW031096.D
 Acq On : 22 Nov 2024 11:27
 Operator : SY/MD
 Sample : P4724-14
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 22 22:10:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112024SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 22 22:09:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	408464	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	393373	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	172449	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	118192	23.736	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.960%
7) Chloroethane-d5	2.899	69	93935	23.901	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.600%
11) 1,1-Dichloroethene-d2	4.021	65	52993	21.538	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.160%
21) 2-Butanone-d5	7.075	46	42766	37.301	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.600%
24) Chloroform-d	7.648	84	242311	21.839	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.360%
26) 1,2-Dichloroethane-d4	8.307	65	123469	22.775	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.120%
32) Benzene-d6	8.276	84	480982	21.591	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.360%
36) 1,2-Dichloropropane-d6	9.270	67	145655	22.174	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.680%
41) Toluene-d8	10.319	98	430761	21.225	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.920%
43) trans-1,3-Dichloroprop...	10.575	79	55928	20.452	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.800%
47) 2-Hexanone-d5	10.922	63	33102	35.063	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.120%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	103076	20.603	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.400%
66) 1,2-Dichlorobenzene-d4	13.849	152	146122	24.245	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.960%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	3782	0.400	ug/L	# 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112224\
Data File : VW031096.D
Acq On : 22 Nov 2024 11:27
Operator : SY/MD
Sample : P4724-14
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 22 22:10:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112024SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 22 22:09:34 2024
Response via : Initial Calibration

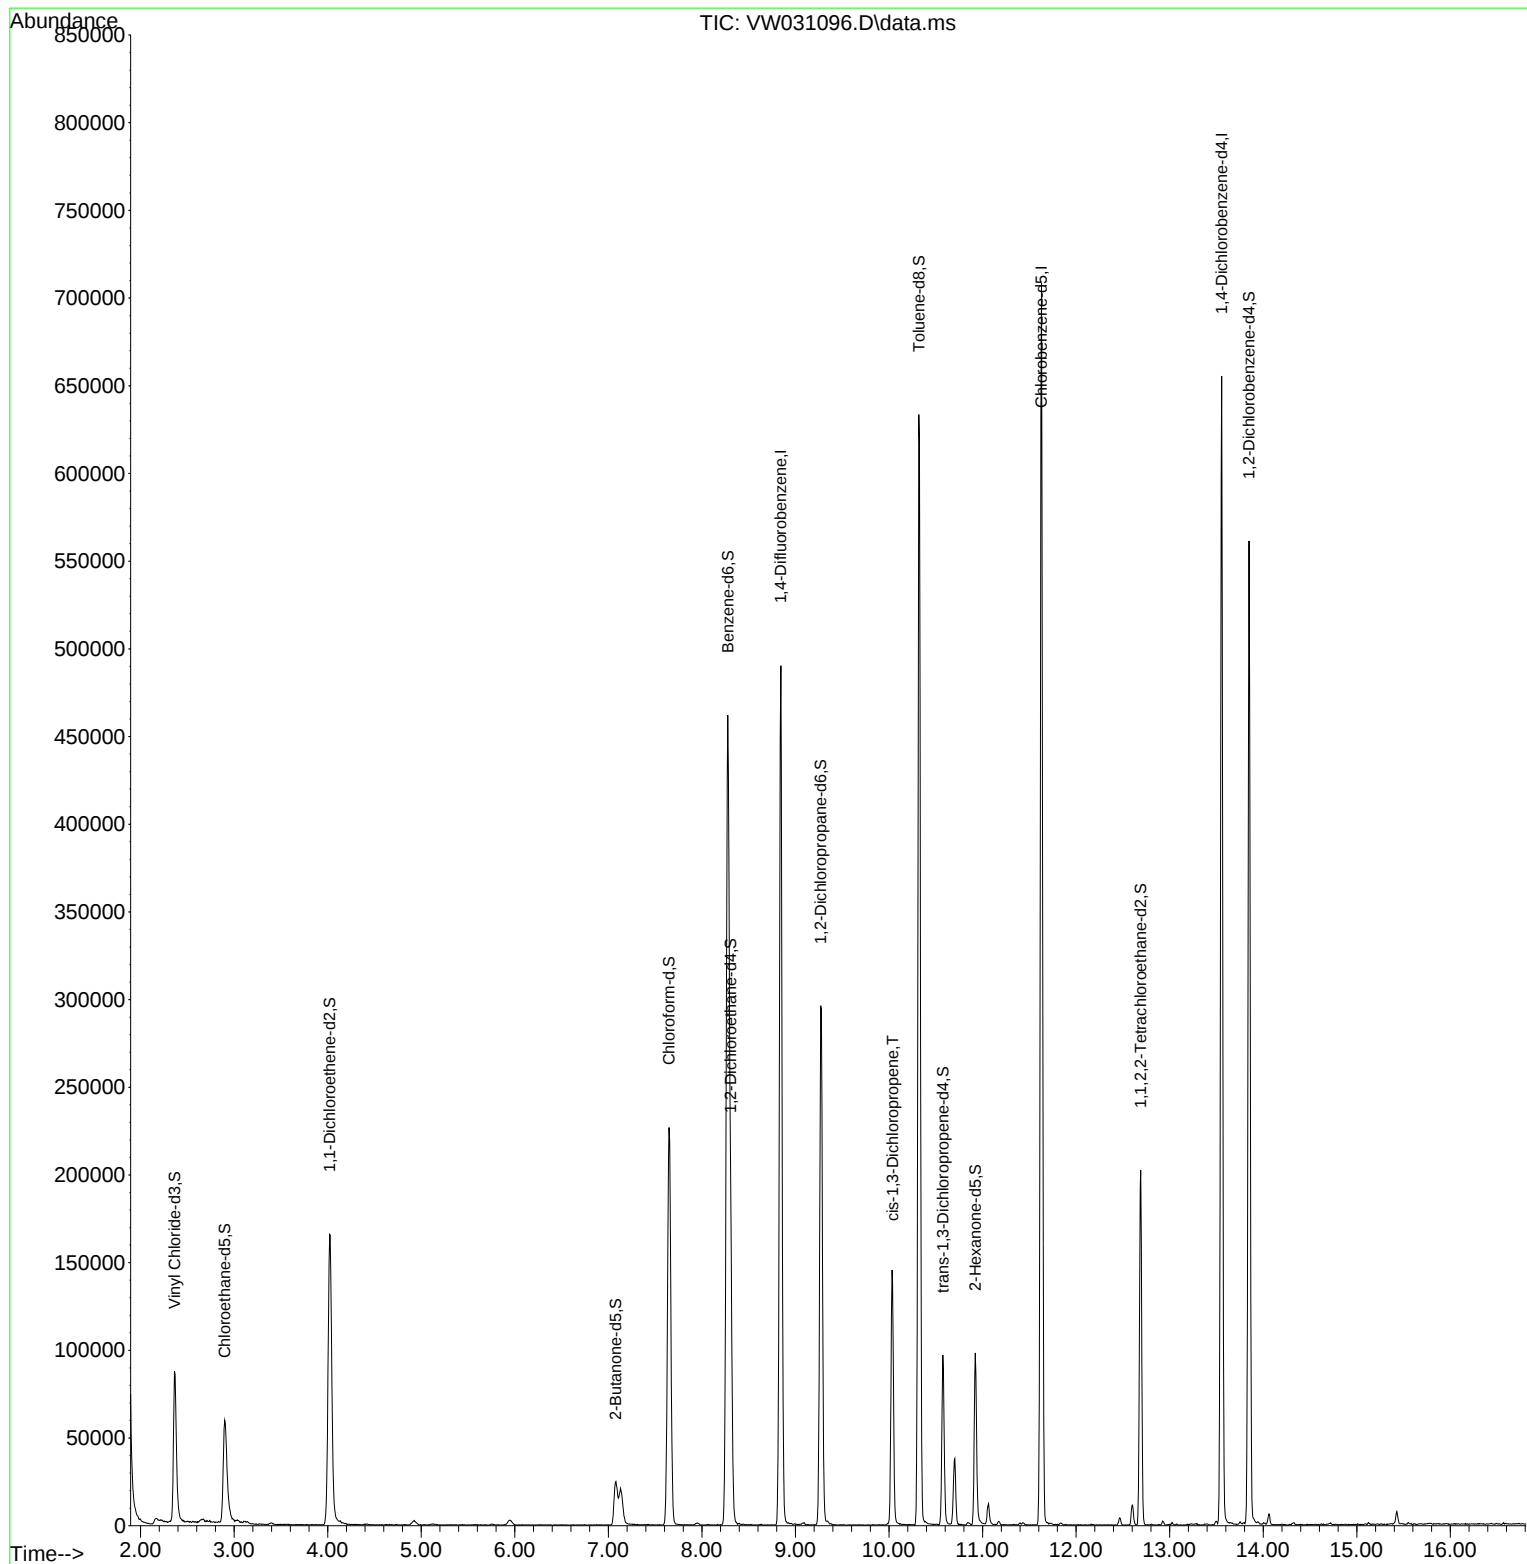

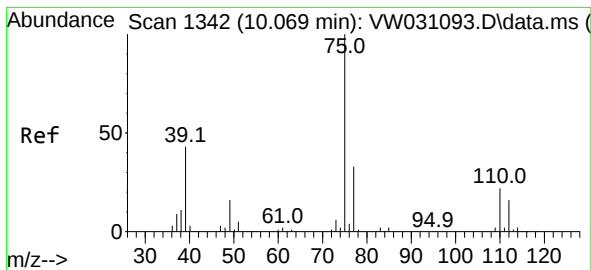

#39
 cis-1,3-Dichloropropene
 Concen: 0.400 ug/L
 RT: 10.038 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW031096.D
 Acq: 22 Nov 2024 11:27

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3782
 Ion Ratio Lower Upper
 75 100
 77 49.5 21.6 40.2#

