
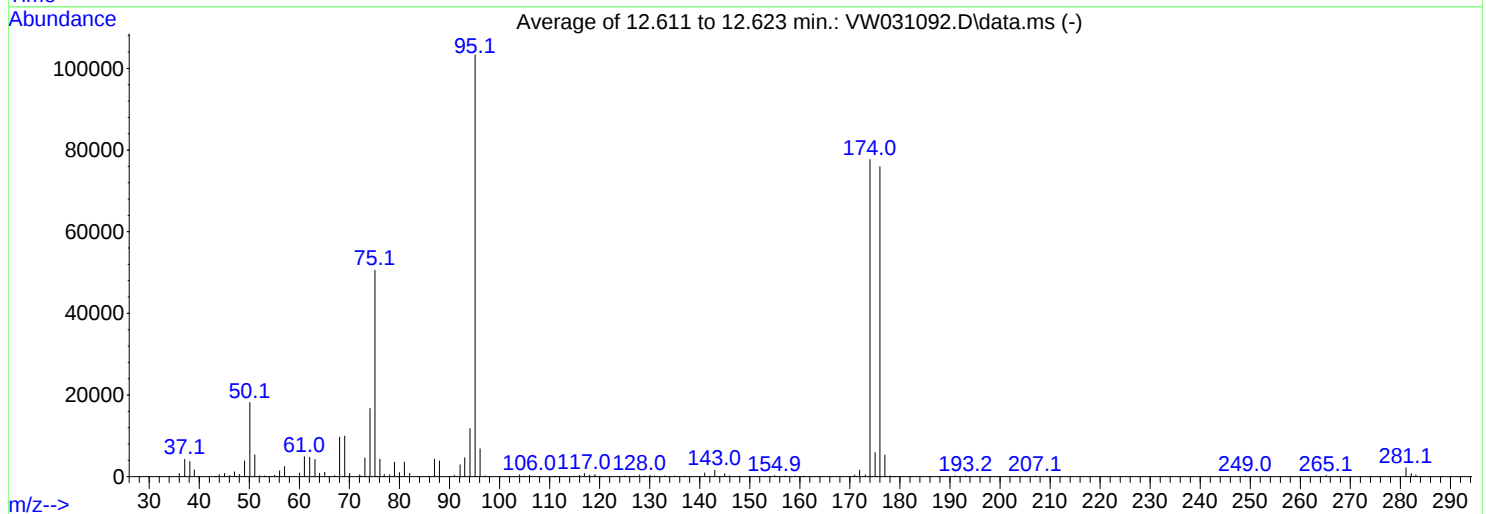


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112224\
Data File : VW031092.D
Acq On : 22 Nov 2024 08:37
Operator : SY/MD
Sample : BFB404
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB404

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112024SMA.M
Title : SFAM01.0
Last Update : Fri Nov 22 22:09:34 2024

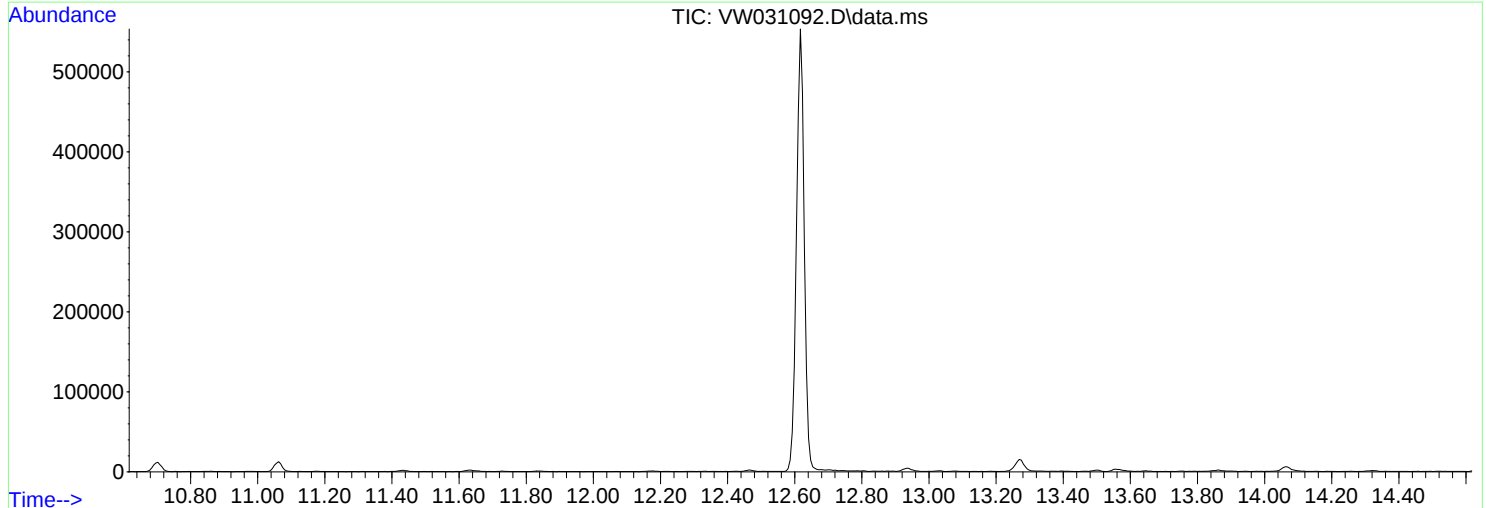

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	18184	PASS
75	95	30	80	48.9	50555	PASS
95	95	100	100	100.0	103325	PASS
96	95	5	9	6.6	6805	PASS
173	174	0.00	2	0.6	448	PASS
174	95	50	120	75.2	77664	PASS
175	174	5	9	7.6	5867	PASS
176	174	95	101	97.8	75923	PASS
177	176	5	9	7.0	5284	PASS

Scan 1751 (12.562 min): VW031092.D\data.ms
BFB404

m/z	Abundance
36.00	144.0
40.00	208.0
44.00	202.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

m/z	Abundance
36.10	963.0
37.10	4409.0
38.10	3890.0
39.00	1698.0
40.10	261.0
44.10	713.0
45.00	725.0
46.10	326.0
47.10	1145.0
48.00	537.0
49.10	3899.0
50.10	18080.0
51.10	5081.0
52.10	223.0
53.00	199.0
53.90	106.0
55.00	384.0
56.10	1280.0
57.00	2273.0
58.10	138.0
59.00	81.0
60.00	772.0
61.00	4738.0
62.10	4721.0
63.10	3796.0
64.00	915.0
65.10	1133.0
66.10	142.0
67.10	264.0
68.00	9470.0
69.00	9542.0
70.10	793.0
72.00	679.0
73.10	4603.0
74.10	16132.0
75.10	48432.0
76.10	3985.0
76.90	447.0
78.00	577.0
79.00	3589.0
80.00	886.0
81.00	3739.0
82.00	841.0
86.00	200.0
87.00	4158.0
88.00	3603.0
90.90	400.0
92.10	2721.0
93.10	4493.0
94.10	11325.0
95.10	92120.0
96.10	6111.0
97.00	248.0
102.90	116.0
104.00	489.0
105.00	182.0
106.00	368.0
107.00	107.0
108.20	56.0
111.20	95.0
112.20	62.0
114.90	98.0
116.00	254.0
116.90	683.0
118.10	420.0
118.90	618.0
123.80	78.0
124.90	247.0
127.00	82.0
128.00	368.0
129.10	123.0
130.00	321.0
130.90	155.0
133.10	335.0
133.80	150.0
135.00	139.0
137.10	135.0
139.90	88.0
141.00	748.0
142.10	170.0
143.00	1676.0
143.90	96.0
145.00	793.0
145.90	159.0
146.90	124.0
148.00	168.0
149.90	137.0
154.90	291.0
156.20	70.0
156.80	87.0
157.10	90.0
159.00	123.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

161.00	137.0
163.00	79.0
171.00	361.0
171.90	1535.0
173.10	1344.0
174.00	60296.0
175.10	5721.0
176.00	64040.0
177.00	4522.0
178.00	194.0
191.00	353.0
192.10	118.0
193.20	347.0
202.80	74.0
205.10	91.0
207.10	184.0
249.10	278.0
250.00	85.0
251.10	137.0
265.20	533.0
266.00	78.0
267.20	145.0
281.20	3617.0
282.20	1180.0
283.20	576.0
284.20	183.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

m/z	Abundance
36.00	1086.0
37.10	4617.0
38.10	3967.0
39.00	1826.0
40.00	277.0
43.10	51.0
44.00	787.0
45.10	952.0
46.10	340.0
47.00	1330.0
48.10	602.0
49.10	3962.0
50.10	20416.0
51.10	6150.0
52.10	299.0
53.10	227.0
53.90	138.0
55.10	360.0
56.00	1716.0
57.10	2609.0
58.00	140.0
59.10	88.0
60.10	1109.0
61.00	5463.0
62.00	5492.0
63.10	4843.0
64.10	921.0
65.00	977.0
67.10	287.0
68.10	10530.0
69.10	11345.0
70.00	855.0
72.10	624.0
73.10	5420.0
74.10	18744.0
75.10	56752.0
76.10	5107.0
77.00	677.0
78.00	463.0
79.00	3913.0
80.00	1244.0
81.00	3779.0
82.10	889.0
85.90	214.0
87.00	4714.0
88.00	4226.0
91.00	421.0
92.10	3317.0
93.10	5196.0
94.10	12640.0
95.10	116776.0
96.10	8078.0
97.10	224.0
103.10	100.0
104.00	348.0
105.00	213.0
106.00	347.0
106.80	64.0
108.20	76.0
110.00	124.0
110.70	75.0
111.10	69.0
111.80	64.0
112.90	98.0
114.90	112.0
115.80	381.0
117.00	947.0
118.00	496.0
119.10	728.0
120.10	59.0
123.80	55.0
125.00	130.0
127.00	177.0
127.90	437.0
129.00	136.0
130.00	361.0
131.00	139.0
132.90	207.0
133.80	57.0
135.00	152.0
137.00	139.0
140.20	167.0
141.00	1124.0
142.00	138.0
143.00	1800.0
145.00	745.0
145.90	248.0
146.90	73.0
147.80	195.0
149.00	82.0
149.90	141.0
153.10	100.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

155.00	348.0
156.20	69.0
157.00	222.0
159.00	187.0
160.80	122.0
162.90	51.0
170.90	383.0
172.00	1799.0
174.00	87328.0
175.00	6085.0
176.00	88120.0
177.00	6272.0
178.10	172.0
178.80	57.0
191.00	222.0
192.10	87.0
193.10	235.0
205.20	93.0
207.00	148.0
249.00	126.0
251.00	68.0
265.20	216.0
266.10	83.0
267.20	73.0
281.10	1768.0
282.20	572.0
283.00	413.0
284.30	84.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

m/z	Abundance
36.00	736.0
37.10	3716.0
38.10	3257.0
39.00	1439.0
39.90	301.0
44.00	624.0
45.10	697.0
46.10	127.0
47.10	1061.0
48.00	567.0
49.00	3700.0
50.10	16057.0
51.10	4817.0
52.10	206.0
53.00	149.0
54.10	73.0
55.00	250.0
56.00	1230.0
57.10	2496.0
60.10	817.0
61.00	4556.0
62.10	4020.0
63.10	4094.0
64.10	617.0
65.10	1095.0
66.00	94.0
67.00	328.0
68.00	8995.0
69.10	8946.0
70.00	805.0
72.30	473.0
73.10	3735.0
74.10	15214.0
75.10	46480.0
76.10	3786.0
77.00	480.0
78.10	405.0
79.00	3035.0
80.00	788.0
81.00	3197.0
82.00	776.0
87.00	3992.0
88.00	3756.0
91.00	303.0
92.10	2653.0
93.00	4149.0
94.10	11304.0
95.10	101080.0
96.10	6225.0
97.00	176.0
103.00	59.0
104.00	452.0
104.90	141.0
106.00	336.0
106.90	123.0
110.90	57.0
111.20	53.0
112.10	73.0
112.80	91.0
114.90	166.0
116.00	263.0
117.00	692.0
117.90	279.0
119.00	813.0
123.80	93.0
125.00	72.0
126.90	83.0
128.00	373.0
128.90	193.0
130.10	280.0
130.90	220.0
132.90	68.0
135.00	245.0
136.90	120.0
141.00	799.0
143.00	1274.0
143.80	77.0
144.20	96.0
145.00	562.0
145.90	175.0
146.90	62.0
148.10	290.0
149.00	71.0
149.70	119.0
153.10	83.0
154.00	64.0
155.00	246.0
156.10	72.0
157.10	163.0
159.10	119.0
160.90	104.0
170.90	398.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404

172.00	1380.0
174.00	85368.0
175.00	5796.0
176.00	75608.0
177.00	5059.0
178.10	173.0
190.90	65.0
193.20	70.0
207.10	107.0
248.90	96.0
265.00	171.0
281.00	1142.0
282.00	434.0
282.60	88.0
283.20	279.0

Instrument :
MSVOA_W
ClientSampleId :
BFB404