

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112520\
Data File : VW017494.D
Acq On : 25 Nov 2020 11:25
Operator : SY/VA
Sample : VW1125SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK11

Manual Integrations
APPROVED

MMDadoda
11/27/2020 1:20:14 PM

Quant Time: Nov 26 07:24:11 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 26 07:23:09 2020
Response via : Initial Calibration

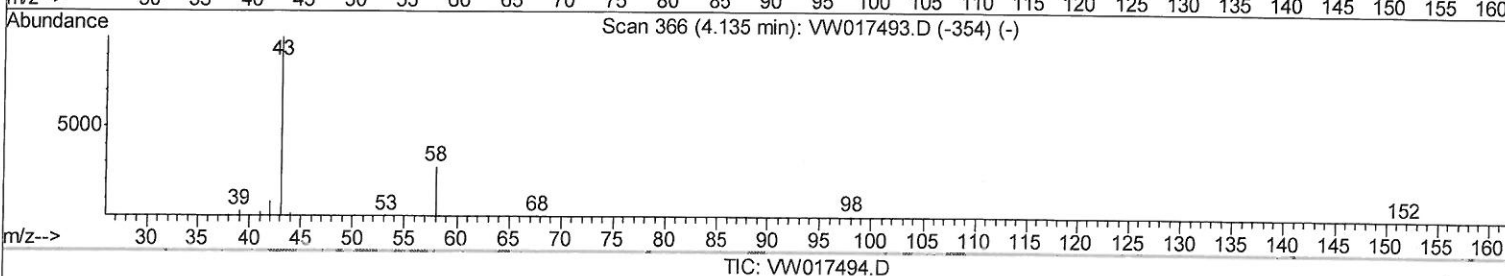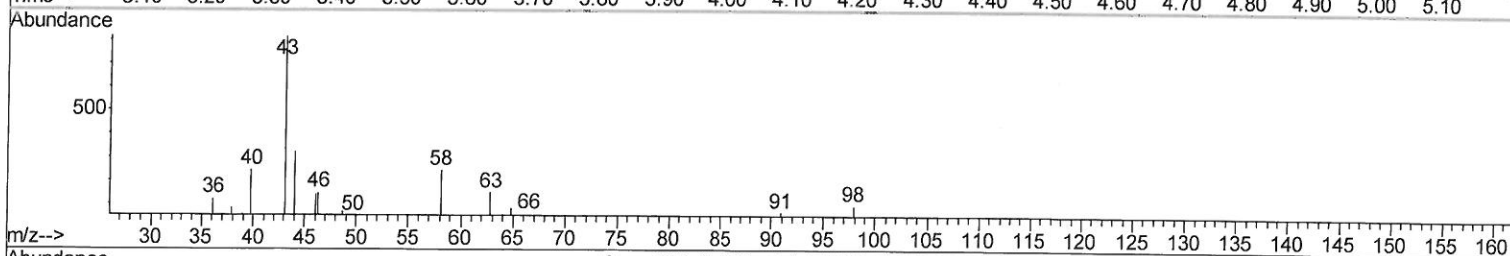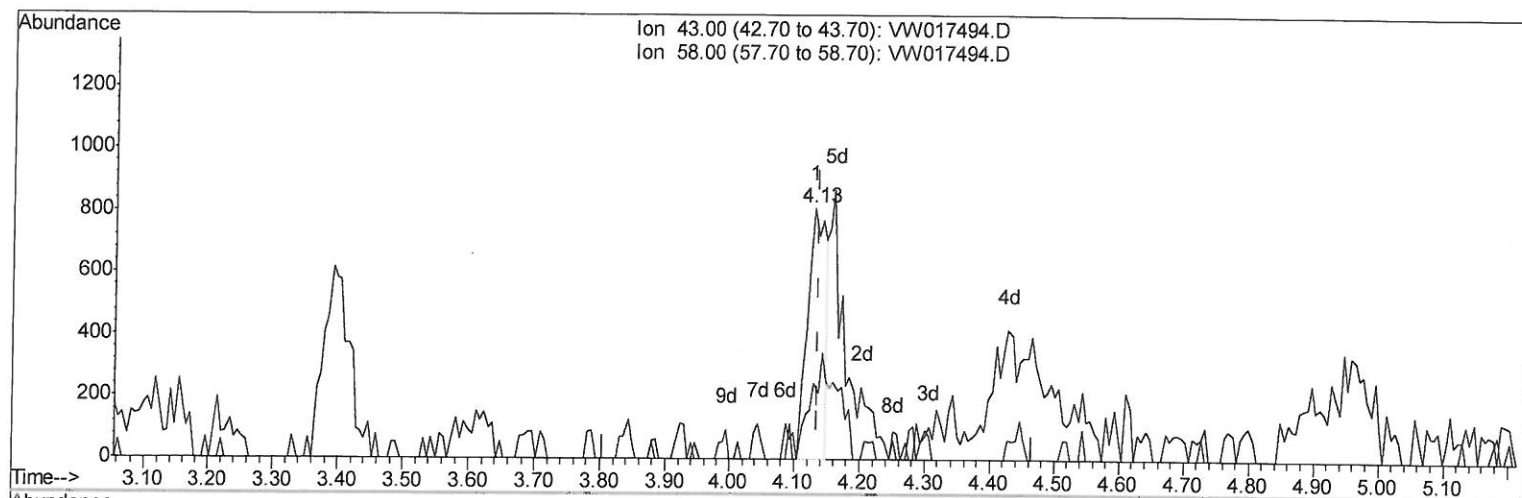

(13) Acetone (T)

4.129min (-0.006) 1.32ug/L

response 1582

Ion	Exp%	Act%
43.00	100	100
58.00	34.20	39.19
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112520\
Data File : VW017494.D
Acq On : 25 Nov 2020 11:25
Operator : SY/VA
Sample : VW1125SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK11

Manual Integrations
APPROVED

MMDadoda
11/27/2020 1:20:14 PM

Quant Time: Nov 26 07:24:11 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 26 07:23:09 2020
Response via : Initial Calibration

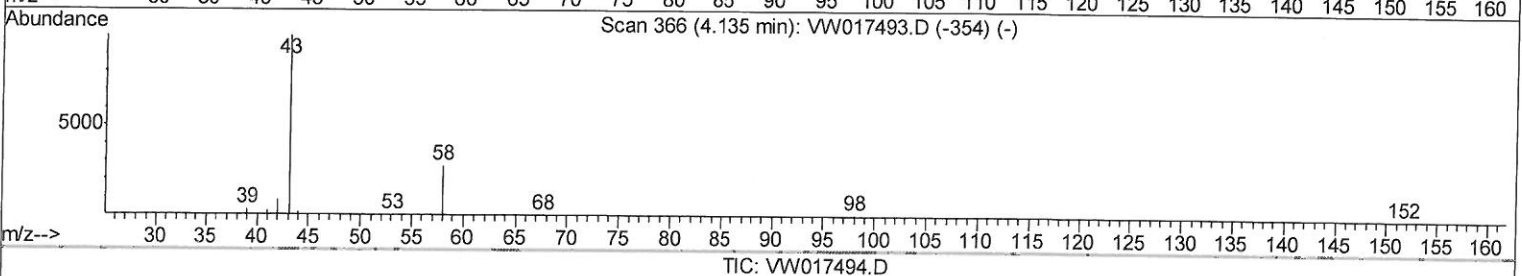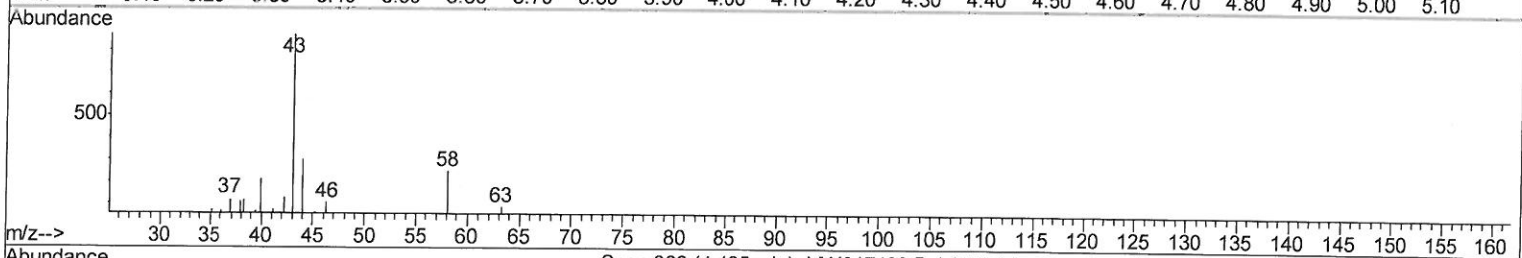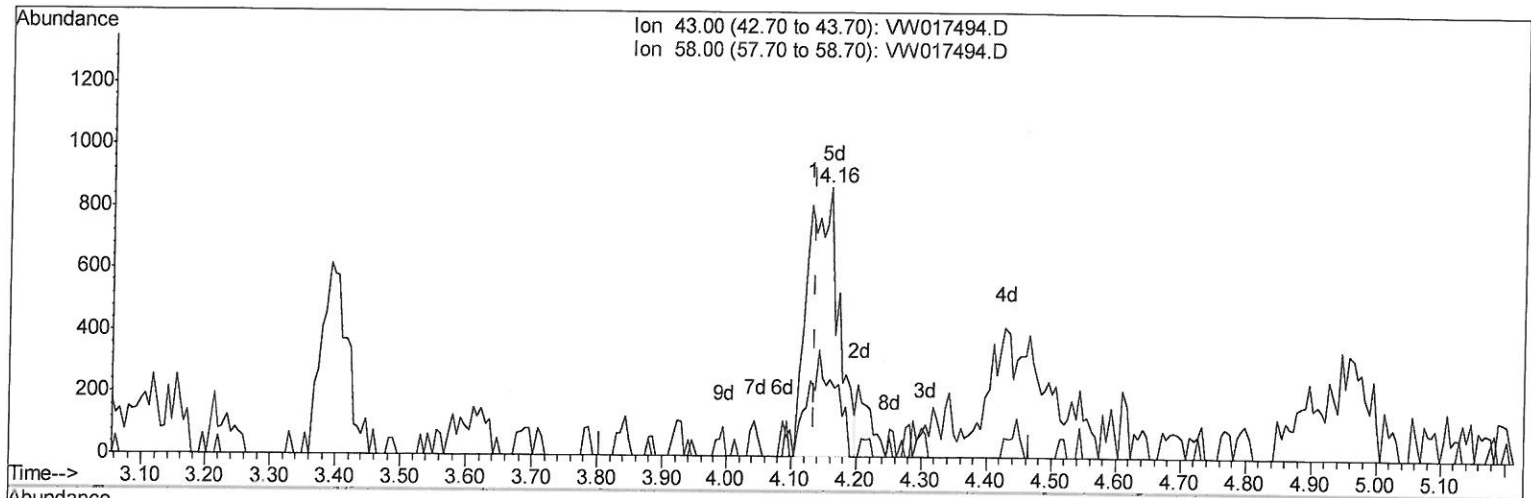

TIC: VW017494.D

(13) Acetone (T)

4.159min (+0.024) 2.36ug/L m

response 2825

Ion	Exp%	Act%
43.00	100	100
58.00	34.20	21.95
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112520\
Data File : VW017494.D
Acq On : 25 Nov 2020 11:25
Operator : SY/VA
Sample : VW1125SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VBLK11

Manual Integrations
APPROVED

MMDadoda
11/27/2020 1:20:14 PM

Quant Time: Nov 26 07:24:11 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 26 07:23:09 2020
Response via : Initial Calibration

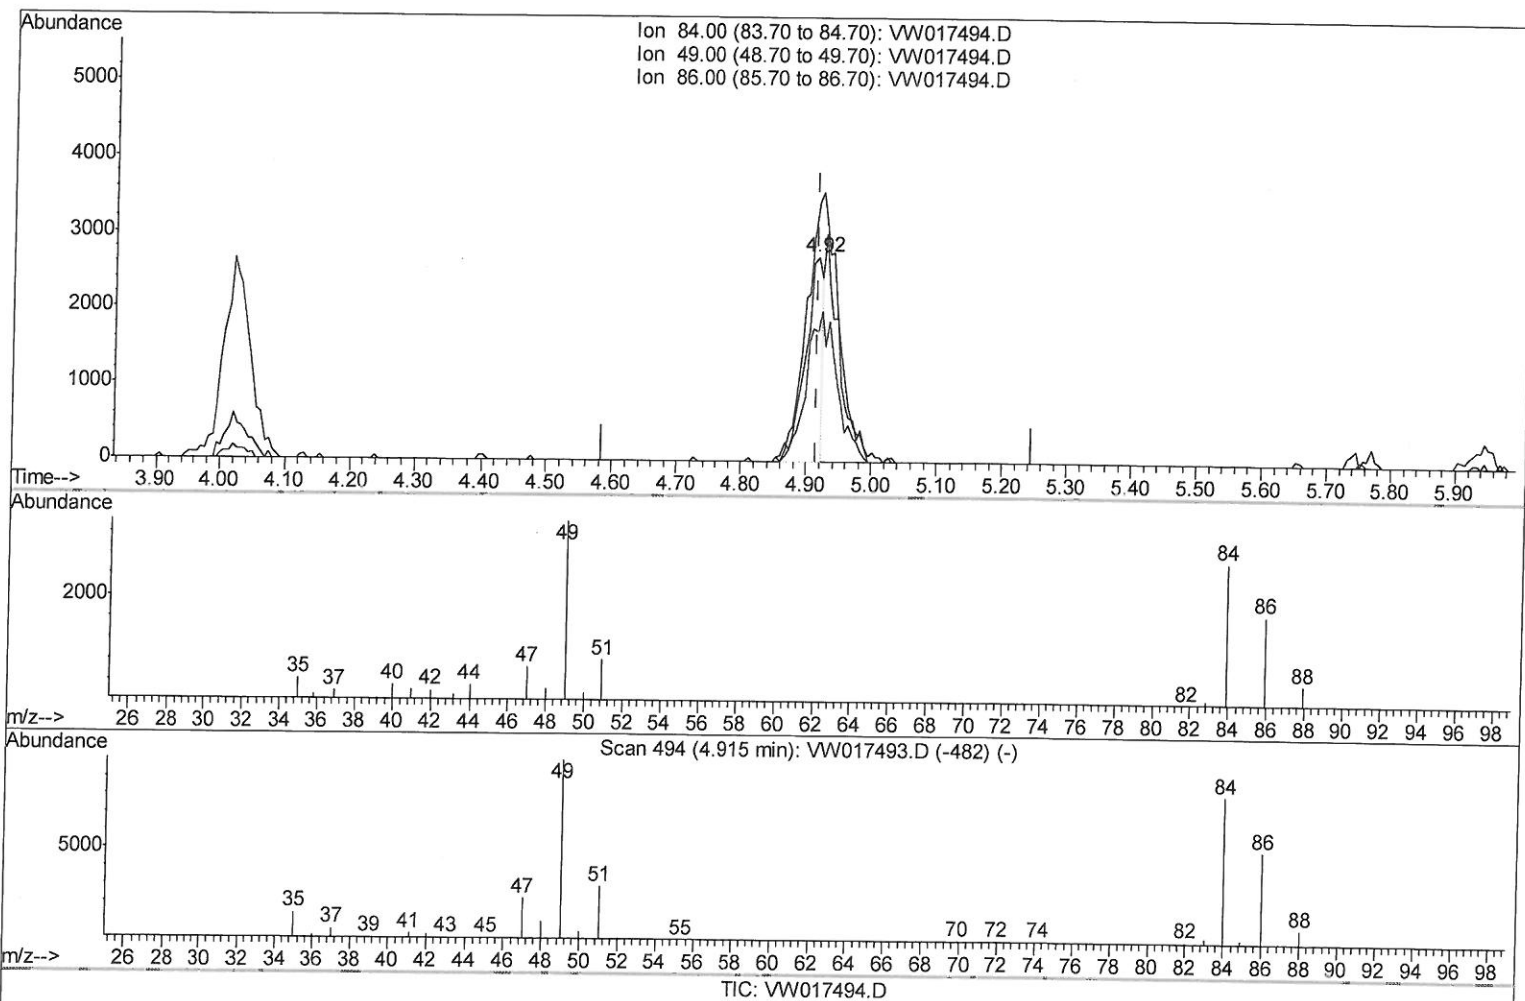

(16) Methylene chloride (T)

4.915min (-0.000) 0.74ug/L

response 4997

Ion	Exp%	Act%
84.00	100	100
49.00	116.00	126.39
86.00	63.60	63.49
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112520\
 Data File : VW017494.D
 Acq On : 25 Nov 2020 11:25
 Operator : SY/VA
 Sample : VW1125SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 VBLK11

Manual Integrations
 APPROVED

MMDadoda
 11/27/2020 1:20:14 PM

Quant Time: Nov 26 07:24:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 26 07:23:09 2020
 Response via : Initial Calibration

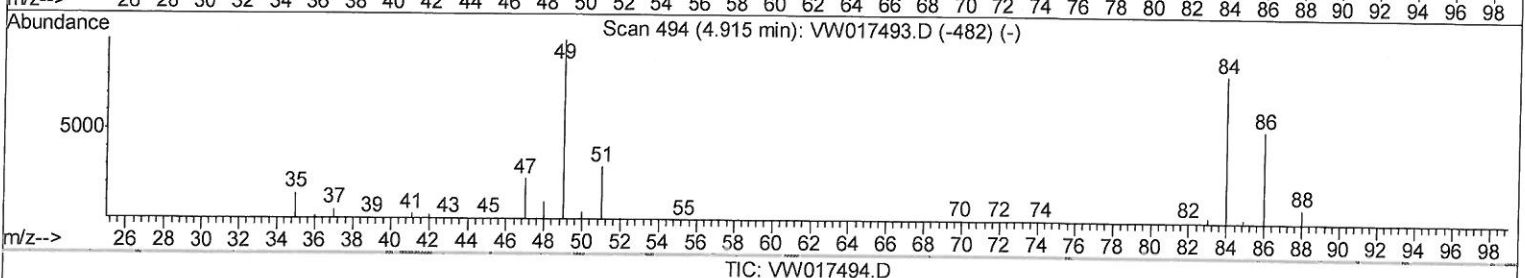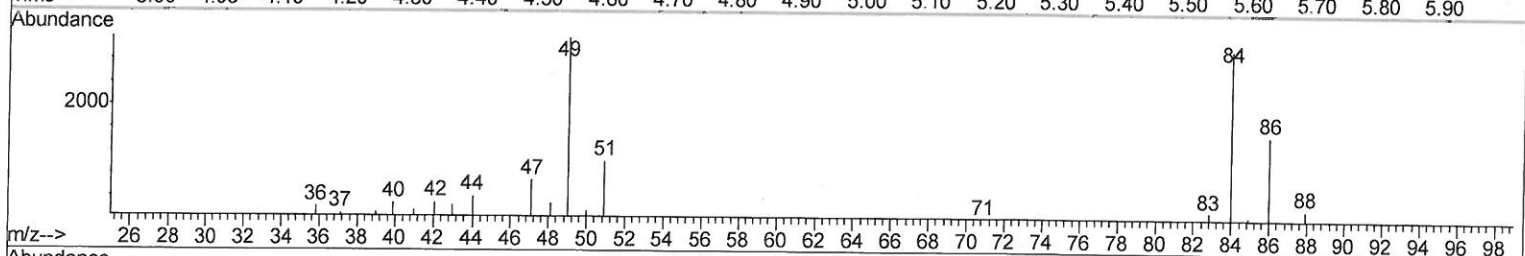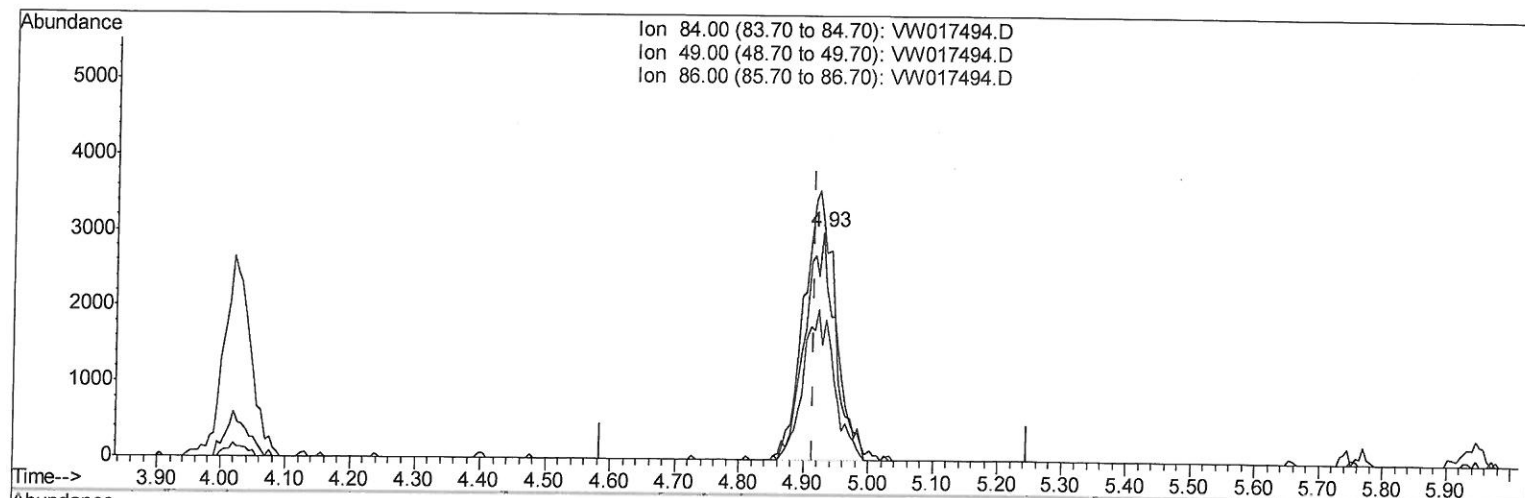

(16) Methylene chloride (T)

4.928min (+0.012) 1.45ug/L m

response 9722

Ion	Exp%	Act%
84.00	100	100
49.00	116.00	105.94
86.00	63.60	50.45
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112520\
 Data File : VW017494.D
 Acq On : 25 Nov 2020 11:25
 Operator : SY/VA
 Sample : VW1125SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK11

Manual Integrations
 APPROVED

MMDadoda
 11/27/2020 1:20:14 PM

Quant Time: Nov 26 07:28:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 26 07:23:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	447863	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	400495	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	194683	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	145112	24.63	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	98.52%		
7) Chloroethane-d5	2.90	69	116799	23.49	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.96%		
10) 1,1-Dichloroethene-d2	4.03	63	245103	18.69	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	74.76%		
20) 2-Butanone-d5	7.08	46	69794	56.18	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	112.36%		
24) Chloroform-d	7.65	84	311581	24.49	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	97.96%		
26) 1,2-Dichloroethane-d4	8.31	65	171089	27.41	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	109.64%		
29) Benzene-d6	8.28	84	599570	24.35	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	97.40%		
33) 1,2-Dichloropropane-d6	9.27	67	169863	24.93	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	99.72%		
37) Toluene-d8	10.32	98	549662	24.51	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	98.04%		
38) trans-1,3-Dichloropropene-	10.58	79	74599	24.50	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	98.00%		
39) 2-Hexanone-d5	10.93	63	46753	55.43	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	110.86%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	125481	25.59	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	102.36%		
61) 1,2-Dichlorobenzene-d4	13.85	152	185770	25.77	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	103.08%		

Target Compounds

				Ovalue
13) Acetone	4.16	43	2825m	2.363 ug/L
16) Methylene chloride	4.93	84	9722m	1.446 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112520\
Data File : VW017494.D
Acq On : 25 Nov 2020 11:25
Operator : SY/VA
Sample : VW1125SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK11

Manual Integrations
APPROVED

MMDadoda
11/27/2020 1:20:14 PM

Quant Time: Nov 26 07:28:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 26 07:23:09 2020
Response via : Initial Calibration

