

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112520\
Data File : VW017496.D
Acq On : 25 Nov 2020 12:20
Operator : SY/VA
Sample : L4860-17
Misc : 1.75G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BE3

Manual Integrations
APPROVED

MMDadoda
11/27/2020 1:20:29 PM

Quant Time: Nov 26 07:24:23 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 26 07:23:09 2020
Response via : Initial Calibration

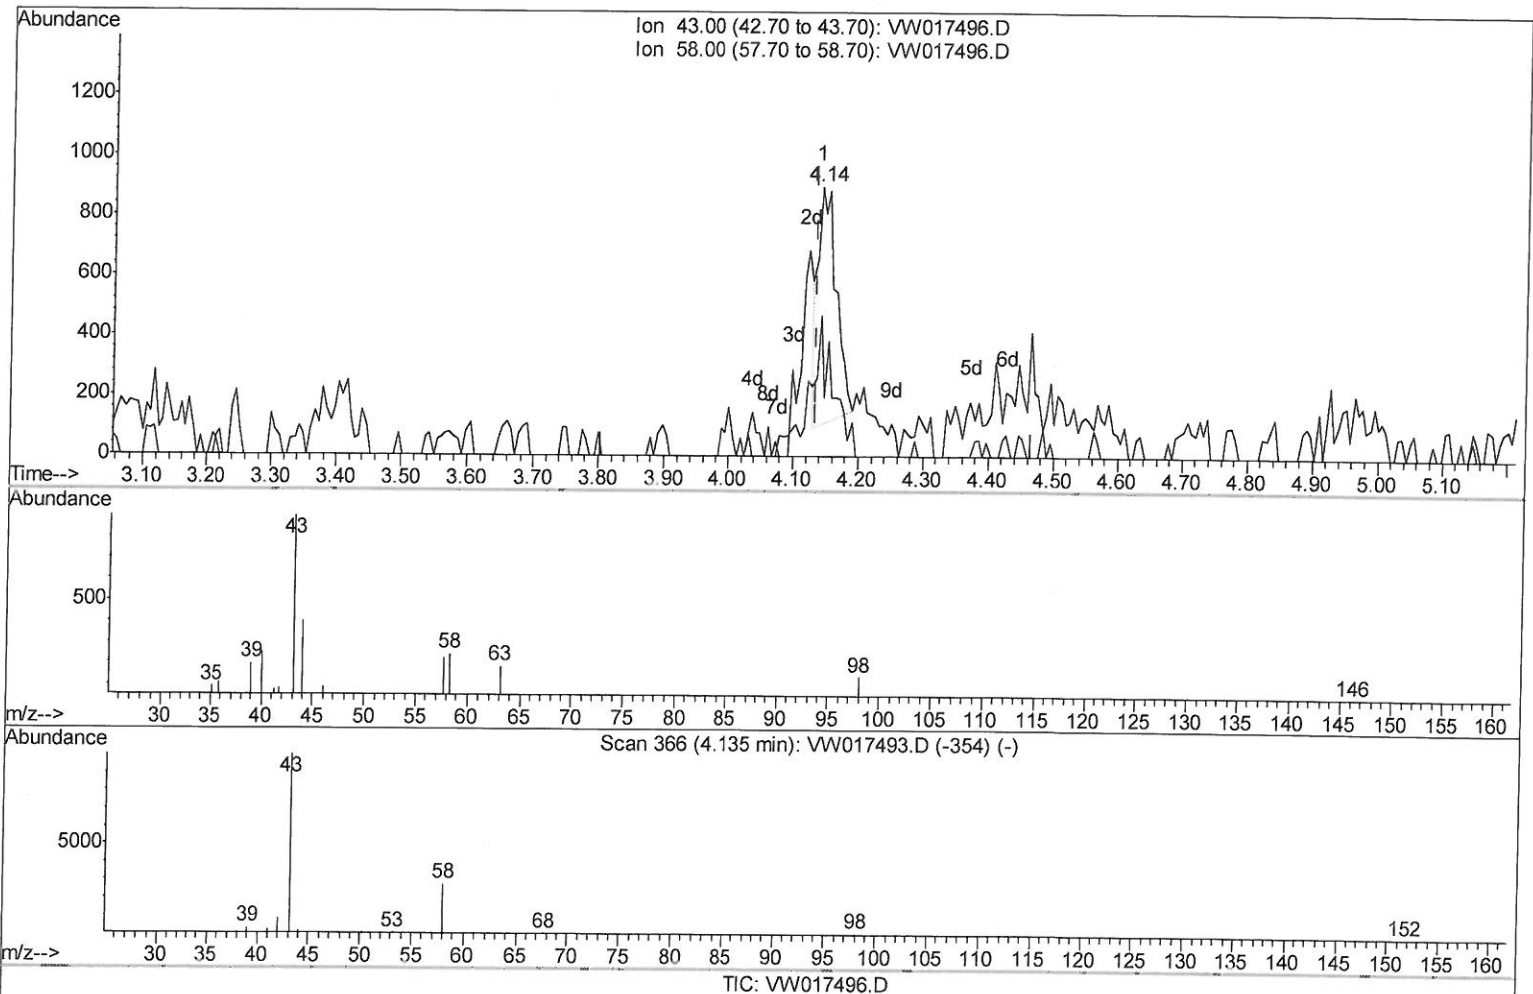

(13) Acetone (T)

4.141min (+0.006) 0.99ug/L

response 1528

Ion	Exp%	Act%
43.00	100	100
58.00	34.20	9.75
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112520\
 Data File : VW017496.D
 Acq On : 25 Nov 2020 12:20
 Operator : SY/VA
 Sample : L4860-17
 Misc : 1.75G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BE3

Manual Integrations
 APPROVED

MMDadoda
 11/27/2020 1:20:29 PM

Quant Time: Nov 26 07:24:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 26 07:23:09 2020
 Response via : Initial Calibration

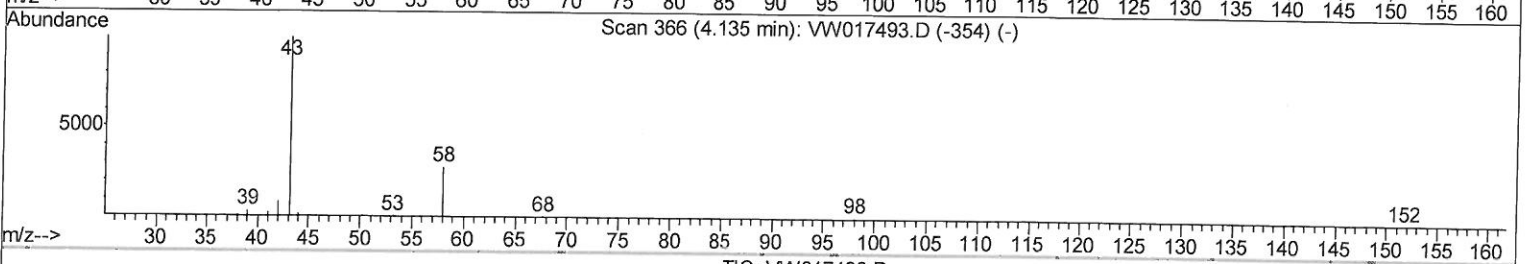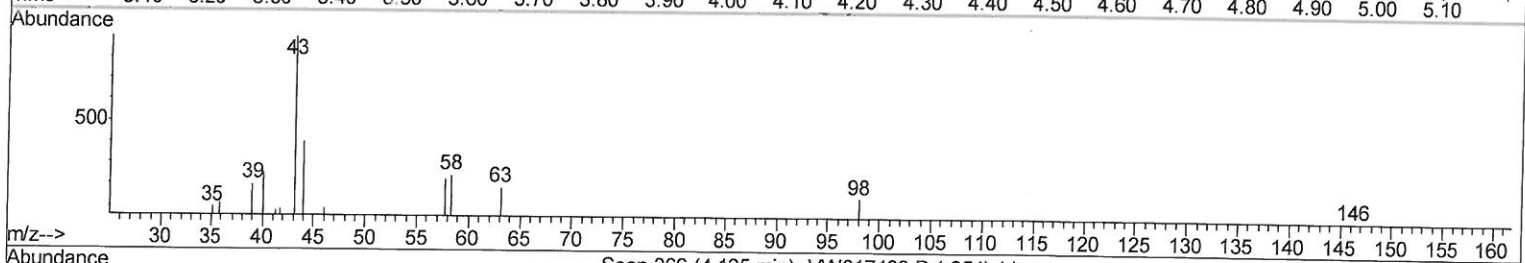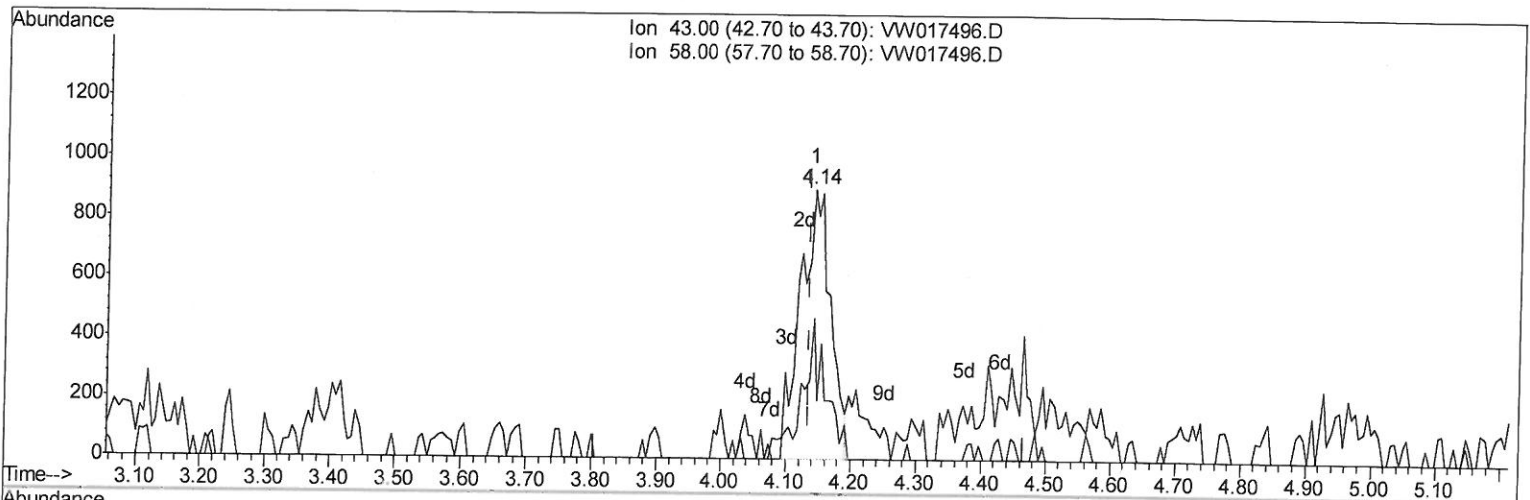

TIC: VW017496.D

(13) Acetone (T)

4.141min (+0.006) 1.91ug/L m

response 2932

Ion	Exp%	Act%
43.00	100	100
58.00	34.20	5.08
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112520\
 Data File : VW017496.D
 Acq On : 25 Nov 2020 12:20
 Operator : SY/VA
 Sample : L4860-17
 Misc : 1.75G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BE3

Manual Integrations
 APPROVED

MMDadoda
 11/27/2020 1:20:29 PM

Quant Time: Nov 26 07:35:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 26 07:23:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	575920	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	513798	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	245410	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	128756	17.00	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	68.00%		
7) Chloroethane-d5	2.90	69	113082	17.69	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.76%		
10) 1,1-Dichloroethene-d2	4.03	63	237444	14.08	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	56.32%		
20) 2-Butanone-d5	7.08	46	58635	36.70	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	73.40%		
24) Chloroform-d	7.65	84	309731	18.93	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	75.72%		
26) 1,2-Dichloroethane-d4	8.31	65	157584	19.63	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	78.52%		
29) Benzene-d6	8.27	84	604393	19.13	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	76.52%		
33) 1,2-Dichloropropane-d6	9.28	67	172746	19.76	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	79.04%		
37) Toluene-d8	10.33	98	557168	19.36	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	77.44%		
38) trans-1,3-Dichloropropene-	10.58	79	70107	17.95	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	71.80%		
39) 2-Hexanone-d5	10.93	63	38614	35.68	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	71.36%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	110979	17.64	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	70.56%		
61) 1,2-Dichlorobenzene-d4	13.85	152	189442	20.85	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	83.40%		

Target Compounds

					Ovalue
13) Acetone	4.14	43	2932m	1.907	ug/L 96
16) Methylene chloride	4.93	84	28105	3.250	ug/L 96
43) 4-Methyl-2-pentanone	10.21	43	2504	0.750	ug/L 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112520\
Data File : VW017496.D
Acq On : 25 Nov 2020 12:20
Operator : SY/VA
Sample : L4860-17
Misc : 1.75G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
C0BE3

Manual Integrations
APPROVED

MMDadoda
11/27/2020 1:20:29 PM

Quant Time: Nov 26 07:35:34 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 26 07:23:09 2020
Response via : Initial Calibration

