

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112520\
 Data File : VW017494.D
 Acq On : 25 Nov 2020 11:25
 Operator : SY/VA
 Sample : VW1125SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK11

Manual Integrations
 APPROVED

MMDadoda
 11/27/2020 1:20:14 PM

Quant Time: Nov 26 07:28:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 26 07:23:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	447863	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	400495	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	194683	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	145112	24.63	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.52%
7) Chloroethane-d5	2.90	69	116799	23.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.96%
10) 1,1-Dichloroethene-d2	4.03	63	245103	18.69	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.76%
20) 2-Butanone-d5	7.08	46	69794	56.18	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.36%
24) Chloroform-d	7.65	84	311581	24.49	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.96%
26) 1,2-Dichloroethane-d4	8.31	65	171089	27.41	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	109.64%
29) Benzene-d6	8.28	84	599570	24.35	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.40%
33) 1,2-Dichloropropane-d6	9.27	67	169863	24.93	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.72%
37) Toluene-d8	10.32	98	549662	24.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.04%
38) trans-1,3-Dichloropropene-	10.58	79	74599	24.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.00%
39) 2-Hexanone-d5	10.93	63	46753	55.43	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.86%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	125481	25.59	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.36%
61) 1,2-Dichlorobenzene-d4	13.85	152	185770	25.77	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.08%

Target Compounds				Ovalue
13) Acetone	4.16	43	2825m	2.363 ug/L
16) Methylene chloride	4.93	84	9722m	1.446 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW112520\
Data File : VW017494.D
Acq On : 25 Nov 2020 11:25
Operator : SY/VA
Sample : VW1125SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VBLK11

Manual Integrations
APPROVED

MMDadoda
11/27/2020 1:20:14 PM

Quant Time: Nov 26 07:28:47 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 26 07:23:09 2020
Response via : Initial Calibration

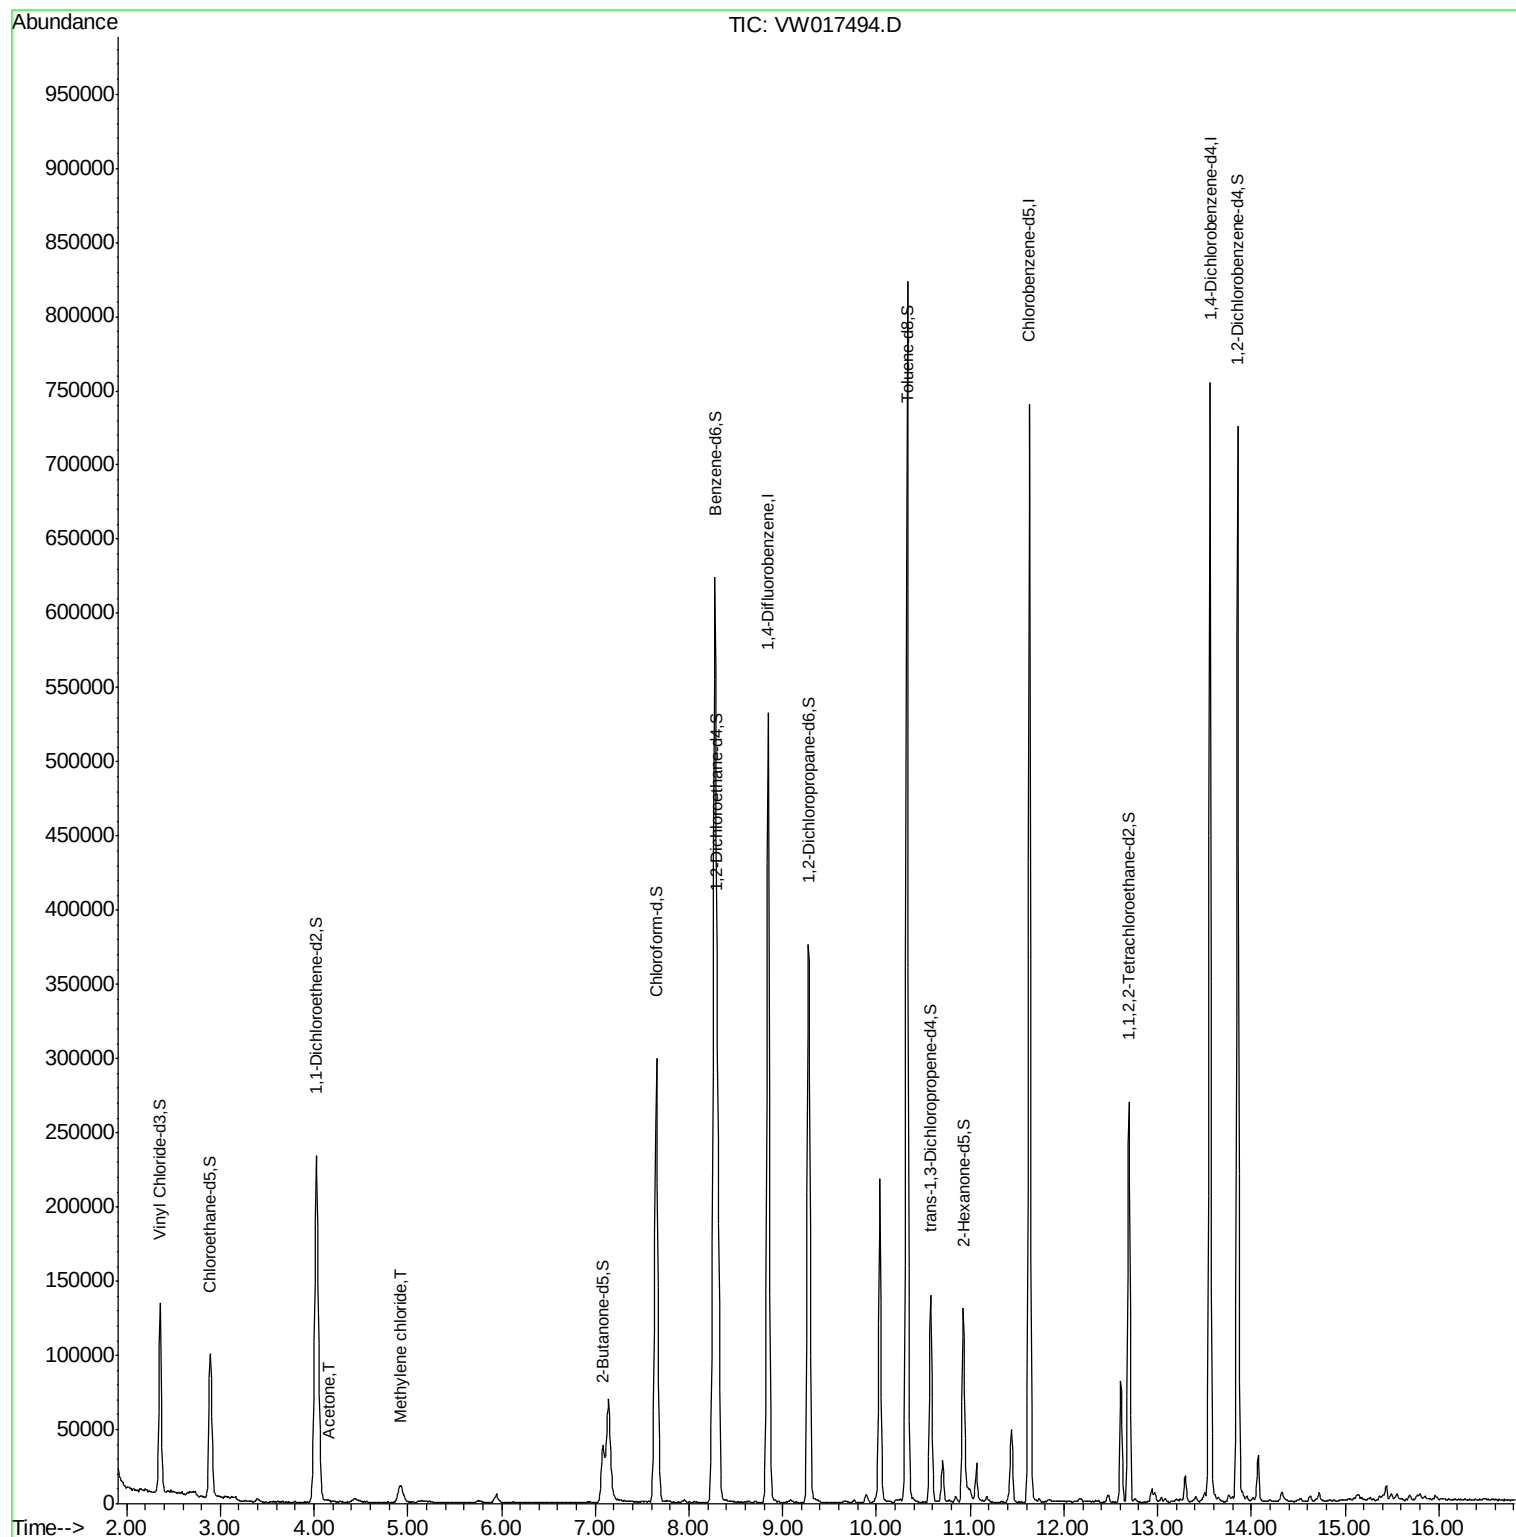

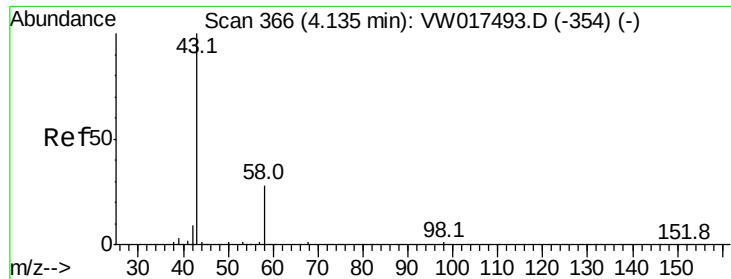

#13

Acetone

Concen: 2.363 ug/L m

RT: 4.16 min Scan# 370

Delta R.T. 0.02 min

Lab File: VW017494.D

Acq: 25 Nov 2020 11:25

Instrument :

MSVOA_W

ClientSampled :

VBLK11

Tot Ion: 43 Resp: 2825

Ion Ratio Lower Upper

43 100





58 21.9 0.0 68.4

Manual Integrations

APPROVED

MMDadoda

11/27/2020 1:20:14 PM

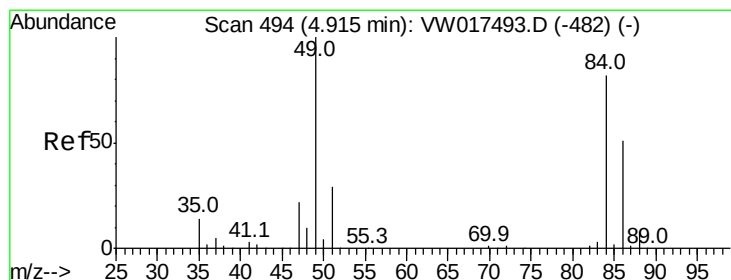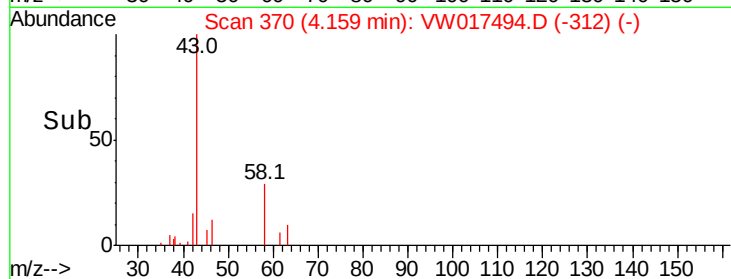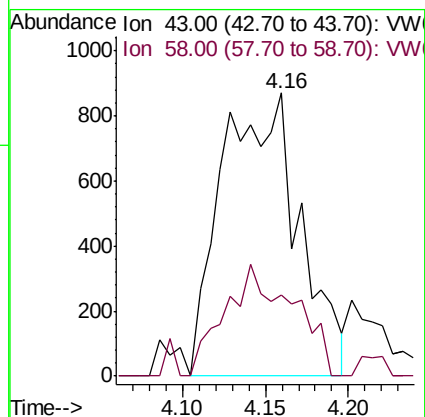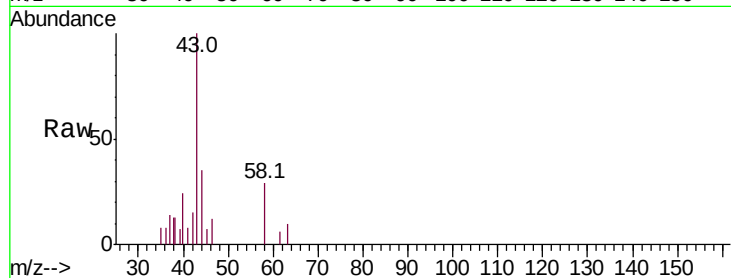

#16

Methylene chloride

Concen: 1.446 ug/L m

RT: 4.93 min Scan# 496

Delta R.T. 0.01 min

Lab File: VW017494.D

Acq: 25 Nov 2020 11:25

Tgt Ion: 84 Resp: 9722

Ion Ratio Lower Upper

84 100

49 105.9 81.2 150.8

86 50.4 44.5 82.7

