


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW112520\
 Data File : VW017492.D
 Acq On : 25 Nov 2020 09:12
 Operator : SY/VA
 Sample : BFB13
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB13

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Title : VOC Analysis
 Last Update : Thu Nov 26 07:23:09 2020

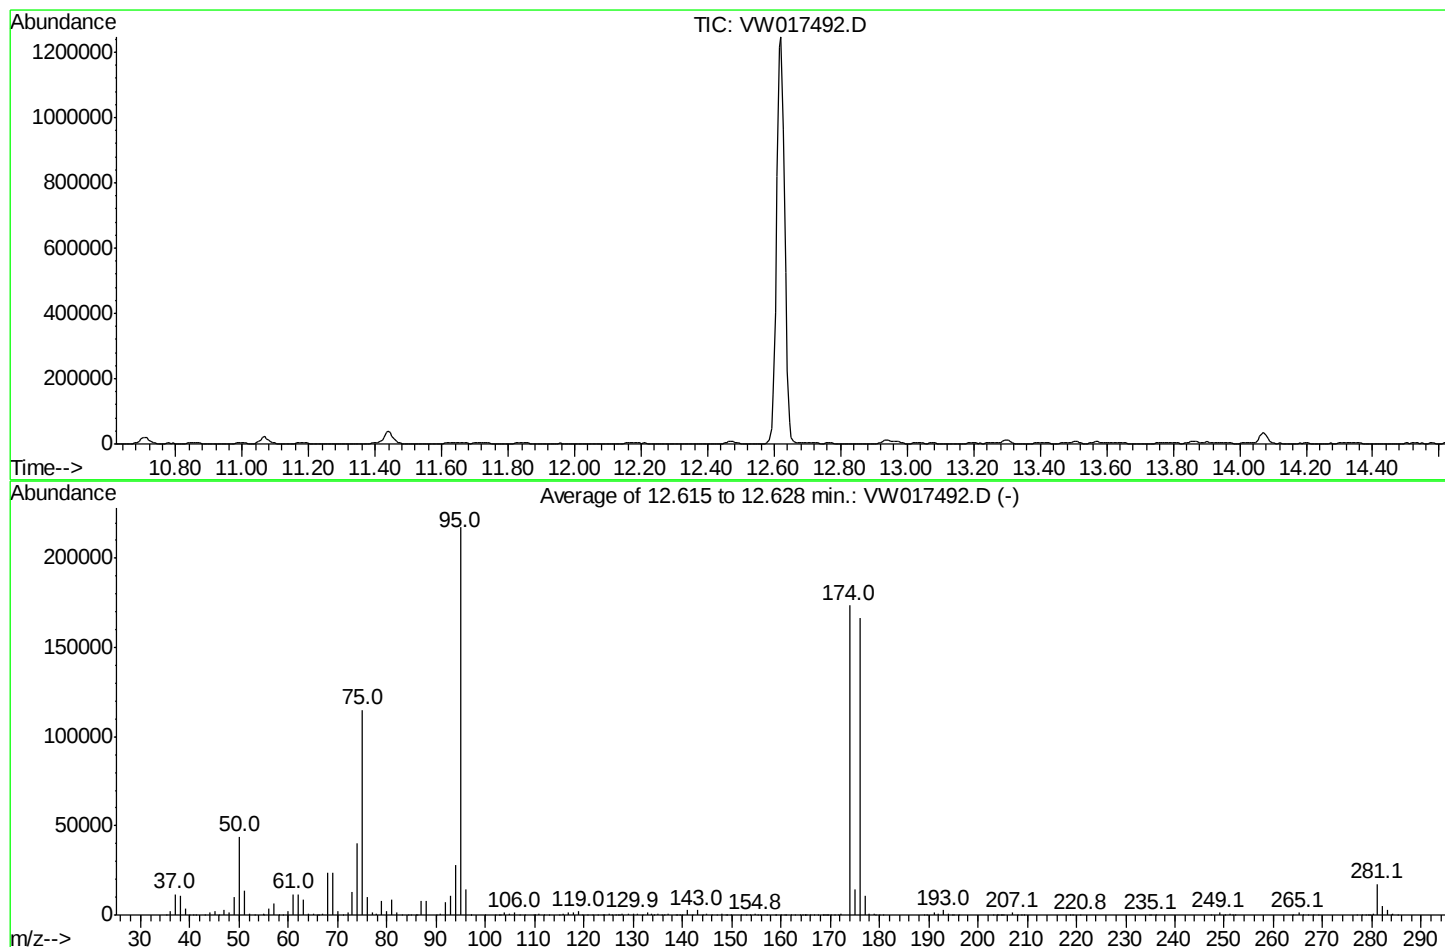

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	44168	PASS
75	95	30	80	52.9	115088	PASS
95	95	100	100	100.0	217408	PASS
96	95	5	9	6.7	14576	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.8	173525	PASS
175	174	5	9	8.3	14329	PASS
176	174	95	101	96.0	166549	PASS
177	176	5	9	6.6	11026	PASS

Scan 1749 (12.567 min): VW017492.D
BFB13

m/z	Abundance
40.10	221.0
42.20	91.0
43.10	87.0
44.10	314.0
68.90	107.0
71.20	53.0
74.70	64.0
168.90	130.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

m/z	Abundance
35.10	105.0
36.10	2578.0
37.00	13343.0
38.00	11642.0
39.10	4274.0
40.00	341.0
41.10	93.0
43.10	343.0
44.00	1664.0
45.10	2598.0
45.90	286.0
47.00	2961.0
48.00	1727.0
49.10	10893.0
50.00	49128.0
51.10	15730.0
52.00	640.0
53.10	160.0
54.90	682.0
56.00	4221.0
57.00	7211.0
58.20	362.0
59.10	474.0
60.00	2515.0
61.00	12866.0
62.00	12452.0
63.10	9402.0
64.00	973.0
65.20	382.0
65.90	274.0
67.00	760.0
68.00	25392.0
69.00	26368.0
70.00	2122.0
71.00	165.0
72.00	1695.0
73.00	14396.0
74.00	44104.0
75.10	125432.0
76.10	10758.0
77.10	1501.0
77.80	707.0
78.90	8834.0
80.00	2878.0
81.00	9777.0
81.90	1850.0
83.20	265.0
84.20	110.0
84.90	98.0
85.90	306.0
87.00	9081.0
87.90	8874.0
90.00	64.0
91.00	1210.0
92.00	7769.0
93.00	10688.0
94.00	29760.0
95.00	231616.0
96.10	16728.0
97.00	601.0
100.00	61.0
101.90	123.0
102.90	720.0
103.90	1506.0
104.90	634.0
105.90	1227.0
107.00	273.0
109.90	421.0
111.00	395.0
112.00	287.0
112.90	289.0
115.00	421.0
115.80	896.0
117.00	1590.0
118.00	1400.0
119.00	1986.0
119.80	142.0
120.90	126.0
121.70	61.0
122.90	153.0
123.80	152.0
124.00	148.0
125.10	1268.0
125.80	440.0
126.50	117.0
127.10	116.0
127.80	826.0
129.00	502.0
130.00	816.0
130.90	412.0
132.00	138.0
133.10	2520.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

133.80	547.0
135.00	595.0
136.20	125.0
137.10	557.0
138.70	101.0
139.50	109.0
141.00	2882.0
142.00	418.0
143.00	2864.0
144.00	174.0
145.00	579.0
145.90	304.0
146.80	389.0
148.00	709.0
148.80	280.0
149.90	319.0
151.90	57.0
153.00	287.0
153.90	191.0
154.80	489.0
155.30	253.0
157.10	272.0
158.80	283.0
160.00	90.0
160.80	451.0
162.10	94.0
163.00	408.0
164.30	125.0
164.80	335.0
165.10	282.0
166.00	92.0
166.70	64.0
168.90	151.0
169.40	108.0
170.00	121.0
171.10	364.0
172.10	1069.0
174.00	170112.0
175.10	14361.0
176.00	160832.0
177.00	11038.0
178.00	681.0
179.10	760.0
180.00	96.0
180.80	65.0
189.10	223.0
189.60	111.0
191.10	2227.0
192.20	698.0
193.00	3782.0
194.00	810.0
194.90	370.0
196.20	90.0
203.10	323.0
204.00	113.0
205.00	729.0
207.10	1988.0
208.10	303.0
209.20	209.0
218.80	162.0
220.90	77.0
235.10	274.0
236.10	141.0
247.40	103.0
249.10	1547.0
250.10	406.0
251.00	658.0
252.20	200.0
264.00	62.0
265.10	1924.0
266.10	529.0
267.10	497.0
268.20	180.0
269.20	58.0
276.90	67.0
279.30	433.0
280.10	856.0
281.10	24064.0
282.20	6213.0
283.20	4873.0
283.90	592.0
284.30	730.0
285.10	333.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

m/z	Abundance
35.20	161.0
36.10	2242.0
37.10	13212.0
38.10	11750.0
39.10	4020.0
40.00	388.0
41.10	86.0
43.20	207.0
44.00	2050.0
45.00	2306.0
46.00	184.0
47.10	2898.0
48.10	1493.0
49.00	10180.0
50.00	48000.0
51.00	15505.0
52.00	703.0
52.90	93.0
55.10	1011.0
56.00	4544.0
57.00	7326.0
58.00	309.0
59.00	332.0
60.00	2685.0
61.00	13115.0
62.10	13001.0
63.00	9032.0
64.00	988.0
65.20	449.0
65.90	141.0
66.90	709.0
68.00	26976.0
69.00	26272.0
70.00	2084.0
71.10	140.0
72.00	1611.0
73.00	13928.0
74.00	45448.0
75.00	125960.0
76.10	11346.0
77.00	1310.0
77.90	1083.0
78.90	8805.0
80.00	2361.0
80.90	8768.0
82.00	1857.0
83.00	256.0
84.30	56.0
86.10	426.0
87.00	8324.0
88.00	8673.0
90.10	54.0
91.00	1125.0
92.00	7642.0
93.00	11731.0
94.00	32960.0
95.00	234880.0
96.00	15606.0
97.20	403.0
103.10	661.0
104.00	1318.0
105.00	466.0
106.00	1400.0
107.00	431.0
110.10	427.0
110.90	481.0
111.90	239.0
113.00	233.0
114.90	407.0
115.90	1087.0
116.90	2112.0
118.00	1372.0
118.90	2251.0
119.80	113.0
120.80	119.0
122.80	130.0
124.10	192.0
125.00	500.0
125.60	254.0
126.80	64.0
127.90	899.0
129.00	532.0
130.00	954.0
131.00	447.0
131.90	107.0
133.00	1708.0
133.80	463.0
134.30	282.0
134.90	700.0
135.80	128.0
136.20	129.0
136.90	476.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

138.90	122.0
140.00	307.0
140.90	2935.0
142.00	355.0
143.00	3110.0
144.00	270.0
144.90	204.0
145.90	473.0
146.90	424.0
147.90	679.0
149.10	286.0
149.90	293.0
151.90	57.0
153.00	205.0
153.80	217.0
154.90	668.0
155.80	99.0
157.00	378.0
159.00	407.0
160.00	101.0
160.80	355.0
162.10	88.0
163.00	235.0
164.00	116.0
165.00	353.0
166.80	68.0
167.40	125.0
168.90	255.0
170.00	161.0
170.90	247.0
172.10	1290.0
174.00	190464.0
175.00	16856.0
176.00	179392.0
177.00	12560.0
178.00	439.0
178.90	552.0
180.00	110.0
180.80	121.0
188.90	175.0
191.10	1725.0
192.00	510.0
193.00	2364.0
193.90	303.0
195.10	354.0
196.20	63.0
203.00	318.0
204.20	57.0
205.00	282.0
207.10	1217.0
208.20	324.0
208.90	199.0
219.10	80.0
220.80	67.0
235.10	346.0
236.10	184.0
247.40	66.0
249.10	1409.0
250.10	476.0
251.10	413.0
251.80	134.0
252.20	136.0
264.00	114.0
265.10	1427.0
266.00	213.0
267.00	422.0
268.00	168.0
269.20	56.0
276.80	177.0
277.90	112.0
278.80	268.0
279.50	287.0
281.10	17352.0
282.20	5891.0
283.10	2689.0
284.10	568.0
285.10	210.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

m/z	Abundance
35.10	81.0
36.00	1501.0
37.00	8017.0
38.10	8044.0
39.10	2767.0
39.90	323.0
40.70	83.0
41.20	82.0
43.00	85.0
44.10	1171.0
45.00	1555.0
46.10	211.0
47.00	2224.0
48.00	1240.0
49.00	8139.0
50.10	35376.0
51.10	10336.0
52.00	554.0
55.00	441.0
56.10	2957.0
57.00	5303.0
58.10	176.0
58.90	258.0
60.00	1961.0
61.00	9303.0
62.10	8587.0
63.00	7113.0
64.10	643.0
65.10	326.0
66.20	63.0
66.90	446.0
68.00	18656.0
69.00	19856.0
70.10	1505.0
71.00	114.0
72.00	1192.0
73.00	9564.0
74.00	32056.0
75.00	93872.0
76.00	8259.0
77.00	1055.0
77.90	622.0
78.90	6697.0
79.90	1688.0
81.00	7060.0
81.90	1439.0
83.10	309.0
87.10	6727.0
88.00	6606.0
90.90	856.0
92.00	5569.0
93.00	9360.0
94.10	21952.0
95.00	185728.0
96.00	11395.0
97.10	461.0
103.90	1086.0
104.90	431.0
106.00	870.0
107.00	207.0
108.00	70.0
110.00	268.0
111.00	304.0
111.80	239.0
113.00	160.0
115.00	230.0
115.90	1048.0
116.90	1586.0
117.90	1136.0
118.90	1518.0
119.90	59.0
122.80	143.0
124.10	172.0
125.10	200.0
125.90	110.0
126.90	53.0
127.80	569.0
129.00	379.0
129.80	752.0
131.00	414.0
133.00	1014.0
133.70	426.0
134.90	505.0
135.90	136.0
137.00	432.0
139.00	92.0
140.00	270.0
141.00	2236.0
142.00	316.0
143.00	2250.0
144.00	279.0
145.00	373.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13

145.70	316.0
146.90	324.0
147.90	651.0
148.80	168.0
150.00	234.0
152.90	133.0
153.80	106.0
154.80	469.0
155.90	130.0
157.10	268.0
159.10	271.0
161.00	420.0
162.90	333.0
163.80	87.0
164.90	208.0
166.80	79.0
167.40	79.0
168.60	110.0
169.10	112.0
169.70	150.0
171.60	563.0
172.20	714.0
174.00	160000.0
175.00	11772.0
176.00	159424.0
177.00	9482.0
178.00	337.0
179.20	97.0
179.90	78.0
189.00	158.0
191.00	874.0
191.90	372.0
193.00	1486.0
194.10	291.0
195.00	199.0
203.00	130.0
204.60	92.0
205.30	147.0
207.20	812.0
208.00	193.0
208.80	94.0
209.30	77.0
220.70	62.0
234.80	139.0
236.20	72.0
249.00	958.0
249.90	258.0
251.00	326.0
251.70	93.0
265.20	800.0
266.10	326.0
266.90	105.0
268.00	69.0
277.80	109.0
279.10	186.0
279.60	163.0
280.20	321.0
281.10	10786.0
282.20	3050.0
283.10	2067.0
284.20	371.0
285.00	127.0

Instrument :
MSVOA_W
ClientSampleId :
BFB13