

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112618\  
 Data File : VW007048.D  
 Acq On : 26 Nov 2018 15:34  
 Operator : VAY/AP  
 Sample : J6003-12  
 Misc : 6.23G/5ML/MSVOA W/SOIL  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 AOC2-05

Quant Time: Nov 27 05:24:54 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W112118S.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Nov 21 03:23:02 2018  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 7.96  | 168  | 92711    | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.85  | 114  | 143519   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.63 | 117  | 145008   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.57 | 152  | 70441    | 50.00 | ug/l  | 0.00     |

## System Monitoring Compounds

|                           |        |     |          |       |         |      |
|---------------------------|--------|-----|----------|-------|---------|------|
| 33) 1,2-Dichloroethane-d4 | 8.31   | 65  | 52174    | 57.48 | ug/l    | 0.00 |
| Spiked Amount             | 50.000 |     | Recovery | =     | 114.96% |      |
| 35) Dibromofluoromethane  | 7.89   | 113 | 49255    | 60.77 | ug/l    | 0.00 |
| Spiked Amount             | 50.000 |     | Recovery | =     | 121.54% |      |
| 50) Toluene-d8            | 10.34  | 98  | 238455   | 66.63 | ug/l    | 0.00 |
| Spiked Amount             | 50.000 |     | Recovery | =     | 133.26% |      |
| 62) 4-Bromofluorobenzene  | 12.62  | 95  | 107514   | 76.34 | ug/l    | 0.00 |
| Spiked Amount             | 50.000 |     | Recovery | =     | 152.68% |      |

## Target Compounds

|                               |       |     |          |          |        | Qvalue |
|-------------------------------|-------|-----|----------|----------|--------|--------|
| 3) Chloromethane              | 2.17  | 50  | 13757    | 18.034   | ug/l # | 68     |
| 6) Chloroethane               | 3.03  | 64  | 2044     | 4.940    | ug/l # | 1      |
| 11) Tert butyl alcohol        | 5.17  | 59  | 292      | 4.942    | ug/l # | 71     |
| 13) Acrolein                  | 3.85  | 56  | 164426   | 2709.683 | ug/l # | 1      |
| 14) Allyl chloride            | 4.78  | 41  | 327587   | 235.358  | ug/l # | 55     |
| 15) Acrylonitrile             | 5.45  | 53  | 120310   | 673.114  | ug/l # | 40     |
| 16) Acetone                   | 4.11  | 43  | 183903   | 1395.511 | ug/l # | 53     |
| 18) Methyl Acetate            | 4.75  | 43  | 142966   | 304.640  | ug/l # | 50     |
| 20) Methylene Chloride        | 4.78  | 84  | 82207    | 81.701   | ug/l # | 17     |
| 23) Vinyl Acetate             | 6.24  | 43  | 103623   | 72.029   | ug/l # | 74     |
| 24) 1,1-Dichloroethane        | 6.23  | 63  | 11245    | 6.823    | ug/l # | 83     |
| 25) 2-Butanone                | 7.17  | 43  | 59789    | 264.897  | ug/l # | 50     |
| 29) Tetrahydrofuran           | 7.54  | 42  | 4788     | 32.754   | ug/l # | 32     |
| 30) Chloroform                | 7.71  | 83  | 35669    | 20.372   | ug/l   | 93     |
| 31) Cyclohexane               | 7.94  | 56  | 1112933  | 636.660  | ug/l # | 55     |
| 36) 1,1-Dichloropropene       | 7.95  | 75  | 8554     | 6.099    | ug/l # | 48     |
| 37) Ethyl Acetate             | 7.17  | 43  | 59789    | 117.644  | ug/l # | 72     |
| 38) Carbon Tetrachloride      | 7.95  | 117 | 9805     | 7.301    | ug/l # | 16     |
| 39) Methylcyclohexane         | 9.34  | 83  | 1252430  | 713.603  | ug/l # | 81     |
| 40) Benzene                   | 8.33  | 78  | 8667736  | 2289.555 | ug/l   | 98     |
| 41) Methacrylonitrile         | 7.53  | 41  | 58346    | 184.863  | ug/l # | 51     |
| 42) 1,2-Dichloroethane        | 8.41  | 62  | 20387    | 18.548   | ug/l # | 74     |
| 43) Isopropyl Acetate         | 8.43  | 43  | 219253   | 226.385  | ug/l # | 49     |
| 45) 1,2-Dichloropropane       | 9.34  | 63  | 27677    | 29.657   | ug/l # | 1      |
| 46) Dibromomethane            | 9.48  | 93  | 782      | 1.673    | ug/l # | 1      |
| 47) Bromodichloromethane      | 9.63  | 83  | 137113   | 111.356  | ug/l # | 25     |
| 48) Methyl methacrylate       | 9.48  | 41  | 302177   | 647.077  | ug/l # | 28     |
| 51) 4-Methyl-2-Pentanone      | 10.27 | 43  | 836399   | 1708.902 | ug/l # | 79     |
| 52) Toluene                   | 10.40 | 92  | 20931023 | 8124.148 | ug/l # | 1      |
| 53) t-1,3-Dichloropropene     | 10.40 | 75  | 288004   | 241.455  | ug/l # | 1      |
| 55) 1,1,2-Trichloroethane     | 10.77 | 97  | 333071   | 484.408  | ug/l # | 29     |
| 56) Ethyl methacrylate        | 10.63 | 69  | 38305    | 47.993   | ug/l # | 23     |
| 58) 2-Chloroethyl Vinyl ether | 9.91  | 63  | 25004    | 59.952   | ug/l # | 45     |
| 59) 2-Hexanone                | 10.94 | 43  | 209624   | 625.441  | ug/l # | 30     |

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112618\  
 Data File : VW007048.D  
 Acq On : 26 Nov 2018 15:34  
 Operator : VAY/AP  
 Sample : J6003-12  
 Misc : 6.23G/5ML/MSVOA W/SOIL  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 AOC2-05

Quant Time: Nov 27 05:24:54 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W112118S.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Nov 21 03:23:02 2018  
 Response via : Initial Calibration


| Internal Standards             | R.T.  | QIon | Response | Conc     | Units  | Dev(Min) |
|--------------------------------|-------|------|----------|----------|--------|----------|
| -----                          |       |      |          |          |        |          |
| 60) Dibromochloromethane       | 11.04 | 129  | 1590     | 2.029    | ug/l   | 79       |
| 61) 1,2-Dibromoethane          | 11.24 | 107  | 102092   | 162.311  | ug/l   | 90       |
| 67) Ethyl Benzene              | 11.74 | 91   | 9416289  | 1693.603 | ug/l   | 99       |
| 68) m/p-Xylenes                | 11.85 | 106  | 9756028  | 4472.518 | ug/l   | 94       |
| 69) o-Xylene                   | 12.18 | 106  | 4239077  | 2060.988 | ug/l   | 95       |
| 70) Styrene                    | 12.18 | 104  | 234574   | 71.657   | ug/l # | 1        |
| 73) Isopropylbenzene           | 12.47 | 105  | 978710   | 178.773  | ug/l   | 99       |
| 74) N-amyl acetate             | 12.26 | 43   | 127092   | 138.515  | ug/l # | 58       |
| 75) 1,1,2,2-Tetrachloroethane  | 12.71 | 83   | 8033     | 11.026   | ug/l # | 1        |
| 76) 1,2,3-Trichloropropane     | 12.81 | 75   | 28460    | 51.416   | ug/l # | 100      |
| 78) n-propylbenzene            | 12.81 | 91   | 4279030  | 645.270  | ug/l   | 99       |
| 79) 2-Chlorotoluene            | 12.88 | 91   | 1442765  | 377.331  | ug/l # | 42       |
| 80) 1,3,5-Trimethylbenzene     | 12.95 | 105  | 4679690  | 988.496  | ug/l   | 99       |
| 81) trans-1,4-Dichloro-2-buten | 12.47 | 75   | 12063    | 54.714   | ug/l # | 64       |
| 82) 4-Chlorotoluene            | 12.95 | 91   | 525653   | 131.004  | ug/l # | 42       |
| 83) tert-Butylbenzene          | 13.26 | 119  | 1639917  | 400.104  | ug/l # | 60       |
| 84) 1,2,4-Trimethylbenzene     | 13.26 | 105  | 12974980 | 2750.876 | ug/l   | 98       |
| 85) sec-Butylbenzene           | 13.26 | 105  | 12974980 | 2240.770 | ug/l # | 57       |
| 86) p-Isopropyltoluene         | 13.45 | 119  | 432849   | 84.733   | ug/l   | 98       |
| 89) n-Butylbenzene             | 13.83 | 91   | 561253   | 116.750  | ug/l # | 69       |
| 90) Hexachloroethane           | 14.10 | 117  | 250161   | 335.426  | ug/l # | 14       |
| 92) 1,2-Dibromo-3-Chloropropan | 14.51 | 75   | 4573     | 37.164   | ug/l # | 6        |
| 93) 1,2,4-Trichlorobenzene     | 15.14 | 180  | 2342     | 1.689    | ug/l # | 79       |
| 95) Naphthalene                | 15.38 | 128  | 1861074  | 739.183  | ug/l   | 99       |
| -----                          |       |      |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW112618\  
 Data File : VW007048.D  
 Acq On : 26 Nov 2018 15:34  
 Operator : VAY/AP  
 Sample : J6003-12  
 Misc : 6.23G/5ML/MSVOA W/SOIL  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 AOC2-05

Quant Time: Nov 27 05:24:54 2018  
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_W\METHOD\82W112118S.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Nov 21 03:23:02 2018  
 Response via : Initial Calibration

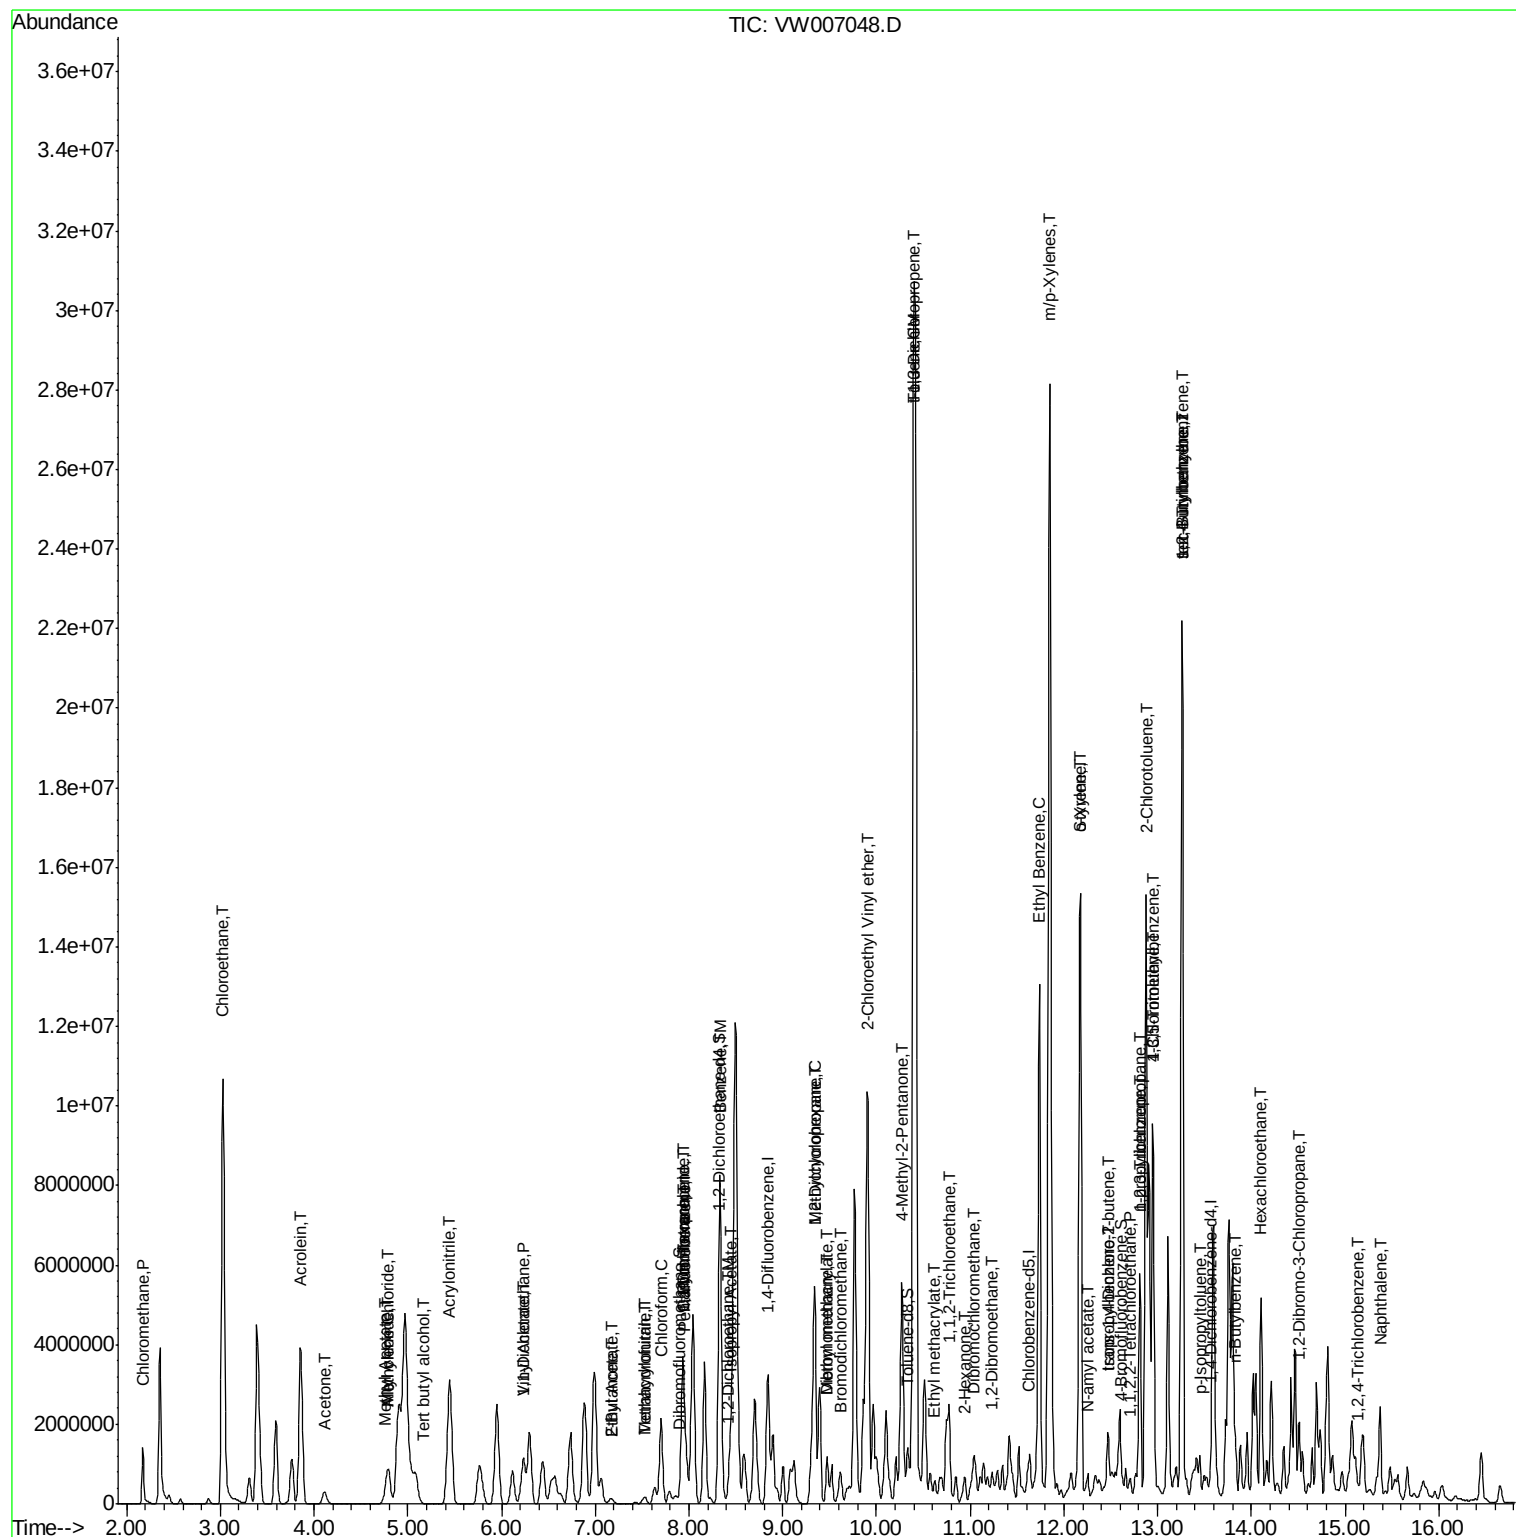



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.96 min Scan# 993

Delta R.T. 0.01 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :


AOC2-05

Tot Ion:168 Resp: 92711

Ion Ratio Lower Upper

168 100

99 66.1 48.2 72.4





Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.96

Time-->



#3

Chloromethane

Concen: 18.034 ug/l

RT: 2.17 min Scan# 44

Delta R.T. -0.04 min

Lab File: VW007048.D


Acq: 26 Nov 2018 15:34

Tgt Ion: 50 Resp: 13757

Ion Ratio Lower Upper

50 100

52 14.3 25.7 38.5#





Abundance Ion 49.90 (49.60 to 50.60): VW

Ion 51.90 (51.60 to 52.60): VW

2.17

Time-->





#6

Chloroethane

Concen: 4.940 ug/l

RT: 3.03 min Scan# 185

Delta R.T. 0.11 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :





AOC2-05

Tot Ion: 64 Resp: 2044

Ion Ratio Lower Upper

64 100

66 115.9 25.3 37.9#

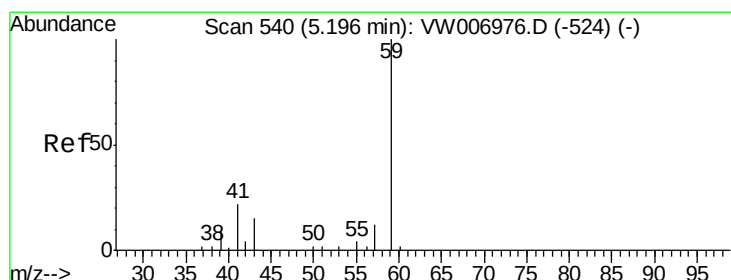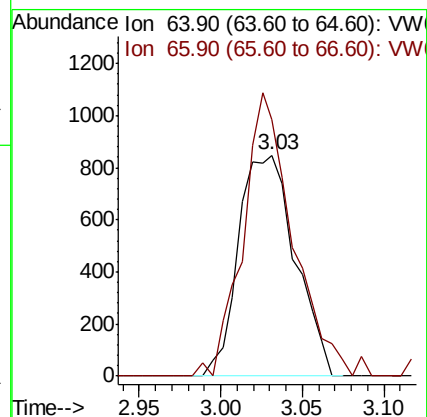

#11

Tert butyl alcohol

Concen: 4.942 ug/l

RT: 5.17 min Scan# 536

Delta R.T. -0.02 min

Lab File: VW007048.D




Acq: 26 Nov 2018 15:34


Tgt Ion: 59 Resp: 292

Ion Ratio Lower Upper

59 100

57 0.0 8.6 13.0#

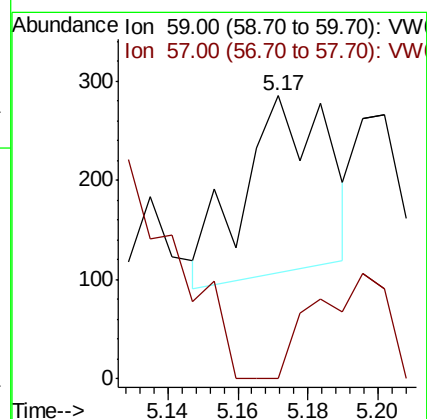

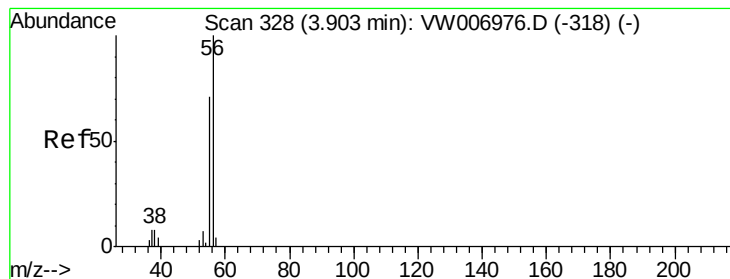

#13

Acrolein

Concen: 2709.683 ug/l

RT: 3.85 min Scan# 320

Delta R.T. -0.05 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :





AOC2-05

Tot Ion: 56 Resp: 164426

Ion Ratio Lower Upper

56 100

55 2188.9 57.5 86.3#

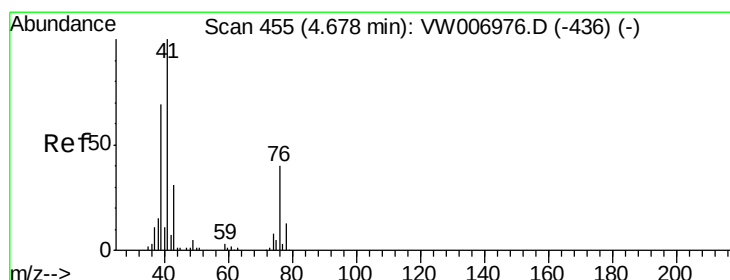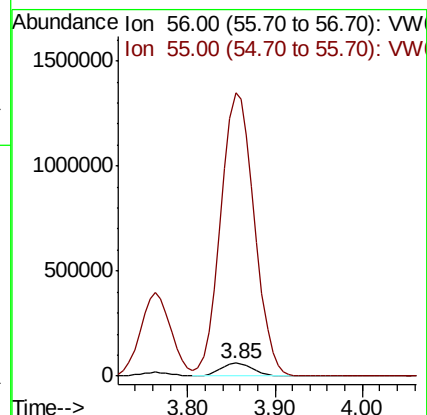

#14

Allyl chloride

Concen: 235.358 ug/l

RT: 4.78 min Scan# 472

Delta R.T. 0.10 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34




Tgt Ion: 41 Resp: 327587


Ion Ratio Lower Upper

41 100

39 98.4 55.4 83.2#

76 0.0 29.6 44.4#

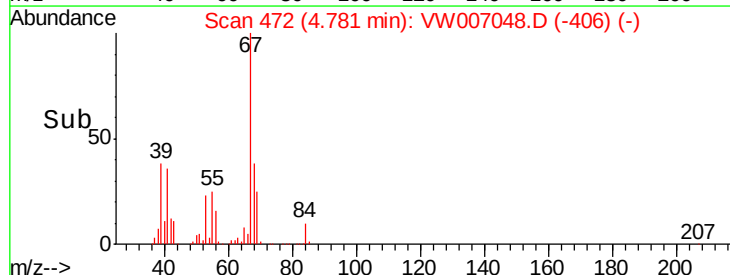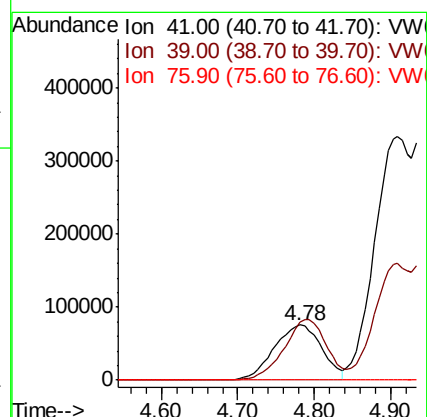



#15

Acrylonitrile

Concen: 673.114 ug/l

RT: 5.45 min Scan# 581

Delta R.T. 0.07 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :

AOC2-05




Tot Ion: 53 Resp: 120310

Ion Ratio Lower Upper

53 100

52 19.7 65.7 98.5#

51 60.7 29.9 44.9#

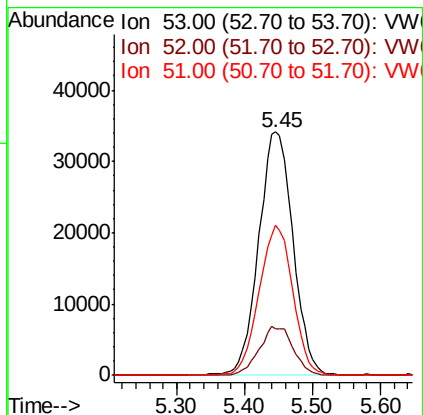

#16

Acetone

Concen: 1395.511 ug/l

RT: 4.11 min Scan# 362

Delta R.T. -0.03 min

Lab File: VW007048.D





Acq: 26 Nov 2018 15:34


Tgt Ion: 43 Resp: 183903

Ion Ratio Lower Upper

43 100

58 5.2 24.8 37.2#









#18  
Methvl Acetate  
Concen: 304.640 ug/l  
RT: 4.75 min Scan# 467  
Delta R.T. 0.07 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34




Instrument :  
MSVOA\_W  
ClientSampled :  
AOC2-05

Tot Ion: 43 Resp: 142966  
Ion Ratio Lower Upper  
43 100  
74 0.2 20.1 30.1#

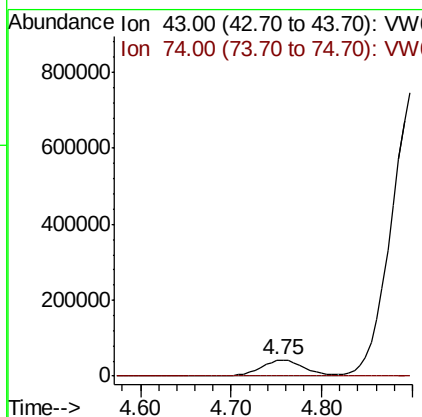


#20  
Methylene Chloride  
Concen: 81.701 ug/l  
RT: 4.78 min Scan# 472  
Delta R.T. -0.14 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34

Tgt Ion: 84 Resp: 82207  
Ion Ratio Lower Upper  
84 100  
49 7.1 93.4 140.0#  
51 54.0 28.4 42.6#  
86 0.0 49.8 74.8#

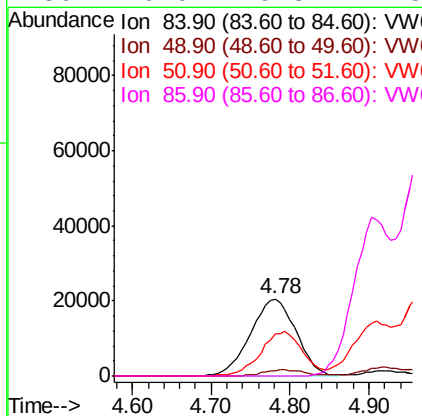





#23

Vinyl Acetate

Concen: 72.029 ug/l

RT: 6.24 min Scan# 711

Delta R.T. -0.02 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampled :





AOC2-05

Tot Ion: 43 Resp: 103623

Ion Ratio Lower Upper

43 100

86 1.0 8.7 13.1#

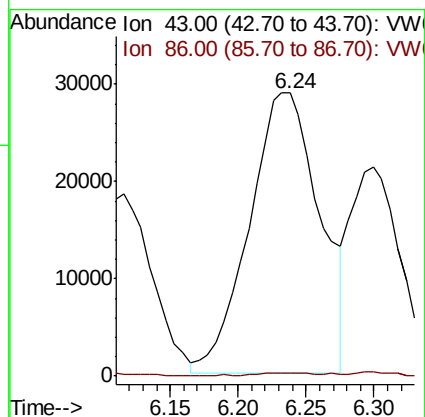

#24

1,1-Dichloroethane

Concen: 6.823 ug/l

RT: 6.23 min Scan# 710

Delta R.T. 0.01 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34




Tgt Ion: 63 Resp: 11245


Ion Ratio Lower Upper

63 100

98 0.0 3.1 9.4#

100 0.0 2.3 6.9#

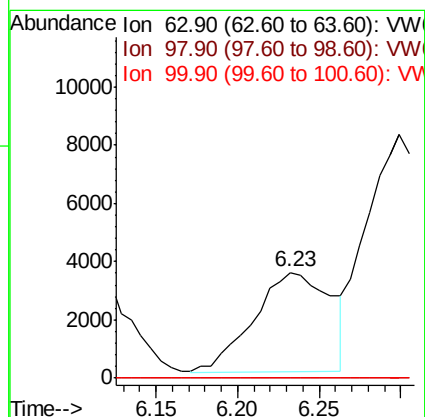



#25

2-Butanone

Concen: 264.897 ug/l

RT: 7.17 min Scan# 864

Delta R.T. -0.01 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampled :





AOC2-05

Tot Ion: 43 Resp: 59789

Ion Ratio Lower Upper

43 100

72 0.9 21.3 31.9#

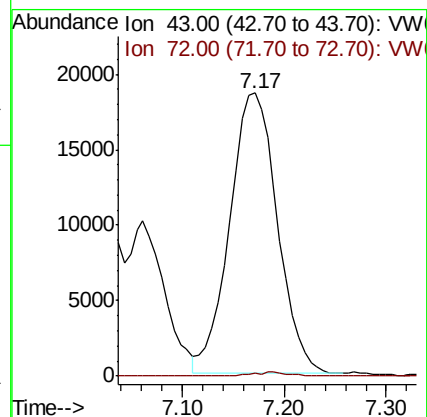

#29

Tetrahydrofuran

Concen: 32.754 ug/l

RT: 7.54 min Scan# 924

Delta R.T. -0.00 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34




Tgt Ion: 42 Resp: 4788


Ion Ratio Lower Upper

42 100

72 0.0 36.2 54.4#

71 0.0 33.8 50.8#

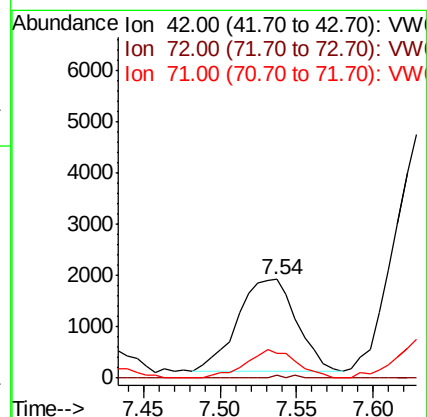



#30

Chloroform

Concen: 20.372 ug/l

RT: 7.71 min Scan# 952

Delta R.T. 0.03 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :





AOC2-05

Tot Ion: 83 Resp: 35669

Ion Ratio Lower Upper

83 100

85 69.0 50.9 76.3

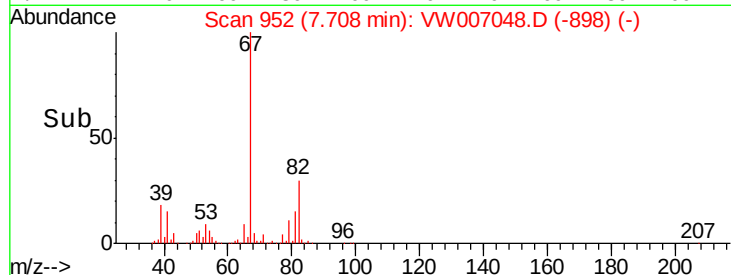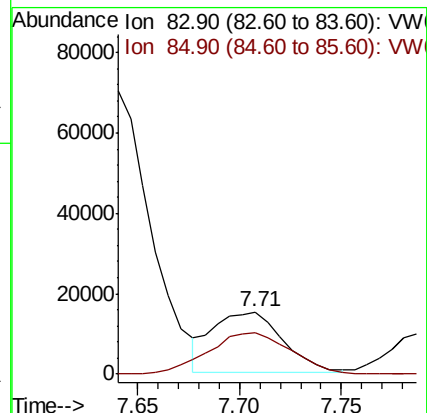

#31

Cyclohexane

Concen: 636.660 ug/l

RT: 7.94 min Scan# 990

Delta R.T. -0.02 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34




Tgt Ion: 56 Resp: 1112933


Ion Ratio Lower Upper

56 100

69 8.2 29.1 43.7#

84 47.1 70.6 105.8#



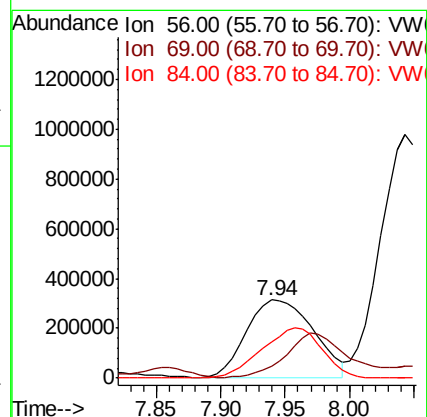





#33  
 1,2-Dichloroethane-d4  
 Concen: 57.482 ug/l  
 RT: 8.31 min Scan# 1051  
 Delta R.T. -0.00 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34




Instrument :  
 MSVOA\_W  
 ClientSampled :  
 AOC2-05


Tot Ion: 65 Resp: 52174  
 Ion Ratio Lower Upper  
 65 100  
 67 61.0 0.0 106.2

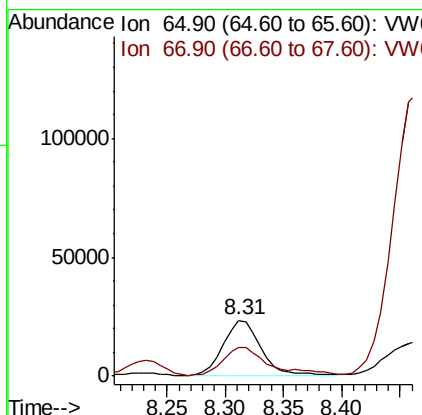

#34  
 1,4-Difluorobenzene  
 Concen: 50.000 ug/l  
 RT: 8.85 min Scan# 1139  
 Delta R.T. -0.00 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34

Tgt Ion: 114 Resp: 143519  
 Ion Ratio Lower Upper  
 114 100  
 63 40.1 0.0 39.4#  
 88 16.8 0.0 34.2



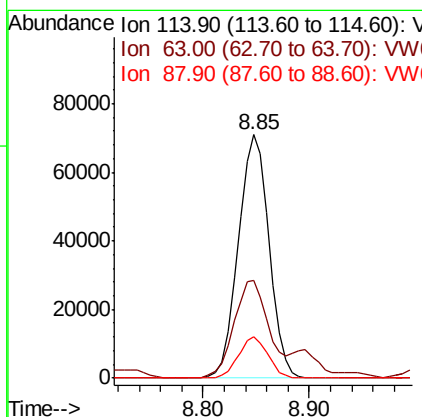





#35  
 Dibromofluoromethane  
 Concen: 60.772 ug/l  
 RT: 7.89 min Scan# 982  
 Delta R.T. -0.00 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34




Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 AOC2-05


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 113     | 100   |       |       |
| 111     | 103.4 | 81.0  | 121.6 |
| 192     | 18.6  | 15.0  | 22.6  |

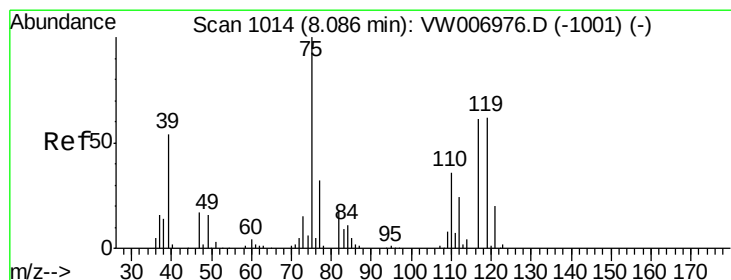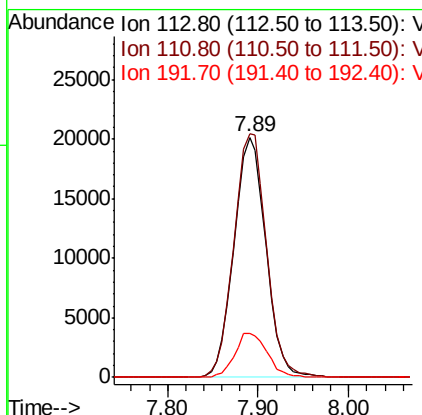

#36  
 1,1-Dichloropropene  
 Concen: 6.099 ug/l  
 RT: 7.95 min Scan# 992  
 Delta R.T. -0.13 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 75      | 100   |       |       |
| 110     | 7.8   | 18.0  | 54.0# |
| 77      | 0.0   | 24.9  | 37.3# |



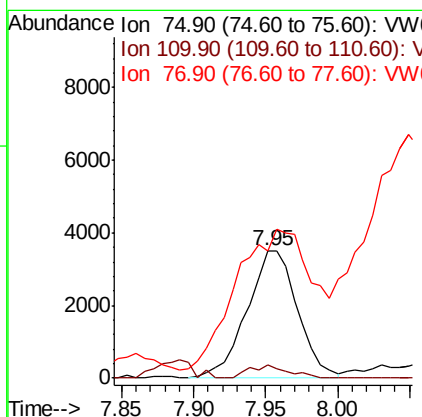





#37  
Ethyl Acetate  
Concen: 117.644 ug/l  
RT: 7.17 min Scan# 864  
Delta R.T. -0.09 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34




Instrument :  
MSVOA\_W  
ClientSampleId :  
AOC2-05


Tot Ion: 43 Resp: 59789  
Ion Ratio Lower Upper  
43 100  
61 0.0 10.4 15.6#  
70 2.6 8.8 13.2#

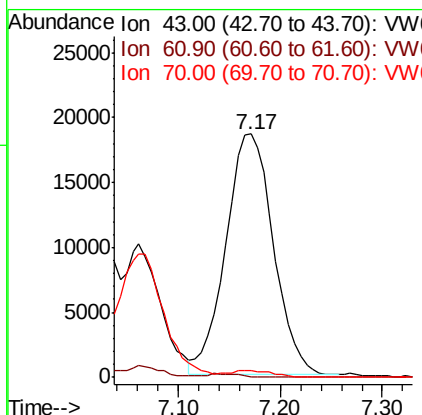

#38  
Carbon Tetrachloride  
Concen: 7.301 ug/l  
RT: 7.95 min Scan# 992  
Delta R.T. -0.12 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34

Tgt Ion: 117 Resp: 9805  
Ion Ratio Lower Upper  
117 100  
119 3.9 74.9 112.3#  
121 0.0 23.6 35.4#


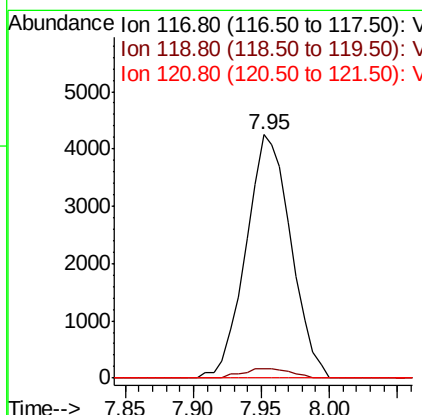






#39  
Methylcyclohexane  
Concen: 713.603 ug/l  
RT: 9.34 min Scan# 1220  
Delta R.T. 0.01 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34




Instrument :  
MSVOA\_W  
ClientSampleId :  
AOC2-05


Tot Ion: 83 Resp: 1252430  
Ion Ratio Lower Upper  
83 100  
55 98.4 59.6 89.4#  
98 49.2 37.1 55.7

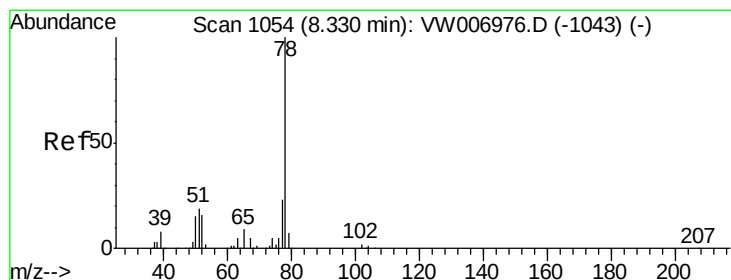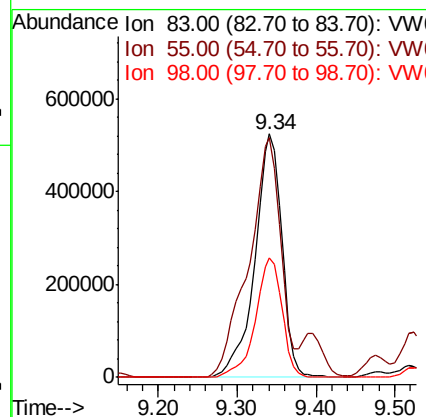

#40  
Benzene  
Concen: 2289.555 ug/l  
RT: 8.33 min Scan# 1054  
Delta R.T. -0.00 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34

Tgt Ion: 78 Resp: 8667736  
Ion Ratio Lower Upper  
78 100  
77 24.3 18.6 28.0



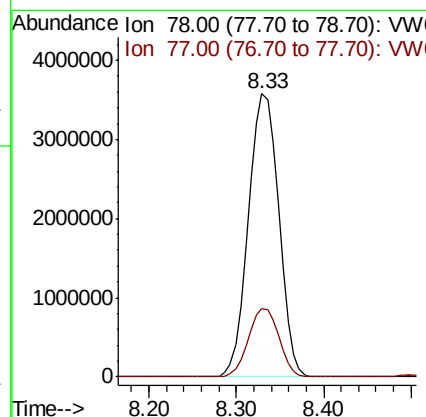





#41  
Methacrylonitrile  
Concen: 184.863 ug/l  
RT: 7.53 min Scan# 923  
Delta R.T. 0.04 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34




Instrument :  
MSVOA\_W  
ClientSampleId :  
AOC2-05

|          |       |       |       |
|----------|-------|-------|-------|
| Tot Ion: | 41    | Resp: | 58346 |
| Ion      | Ratio | Lower | Upper |
| 41       | 100   |       |       |
| 39       | 61.8  | 48.6  | 73.0  |
| 67       | 0.0   | 59.8  | 89.8# |
| 52       | 5.4   | 24.8  | 37.2# |

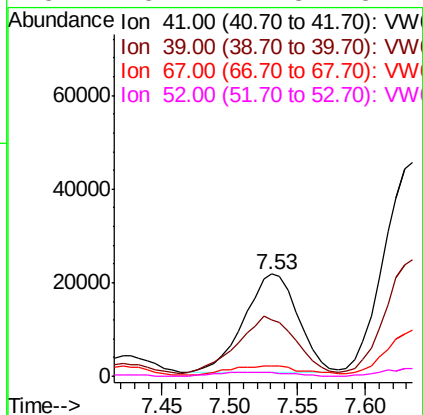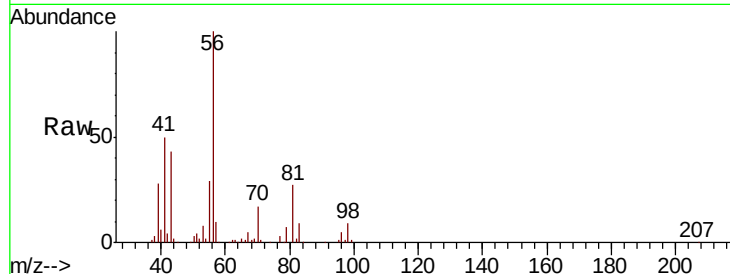


#42  
1,2-Dichloroethane  
Concen: 18.548 ug/l  
RT: 8.41 min Scan# 1067  
Delta R.T. 0.01 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 62    | Resp: | 20387 |
| Ion      | Ratio | Lower | Upper |
| 62       | 100   |       |       |
| 98       | 0.0   | 0.0   | 18.6  |







#43

Isopropyl Acetate

Concen: 226.385 ug/l

RT: 8.43 min Scan# 1071

Delta R.T. 0.01 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :

AOC2-05





Tot Ion: 43 Resp: 219253

Ion Ratio Lower Upper

43 100

61 0.0 26.1 39.1#

87 0.0 11.2 16.8#

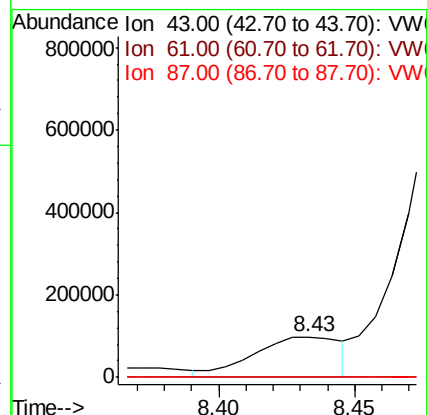

#45

1,2-Dichloropropane

Concen: 29.657 ug/l

RT: 9.34 min Scan# 1220

Delta R.T. -0.03 min

Lab File: VW007048.D




Acq: 26 Nov 2018 15:34


Tgt Ion: 63 Resp: 27677

Ion Ratio Lower Upper

63 100

65 209.0 24.4 36.6#

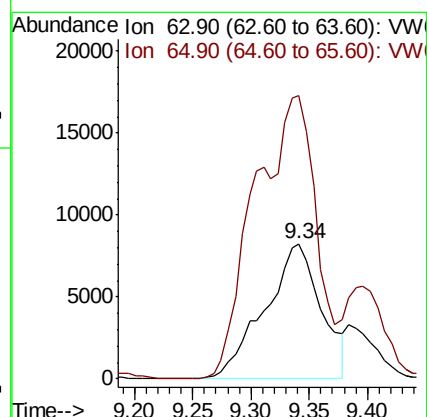



#46

Dibromomethane

Concen: 1.673 ug/l

RT: 9.48 min Scan# 1242

Delta R.T. 0.01 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :

AOC2-05





Tot Ion: 93 Resp: 782

Ion Ratio Lower Upper

93 100

95 1268.4 66.1 99.1#

174 0.0 79.7 119.5#

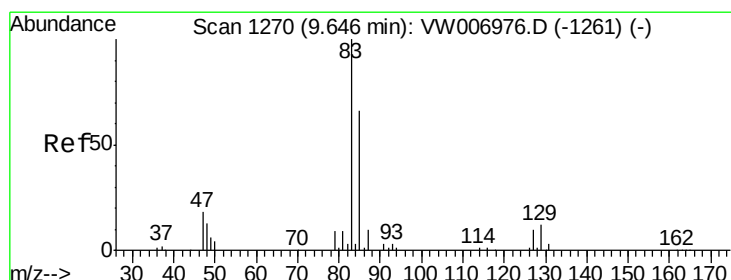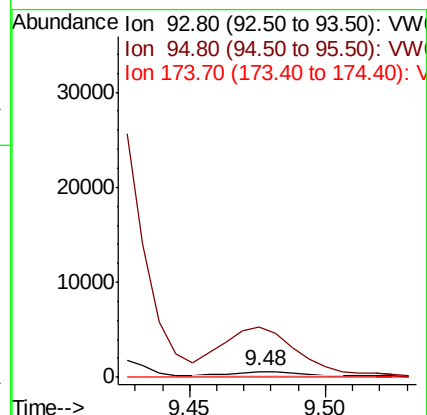

#47

Bromodichloromethane

Concen: 111.356 ug/l

RT: 9.63 min Scan# 1267

Delta R.T. -0.02 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34




Tgt Ion: 83 Resp: 137113


Ion Ratio Lower Upper

83 100

85 0.8 52.9 79.3#

127 0.0 7.8 11.6#



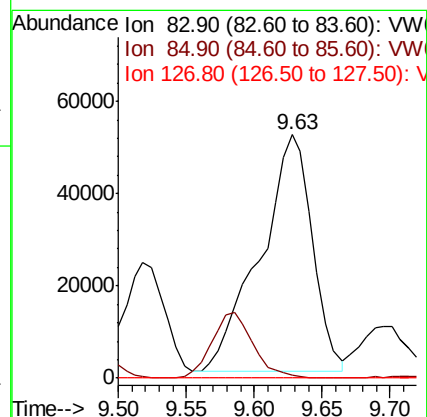
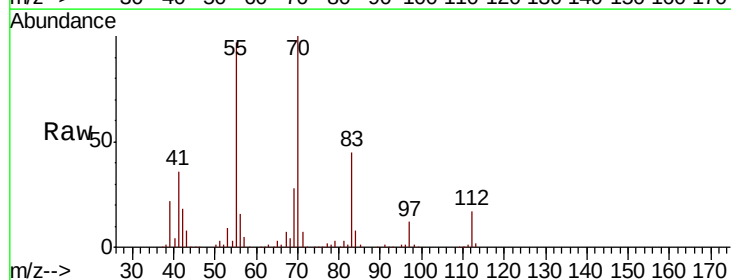




#48  
Methyl methacrylate  
Concen: 647.077 ug/l  
RT: 9.48 min Scan# 1242  
Delta R.T. 0.04 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34




Instrument :  
MSVOA\_W  
ClientSampleId :  
AOC2-05


Tot Ion: 41 Resp: 302177  
Ion Ratio Lower Upper  
41 100  
69 0.0 71.4 107.0#  
39 30.0 44.8 67.2#

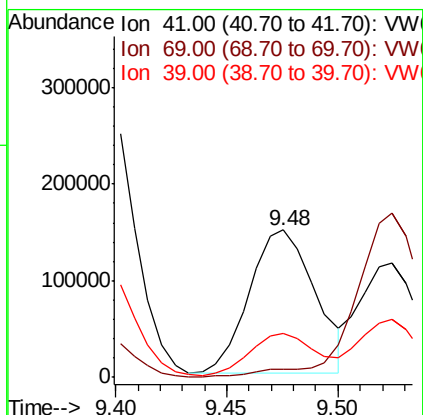

#50  
Toluene-d8  
Concen: 66.626 ug/l  
RT: 10.34 min Scan# 1383  
Delta R.T. 0.01 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34

Tgt Ion: 98 Resp: 238455  
Ion Ratio Lower Upper  
98 100  
100 52.1 52.2 78.2#









#51  
 4-Methyl-2-Pentanone  
 Concen: 1708.902 ug/l  
 RT: 10.27 min Scan# 1373  
 Delta R.T. 0.06 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34




Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 AOC2-05


Tot Ion: 43 Resp: 836399  
 Ion Ratio Lower Upper  
 43 100  
 58 26.8 31.8 47.6#

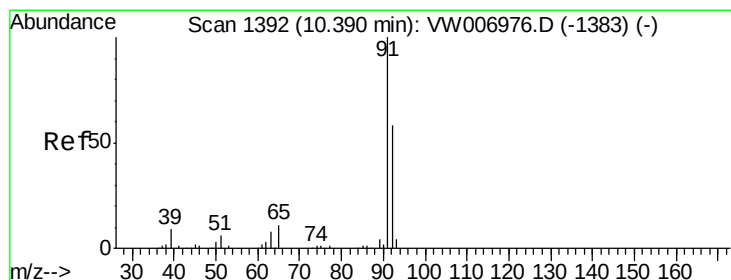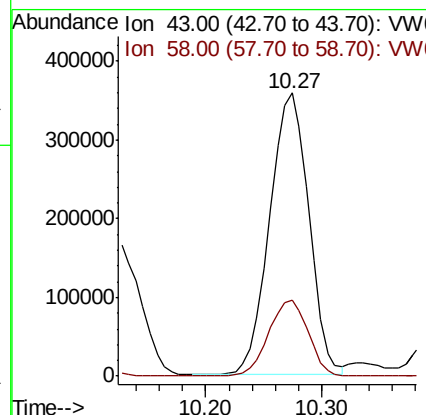

#52  
 Toluene  
 Concen: 8124.148 ug/l  
 RT: 10.40 min Scan# 1394  
 Delta R.T. 0.01 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34

Tgt Ion: 92 Resp: 20931023  
 Ion Ratio Lower Upper  
 92 100  
 91 0.0 137.3 205.9#

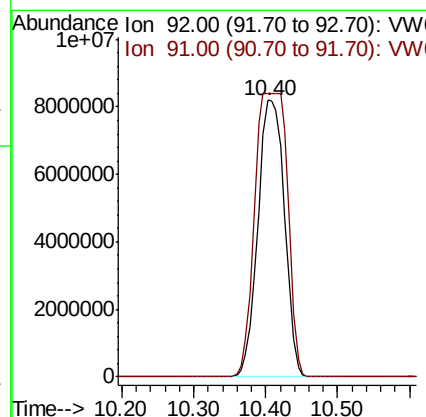

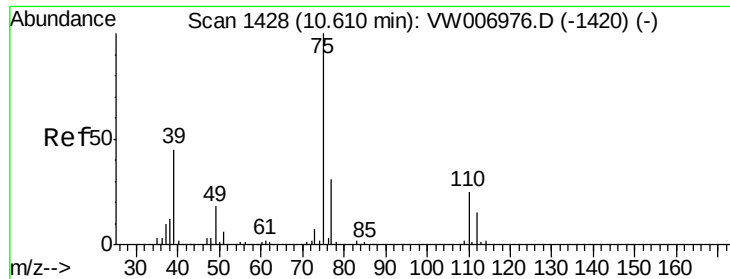

#53

t-1,3-Dichloropropene

Concen: 241.455 ug/l

RT: 10.40 min Scan# 1394

Delta R.T. -0.21 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :


AOC2-05

Tot Ion: 75 Resp: 288004

Ion Ratio Lower Upper

75 100

77 161.9 24.7 37.1#



Abundance Ion 74.90 (74.60 to 75.60): VW

Ion 76.90 (76.60 to 77.60): VW

200000

150000



100000

50000

0

10.30 10.40 10.50

Time-->

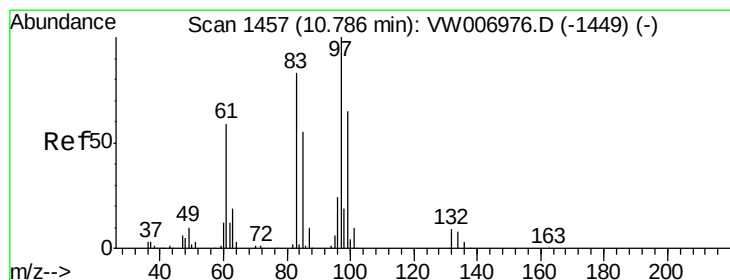

#55

1,1,2-Trichloroethane

Concen: 484.408 ug/l

RT: 10.77 min Scan# 1454

Delta R.T. -0.02 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Tgt Ion: 97 Resp: 333071


Ion Ratio Lower Upper

97 100

83 10.0 66.4 99.6#

85 85.2 44.1 66.1#

99 0.4 51.7 77.5#



Abundance Ion 96.90 (96.60 to 97.60): VW

Ion 82.90 (82.60 to 83.60): VW

Ion 84.90 (84.60 to 85.60): VW

Ion 98.90 (98.60 to 99.60): VW

300000


200000


100000

0

10.70 10.75 10.80

Time-->









#56  
Ethyl methacrylate  
Concen: 47.993 ug/l  
RT: 10.63 min Scan# 1431  
Delta R.T. -0.02 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34




Instrument :  
MSVOA\_W  
ClientSampled :  
AOC2-05


Tot Ion: 69 Resp: 38305  
Ion Ratio Lower Upper  
69 100  
41 135.4 53.4 80.0#  
39 0.0 28.2 42.4#

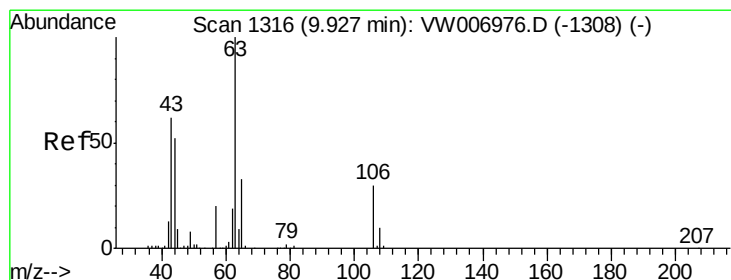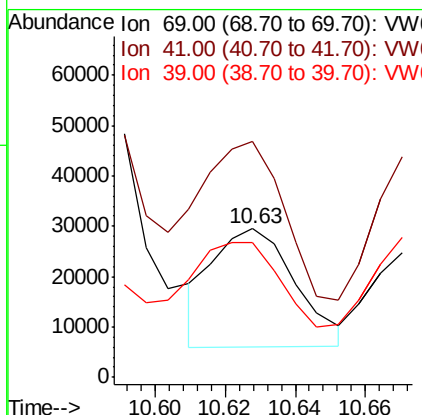

#58  
2-Chloroethyl Vinyl ether  
Concen: 59.952 ug/l  
RT: 9.91 min Scan# 1313  
Delta R.T. -0.02 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34

Tgt Ion: 63 Resp: 25004  
Ion Ratio Lower Upper  
63 100  
106 0.0 23.5 35.3#

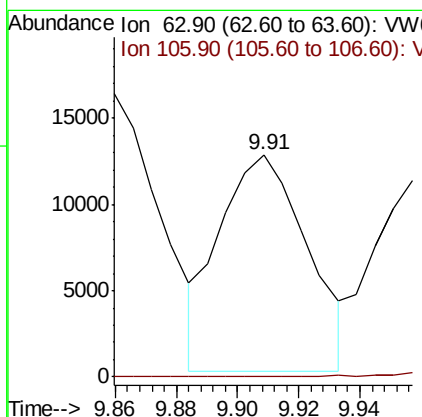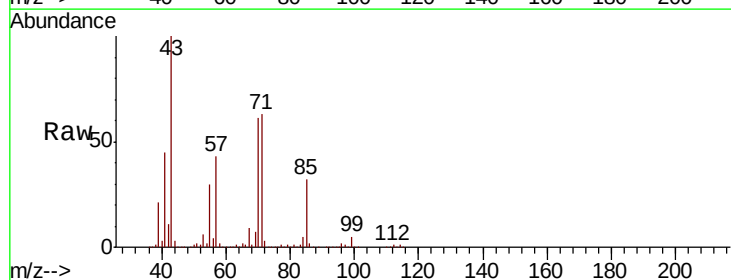

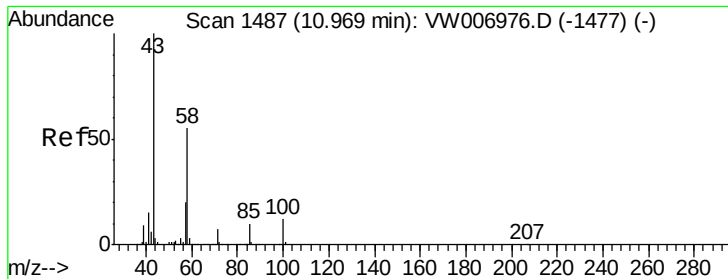

#59

2-Hexanone

Concen: 625.441 ug/l

RT: 10.94 min Scan# 1482

Delta R.T. -0.03 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampled :





AOC2-05

Tot Ion: 43 Resp: 209624

Ion Ratio Lower Upper

43 100

58 3.9 27.3 81.8#

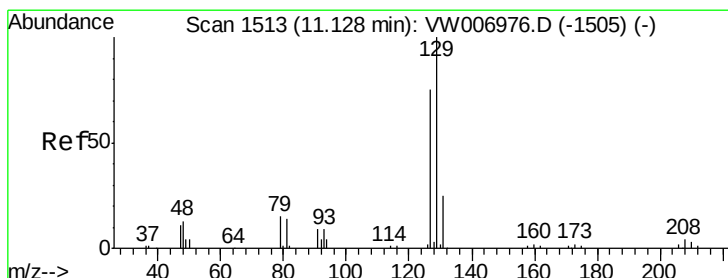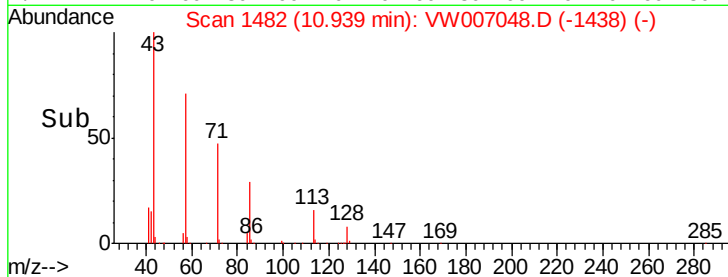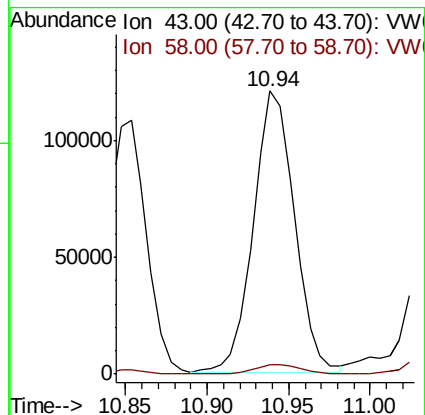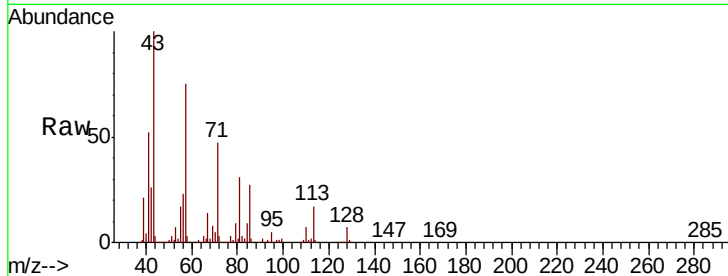

#60

Dibromochloromethane

Concen: 2.029 ug/l

RT: 11.04 min Scan# 1499

Delta R.T. -0.09 min

Lab File: VW007048.D




Acq: 26 Nov 2018 15:34


Tgt Ion: 129 Resp: 1590

Ion Ratio Lower Upper

129 100

127 58.7 38.3 114.8

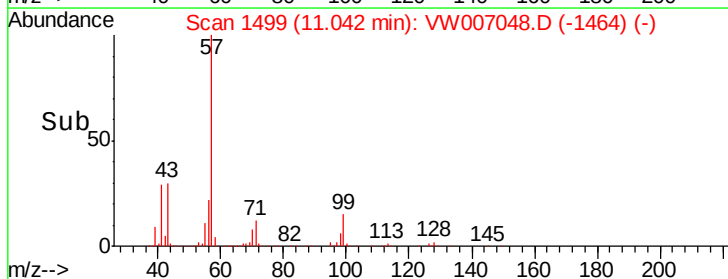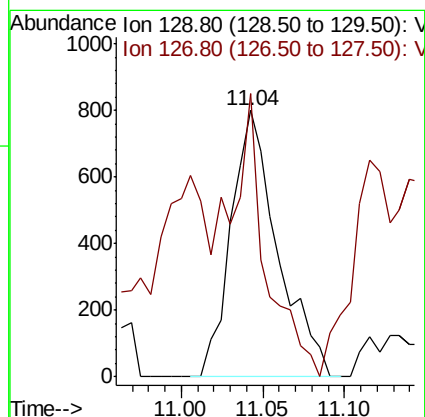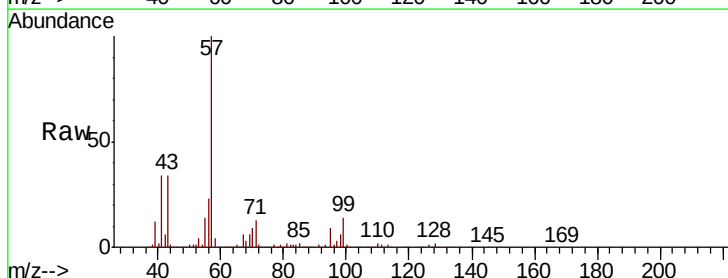



#61

1,2-Dibromoethane

Concen: 162.311 ug/l

RT: 11.24 min Scan# 1531

Delta R.T. -0.00 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampled :


AOC2-05

Tot Ion:107 Resp: 102092

Ion Ratio Lower Upper




107 100

109 103.7 75.1 112.7



Abundance Ion 106.90 (106.60 to 107.60): V

Ion 108.80 (108.50 to 109.50): V

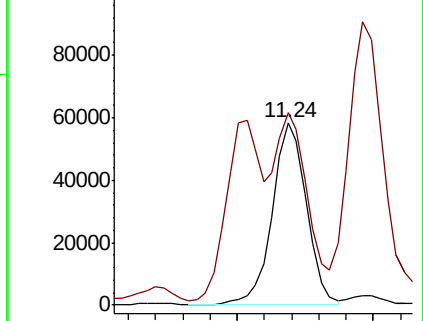

#62

4-Bromofluorobenzene

Concen: 76.338 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. -0.00 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34


Tgt Ion: 95 Resp: 107514

Ion Ratio Lower Upper

95 100

174 48.8 0.0 143.6



176 47.5 0.0 140.4




Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

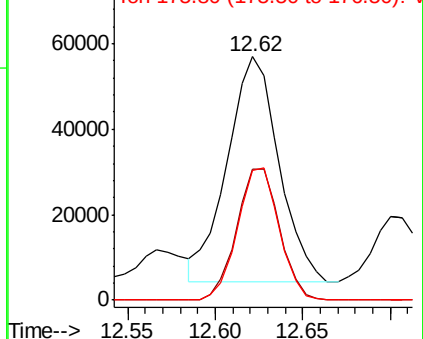









#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.63 min Scan# 1596  
Delta R.T. -0.00 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34




Instrument :  
MSVOA\_W  
ClientSampled :  
AOC2-05


Tot Ion:117 Resp: 145008  
Ion Ratio Lower Upper  
117 100  
82 58.6 44.2 66.2  
119 31.7 25.9 38.9



#67  
Ethyl Benzene  
Concen: 1693.603 ug/l  
RT: 11.74 min Scan# 1613  
Delta R.T. 0.01 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34

Tgt Ion: 91 Resp: 9416289  
Ion Ratio Lower Upper  
91 100  
106 31.3 25.4 38.2









#68  
m/p-Xylenes  
Concen: 4472.518 ug/l  
RT: 11.85 min Scan# 1631  
Delta R.T. 0.01 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34




Instrument :  
MSVOA\_W  
ClientSampleId :  
AOC2-05


Tot Ion:106 Resp: 9756028  
Ion Ratio Lower Upper  
106 100  
91 196.7 164.8 247.2

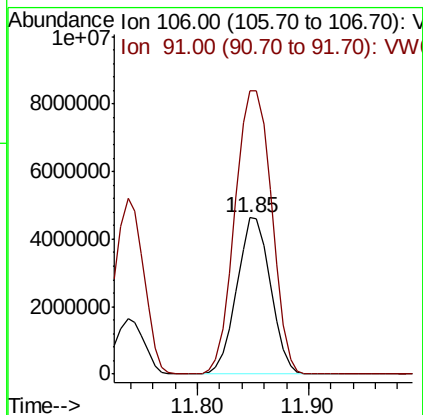

#69  
o-Xylene  
Concen: 2060.988 ug/l  
RT: 12.18 min Scan# 1685  
Delta R.T. 0.01 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34

Tgt Ion:106 Resp: 4239077  
Ion Ratio Lower Upper  
106 100  
91 224.0 107.9 323.8





#70

Stvrene

Concen: 71.657 ug/l

RT: 12.18 min Scan# 1685

Delta R.T. -0.01 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampled :

AOC2-05


Tot Ion:104 Resp: 234574

Ion Ratio Lower Upper

104 100

78 310.7 41.8 62.8#




103 259.9 44.4 66.6#



Abundance Ion 104.00 (103.70 to 104.70): V

Ion 78.00 (77.70 to 78.70): VW

Ion 103.00 (102.70 to 103.70): V

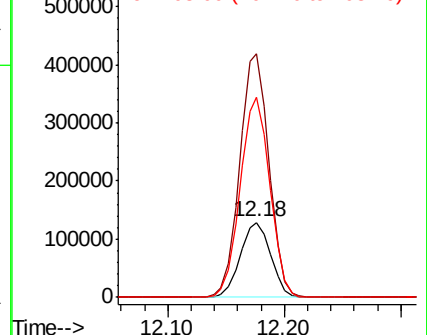

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.57 min Scan# 1913

Delta R.T. 0.01 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34


Tgt Ion:152 Resp: 70441

Ion Ratio Lower Upper

152 100

115 0.0 31.4 94.2#



150 154.7 0.0 353.4




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

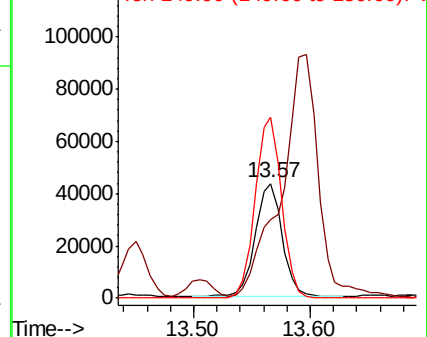

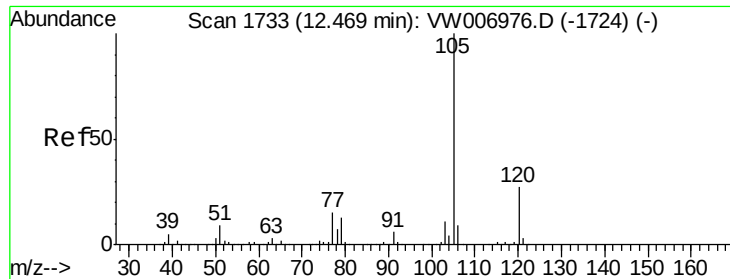

#73

Isopropylbenzene

Concen: 178.773 ug/l

RT: 12.47 min Scan# 1733

Delta R.T. -0.00 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :


AOC2-05

Tot Ion:105 Resp: 978710

Ion Ratio Lower Upper




105 100

120 26.1 13.3 39.8



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

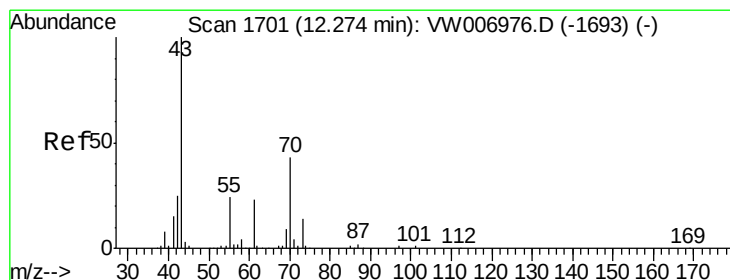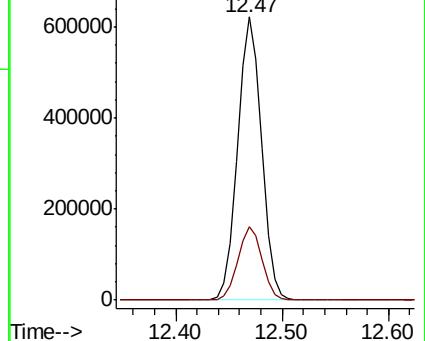

#74

N-ethyl acetate

Concen: 138.515 ug/l

RT: 12.26 min Scan# 1698

Delta R.T. -0.02 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Tgt Ion: 43 Resp: 127092


Ion Ratio Lower Upper

43 100

70 21.0 34.0 51.0#

55 0.0 19.4 29.0#

61 0.0 19.4 29.2#






Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 70.00 (69.70 to 70.70): VW

Ion 55.00 (54.70 to 55.70): VW

Ion 61.00 (60.70 to 61.70): VW

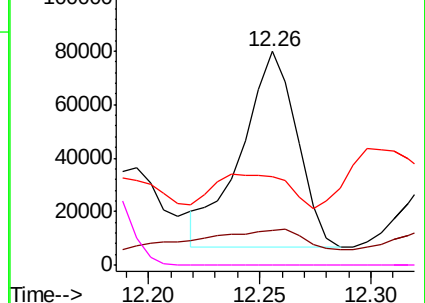



#75

1,1,2,2-Tetrachloroethane

Concen: 11.026 ug/l

RT: 12.71 min Scan# 1772

Delta R.T. -0.01 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :

AOC2-05





Tot Ion: 83 Resp: 8033

Ion Ratio Lower Upper

83 100

131 0.0 5.7 17.1#

85 434.2 33.1 99.2#



#76

1,2,3-Trichloropropane

Concen: 51.416 ug/l

RT: 12.81 min Scan# 1789

Delta R.T. 0.04 min

Lab File: VW007048.D




Acq: 26 Nov 2018 15:34


Tgt Ion: 75 Resp: 28460

Ion Ratio Lower Upper

75 100

77 648.2 0.0 0.0#





#78

n-propylbenzene

Concen: 645.270 ug/l

RT: 12.81 min Scan# 1789

Delta R.T. -0.00 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :





AOC2-05

Tot Ion: 91 Resp: 4279030

Ion Ratio Lower Upper

91 100

120 23.1 11.7 35.1

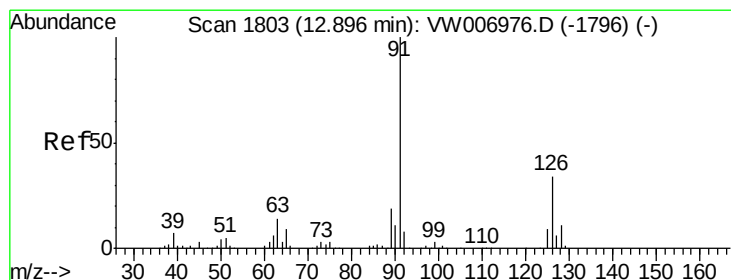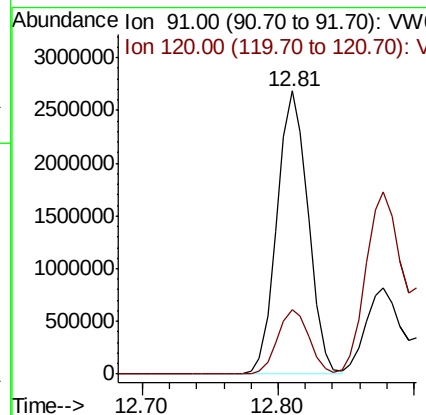

#79

2-Chlorotoluene

Concen: 377.331 ug/l

RT: 12.88 min Scan# 1800

Delta R.T. -0.02 min

Lab File: VW007048.D




Acq: 26 Nov 2018 15:34


Tgt Ion: 91 Resp: 1442765

Ion Ratio Lower Upper

91 100

126 0.1 16.7 50.0#


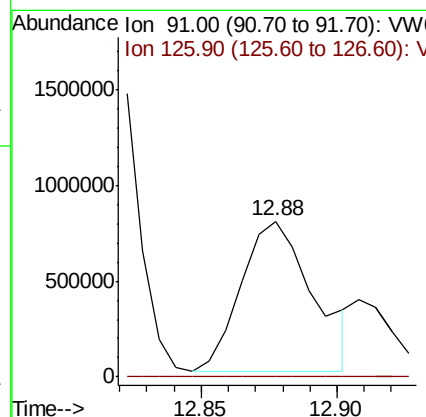






#80  
 1,3,5-Trimethylbenzene  
 Concen: 988.496 ug/l  
 RT: 12.95 min Scan# 1812  
 Delta R.T. -0.00 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34




Instrument :  
 MSVOA\_W  
 ClientSampled :  
 AOC2-05


Tot Ion:105 Resp: 4679690  
 Ion Ratio Lower Upper  
 105 100  
 120 46.6 23.8 71.2

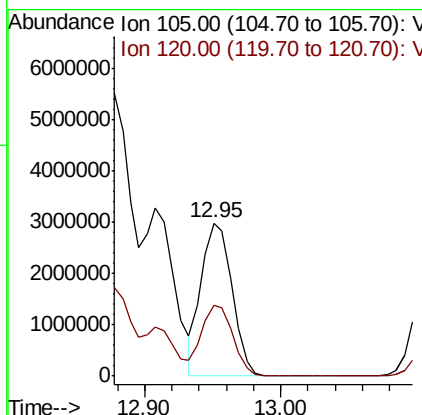

#81  
 trans-1,4-Dichloro-2-butene  
 Concen: 54.714 ug/l  
 RT: 12.47 min Scan# 1733  
 Delta R.T. -0.05 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34

Tgt Ion: 75 Resp: 12063  
 Ion Ratio Lower Upper  
 75 100  
 53 102.9 77.6 116.4  
 89 114.5 39.3 58.9#

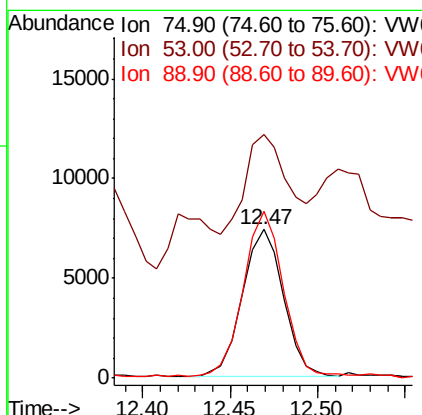



#82

4-Chlorotoluene

Concen: 131.004 ug/l

RT: 12.95 min Scan# 1812

Delta R.T. -0.04 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34

Instrument :

MSVOA\_W

ClientSampleId :





AOC2-05

Tot Ion: 91 Resp: 525653

Ion Ratio Lower Upper

91 100

126 0.5 16.6 49.7#

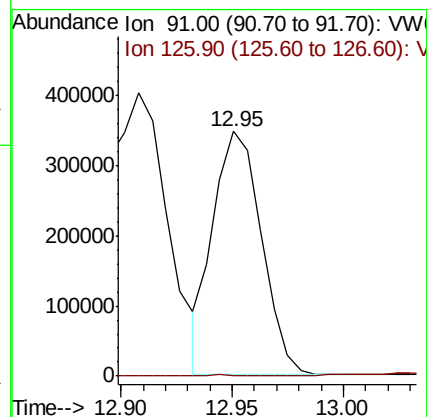

#83

tert-Butylbenzene

Concen: 400.104 ug/l

RT: 13.26 min Scan# 1863

Delta R.T. 0.05 min

Lab File: VW007048.D

Acq: 26 Nov 2018 15:34




Tgt Ion: 119 Resp: 1639917

Ion Ratio Lower Upper


119 100

91 96.2 33.5 100.5

134 0.0 12.6 37.8#

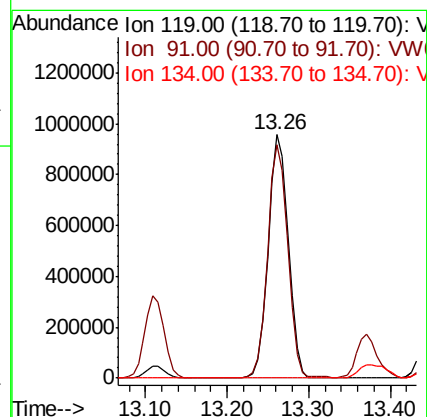









#84  
1,2,4-Trimethylbenzene  
Concen: 2750.876 ug/l  
RT: 13.26 min Scan# 1863  
Delta R.T. 0.01 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34




Instrument :  
MSVOA\_W  
ClientSampleId :  
AOC2-05


Tot Ion:105 Resp:12974980  
Ion Ratio Lower Upper  
105 100  
120 44.8 21.8 65.3

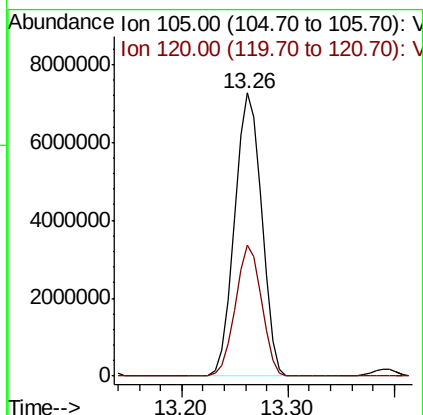

#85  
sec-Butylbenzene  
Concen: 2240.770 ug/l  
RT: 13.26 min Scan# 1863  
Delta R.T. -0.13 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34

Tgt Ion:105 Resp:12974980  
Ion Ratio Lower Upper  
105 100  
134 0.0 9.8 29.3#









#86  
 p-Isopropyltoluene  
 Concen: 84.733 ug/l  
 RT: 13.45 min Scan# 1894  
 Delta R.T. -0.05 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34




Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 AOC2-05


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 119     | 100   |       |       |
| 134     | 27.5  | 12.8  | 38.3  |
| 91      | 24.3  | 12.2  | 36.6  |

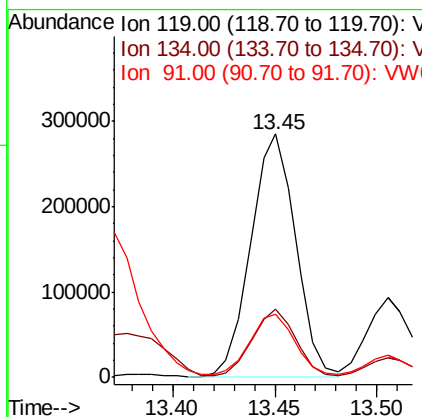

#89  
 n-Butylbenzene  
 Concen: 116.750 ug/l  
 RT: 13.83 min Scan# 1956  
 Delta R.T. -0.00 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 91      | 100   |       |       |
| 92      | 68.4  | 26.8  | 80.4  |
| 134     | 0.0   | 13.3  | 39.8# |



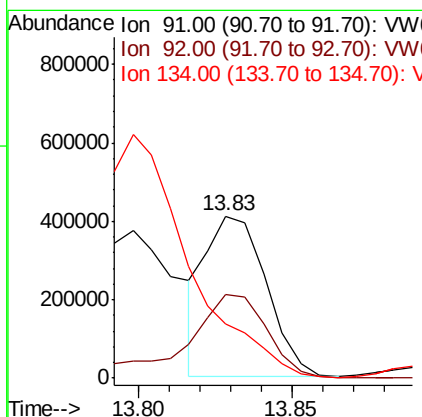



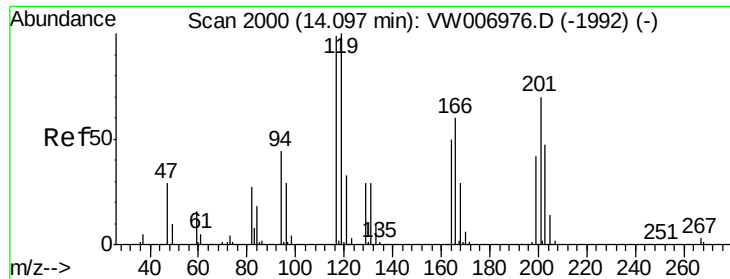

#90  
Hexachloroethane  
Concen: 335.426 ug/l  
RT: 14.10 min Scan# 2001  
Delta R.T. 0.01 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34




Instrument :  
MSVOA\_W  
ClientSampled :  
AOC2-05


Tot Ion:117 Resp: 250161  
Ion Ratio Lower Upper  
117 100  
201 0.0 35.9 107.5#



#92  
1,2-Dibromo-3-Chloropropane  
Concen: 37.164 ug/l  
RT: 14.51 min Scan# 2068  
Delta R.T. 0.02 min  
Lab File: VW007048.D  
Acq: 26 Nov 2018 15:34

Tgt Ion: 75 Resp: 4573  
Ion Ratio Lower Upper  
75 100  
155 11.5 42.6 127.8#  
157 0.0 55.0 165.0#









#93  
 1,2,4-Trichlorobenzene  
 Concen: 1.689 ug/l  
 RT: 15.14 min Scan# 2171  
 Delta R.T. -0.00 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 AOC2-05

Tot Ion:180 Resp: 2342  
 Ion Ratio Lower Upper  
 180 100  
 182 101.5 47.1 141.3  
 145 0.0 16.5 49.5#

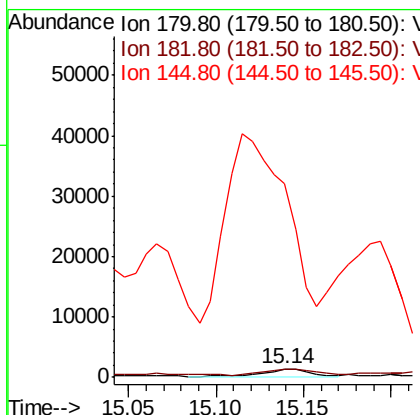

#95  
 Naphthalene  
 Concen: 739.183 ug/l  
 RT: 15.38 min Scan# 2210  
 Delta R.T. -0.00 min  
 Lab File: VW007048.D  
 Acq: 26 Nov 2018 15:34

Tgt Ion:128 Resp: 1861074  
 Ion Ratio Lower Upper  
 128 100  
 127 13.6 10.5 15.7  
 129 10.9 8.7 13.1

