


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW112618\
Data File : VW007062.D
Acq On : 26 Nov 2018 22:47
Operator : VAY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W112118S.M
Title : SW846 8260
Last Update : Wed Nov 21 03:23:02 2018

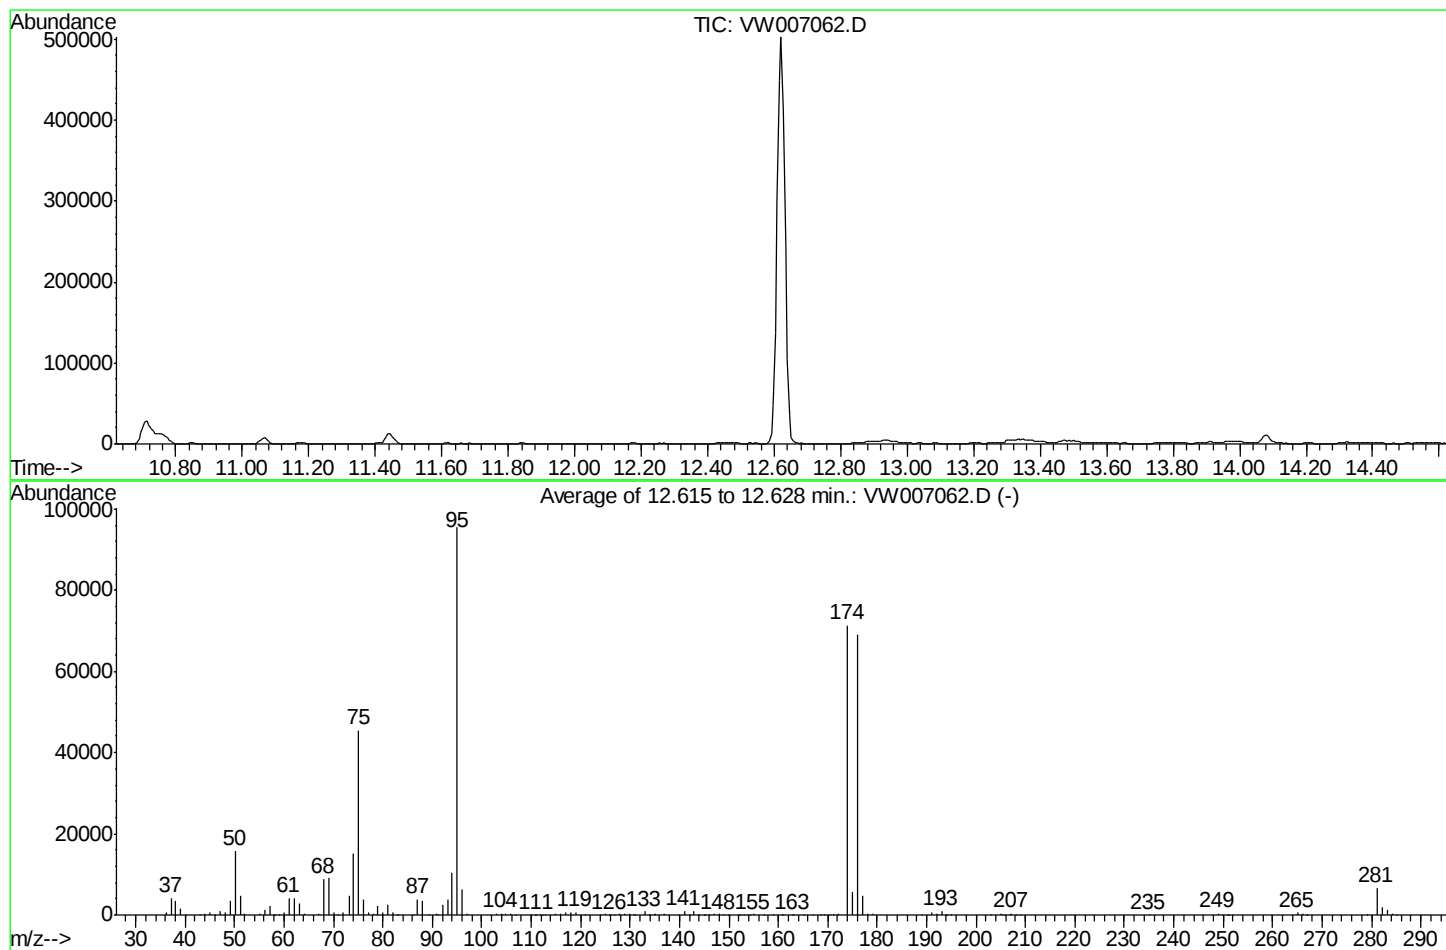

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	15830	PASS
75	95	30	60	47.7	45568	PASS
95	95	100	100	100.0	95501	PASS
96	95	5	9	6.5	6238	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.7	71304	PASS
175	174	5	9	8.1	5799	PASS
176	174	95	101	96.9	69112	PASS
177	176	5	9	7.0	4855	PASS