

Data File : VW014126.D
Acq On : 26 Nov 2019 11:11
Operator : SY/VA
Sample : K6007-03
Misc : 5.71G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BL1

Quant Time: Nov 27 07:07:09 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 27 06:15:20 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	292278	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	268399	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	118523	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	79361	17.02	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.08%
7) Chloroethane-d5	2.89	69	77821	20.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.32%
10) 1,1-Dichloroethene-d2	4.01	63	135322	14.14	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.56%
20) 2-Butanone-d5	7.07	46	70482	52.03	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.06%
24) Chloroform-d	7.64	84	217157	24.16	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.64%
26) 1,2-Dichloroethane-d4	8.30	65	116181	25.71	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.84%
29) Benzene-d6	8.27	84	442119	23.22	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.88%
33) 1,2-Dichloropropane-d6	9.27	67	140780	25.24	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.96%
37) Toluene-d8	10.32	98	392875	21.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.04%
38) trans-1,3-Dichloropropene-	10.57	79	49682	20.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.20%
39) 2-Hexanone-d5	10.92	63	52026	49.18	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.36%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	110525	26.24	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.96%
61) 1,2-Dichlorobenzene-d4	13.85	152	126676	26.60	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.40%


Target Compounds						Qvalue
59) 1,2,3-Trichloropropane	13.56	75	12524	4.096	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW014126.D
Acq On : 26 Nov 2019 11:11
Operator : SY/VA
Sample : K6007-03
Misc : 5.71G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BL1

Quant Time: Nov 27 07:07:09 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 27 06:15:20 2019
Response via : Initial Calibration

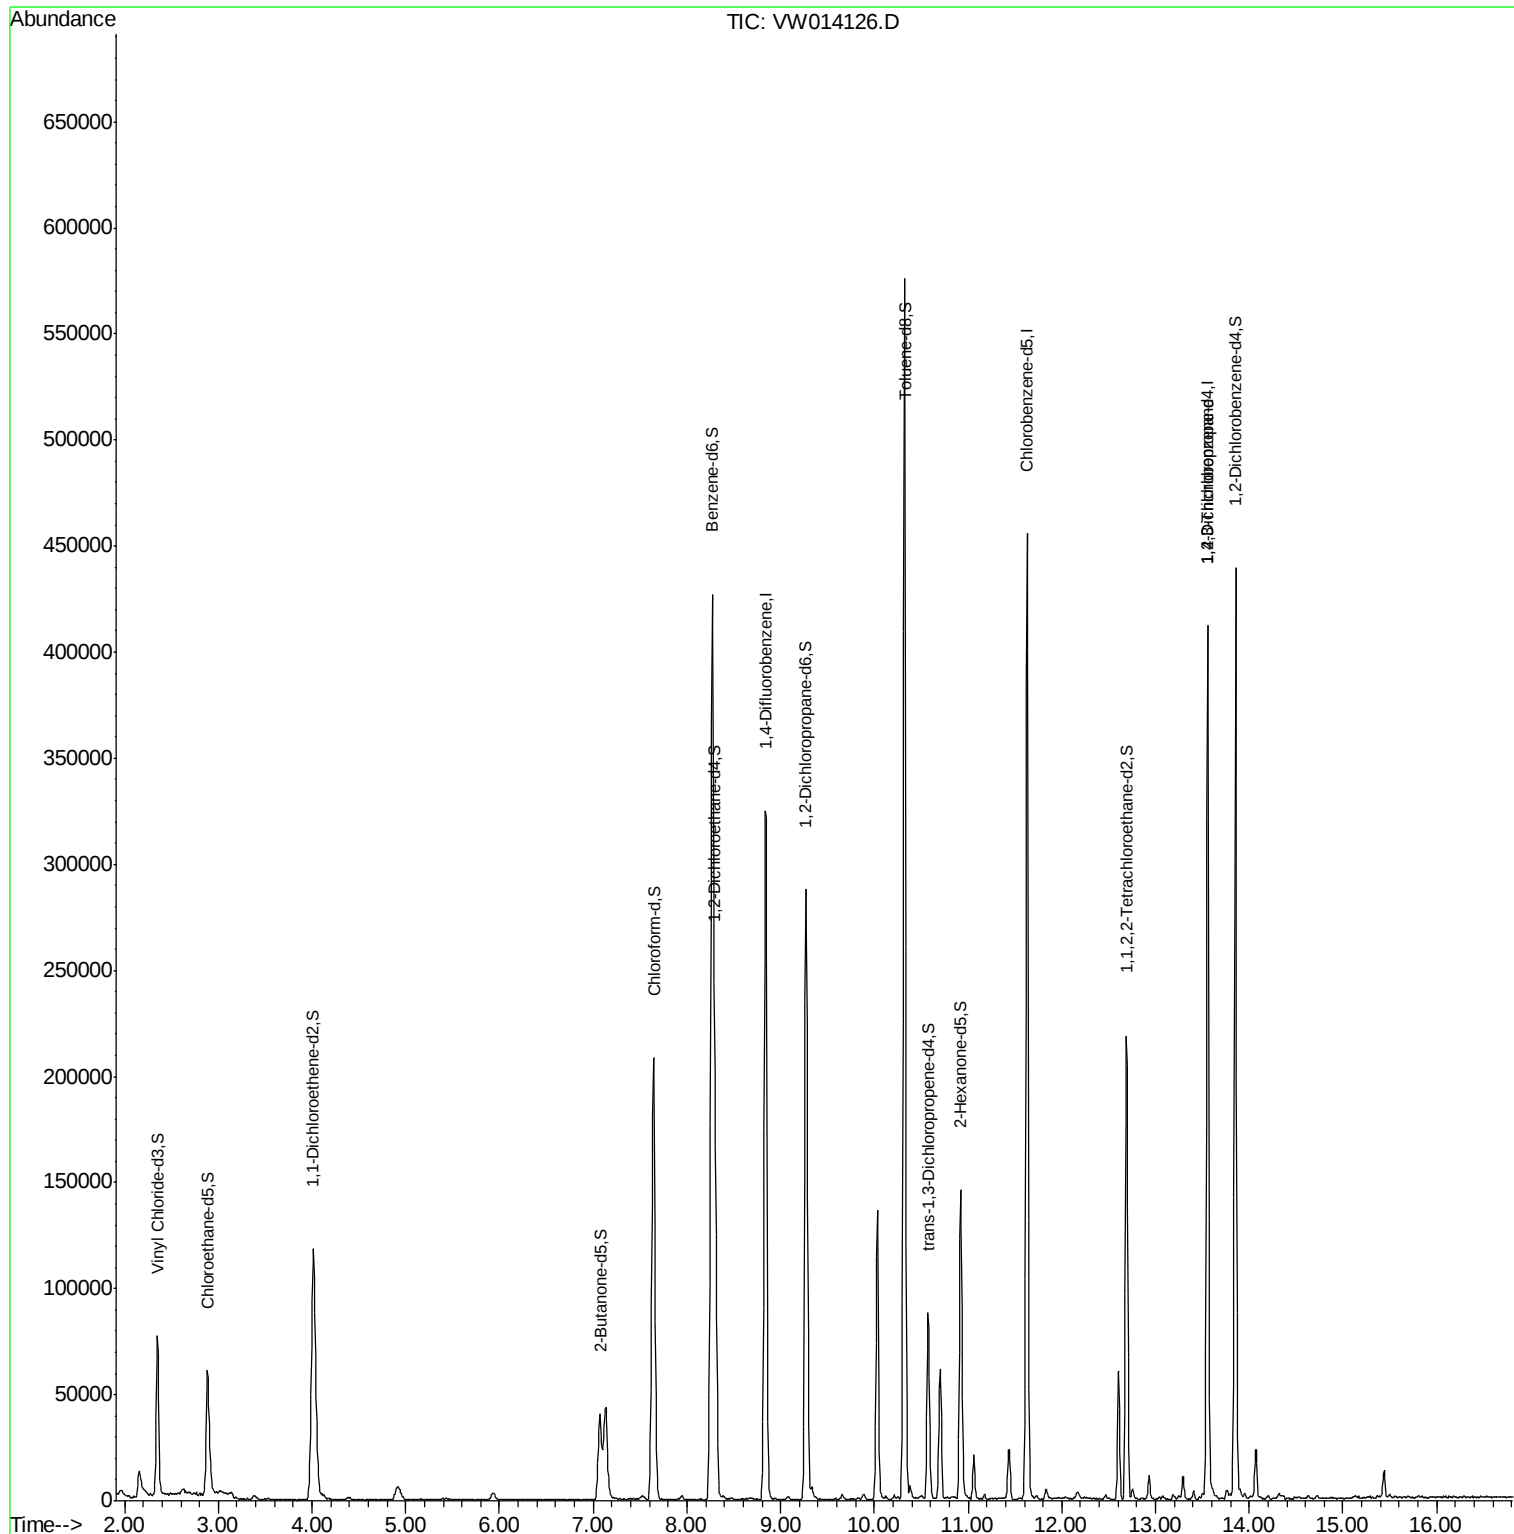

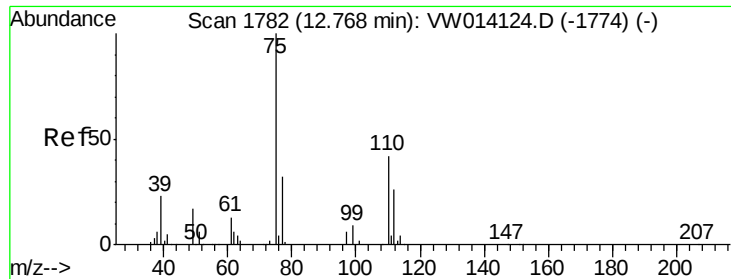

#59

1,2,3-Trichloropropane

Concen: 4.096 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW014126.D

Acq: 26 Nov 2019 11:11

Instrument :

MSVOA_W

ClientSampleId :

C0BL1

Tgt Ion: 75 Resp: 12524

Ion Ratio Lower Upper

75 100

77 35.9 25.9 38.9

