

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112619\
 Data File : VW014127.D
 Acq On : 26 Nov 2019 11:38
 Operator : SY/VA
 Sample : K6007-04RE
 Misc : 5.25G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BL2RE

Quant Time: Nov 27 07:31:33 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 27 06:15:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	273339	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	189240	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	46662	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	67258	15.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.68%
7) Chloroethane-d5	2.89	69	72507	20.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.04%
10) 1,1-Dichloroethene-d2	4.01	63	109694	12.26	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.04%
20) 2-Butanone-d5	7.07	46	67048	52.92	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.84%
24) Chloroform-d	7.65	84	207996	24.75	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.00%
26) 1,2-Dichloroethane-d4	8.31	65	98802	23.38	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.52%
29) Benzene-d6	8.27	84	413359	30.79	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	123.16%
33) 1,2-Dichloropropane-d6	9.27	67	137310	34.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	139.64%#
37) Toluene-d8	10.32	98	318801	25.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.16%
38) trans-1,3-Dichloropropene-	10.57	79	24816	14.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	58.92%
39) 2-Hexanone-d5	10.92	63	47432	63.59	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	127.18%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	103647	34.90	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	139.60%#
61) 1,2-Dichlorobenzene-d4	13.85	152	78154	41.69	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	166.76%#


Target Compounds					Ovalue
13) Acetone	4.12	43	7626	5.915 ug/L	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW112619\
Data File : VW014127.D
Acq On : 26 Nov 2019 11:38
Operator : SY/VA
Sample : K6007-04RE
Misc : 5.25G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BL2RE

Quant Time: Nov 27 07:31:33 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 27 06:15:20 2019
Response via : Initial Calibration

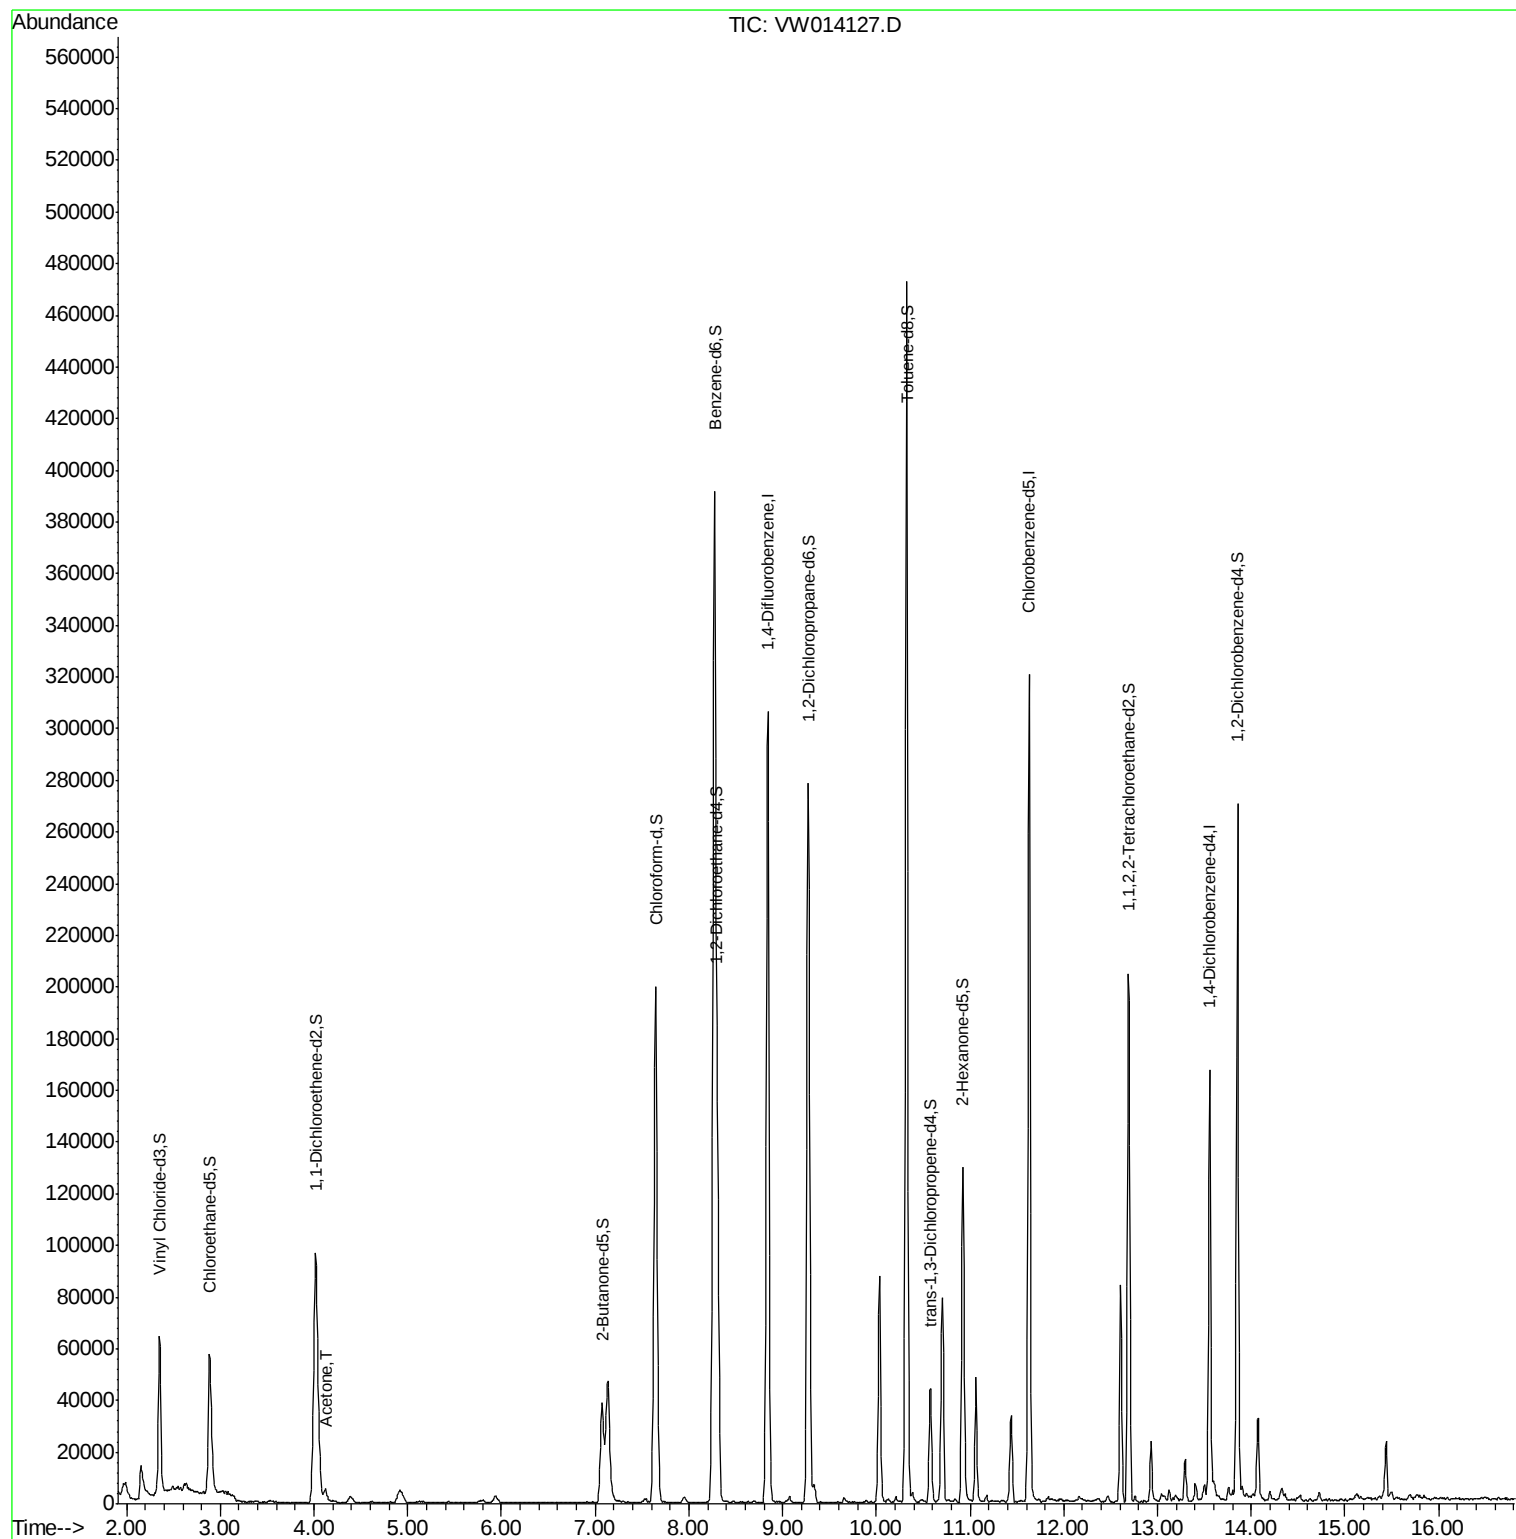

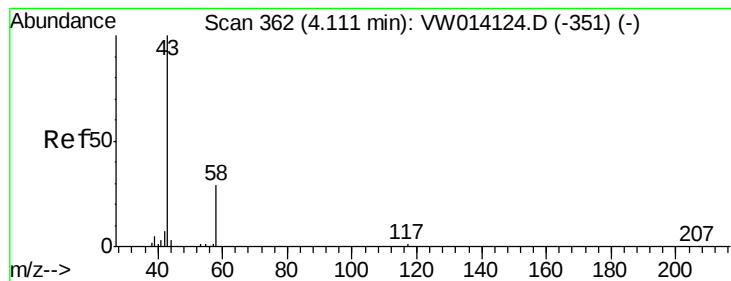

#13
 Acetone
 Concen: 5.915 ug/L
 RT: 4.12 min Scan# 364
 Delta R.T. 0.01 min
 Lab File: VW014127.D
 Acq: 26 Nov 2019 11:38

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BL2RE

Tot Ion: 43 Resp: 7626
 Ion Ratio Lower Upper
 43 100
 58 18.1 0.0 65.4

