


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
Data File : VW020961.D
Acq On : 26 Nov 2021 16:39
Operator : SY/VA
Sample : M4833-22
Misc : 5.87g/10.0mL/MSVOA_W/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
ESQN9

Quant Time: Nov 27 00:59:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 27 00:54:15 2021
Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 11/28/2021
Supervised By : Mahesh Dadoda 11/29/2021

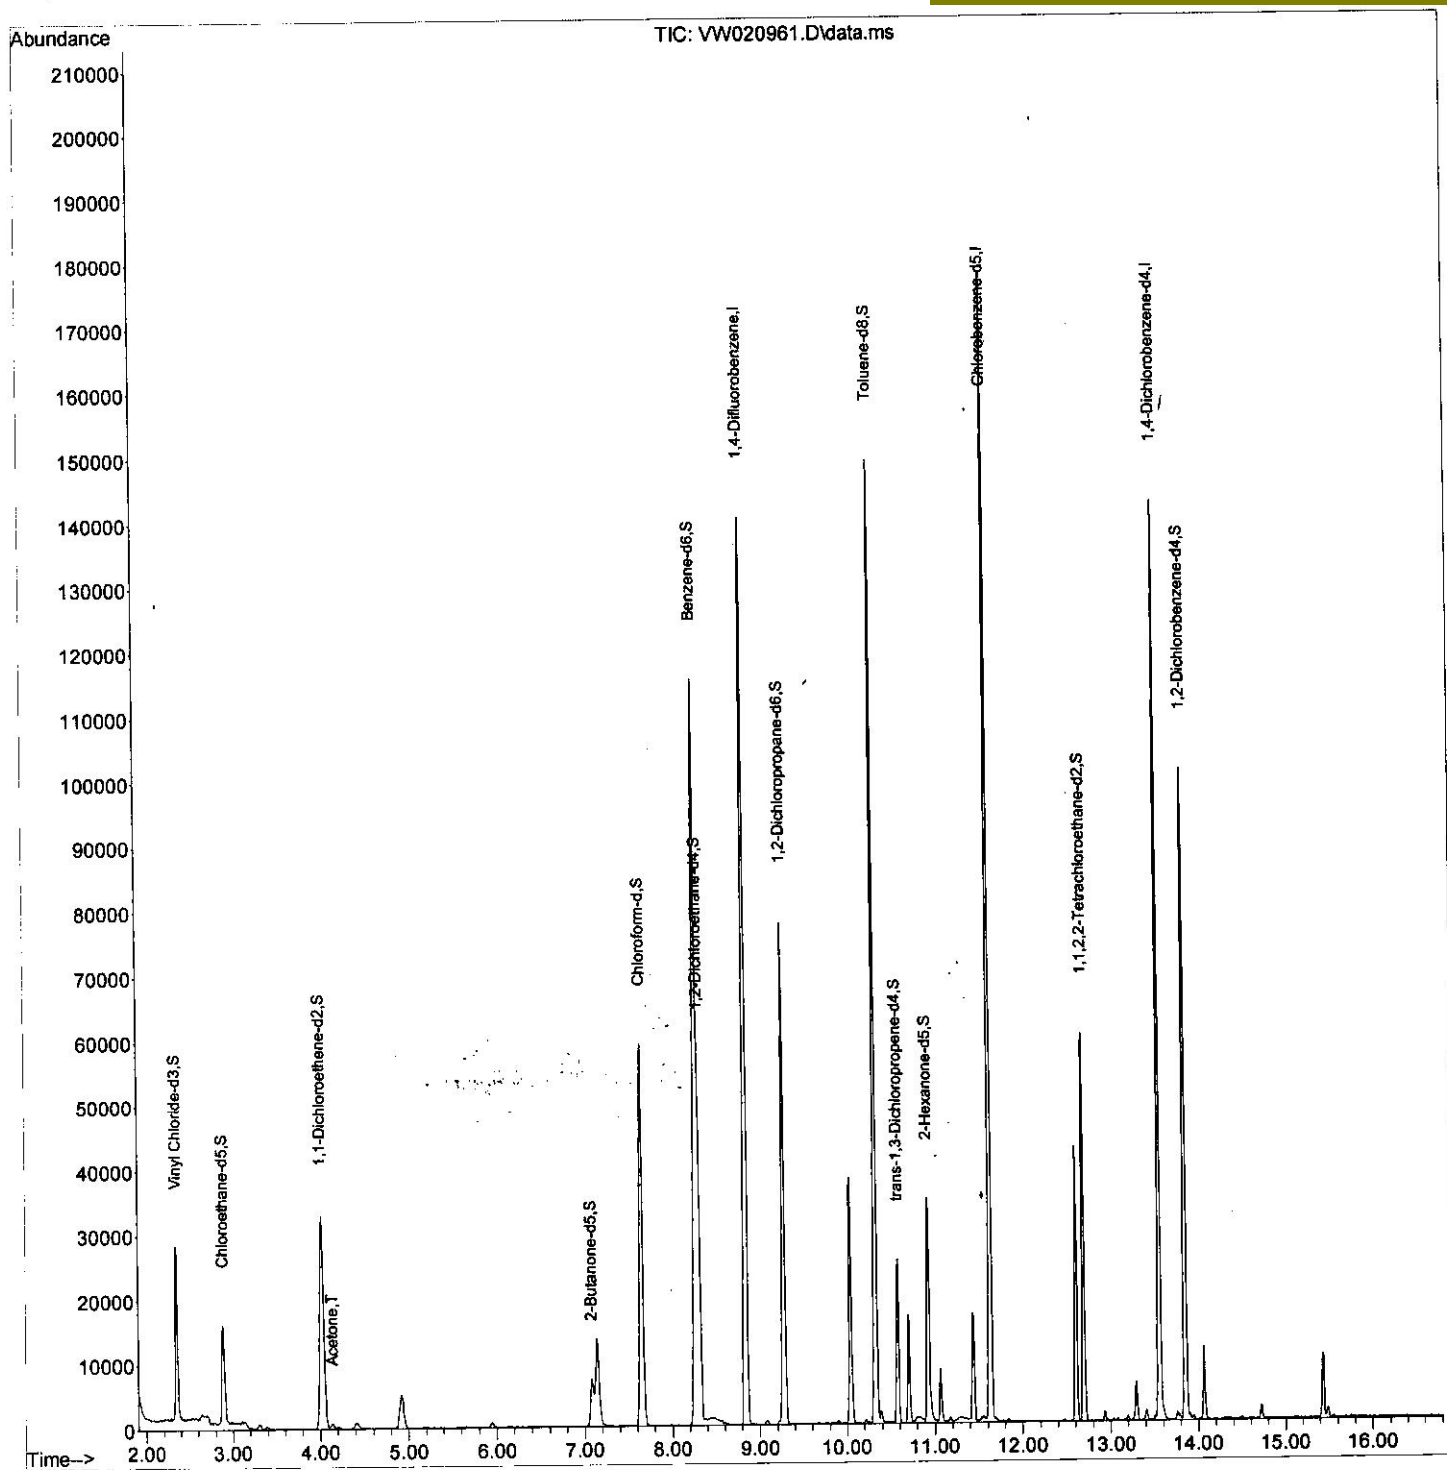

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
 Data File : VW020961.D
 Acq On : 26 Nov 2021 16:39
 Operator : SY/VA
 Sample : M4833-22
 Misc : 5.87g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 ESQN9

Quant Time: Nov 27 00:59:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 27 00:54:15 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 11/28/2021
 Supervised By : Mahesh Dadoda 11/29/2021

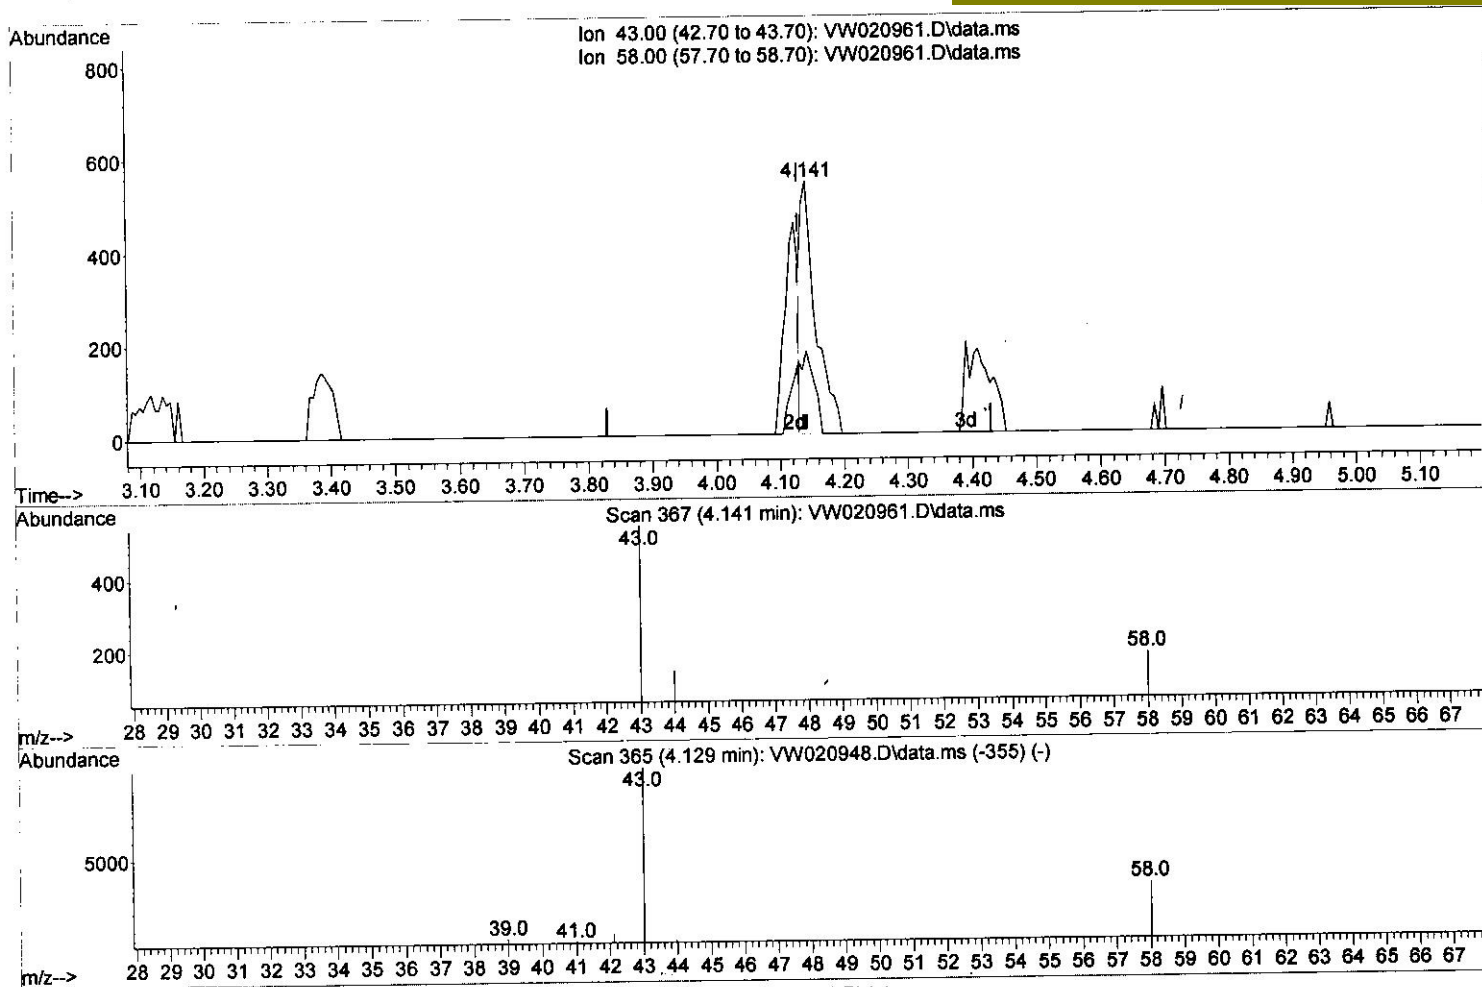

(13) Acetone (T)

4.141min (+ 0.012) 2.88 ug/L

response 902

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	43.90
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
 Data File : VW020961.D
 Acq On : 26 Nov 2021 16:39
 Operator : SY/VA
 Sample : M4833-22
 Misc : 5.87g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 ESQN9

Quant Time: Nov 27 00:59:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 27 00:54:15 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 11/28/2021
 Supervised By : Mahesh Dadoda 11/29/2021

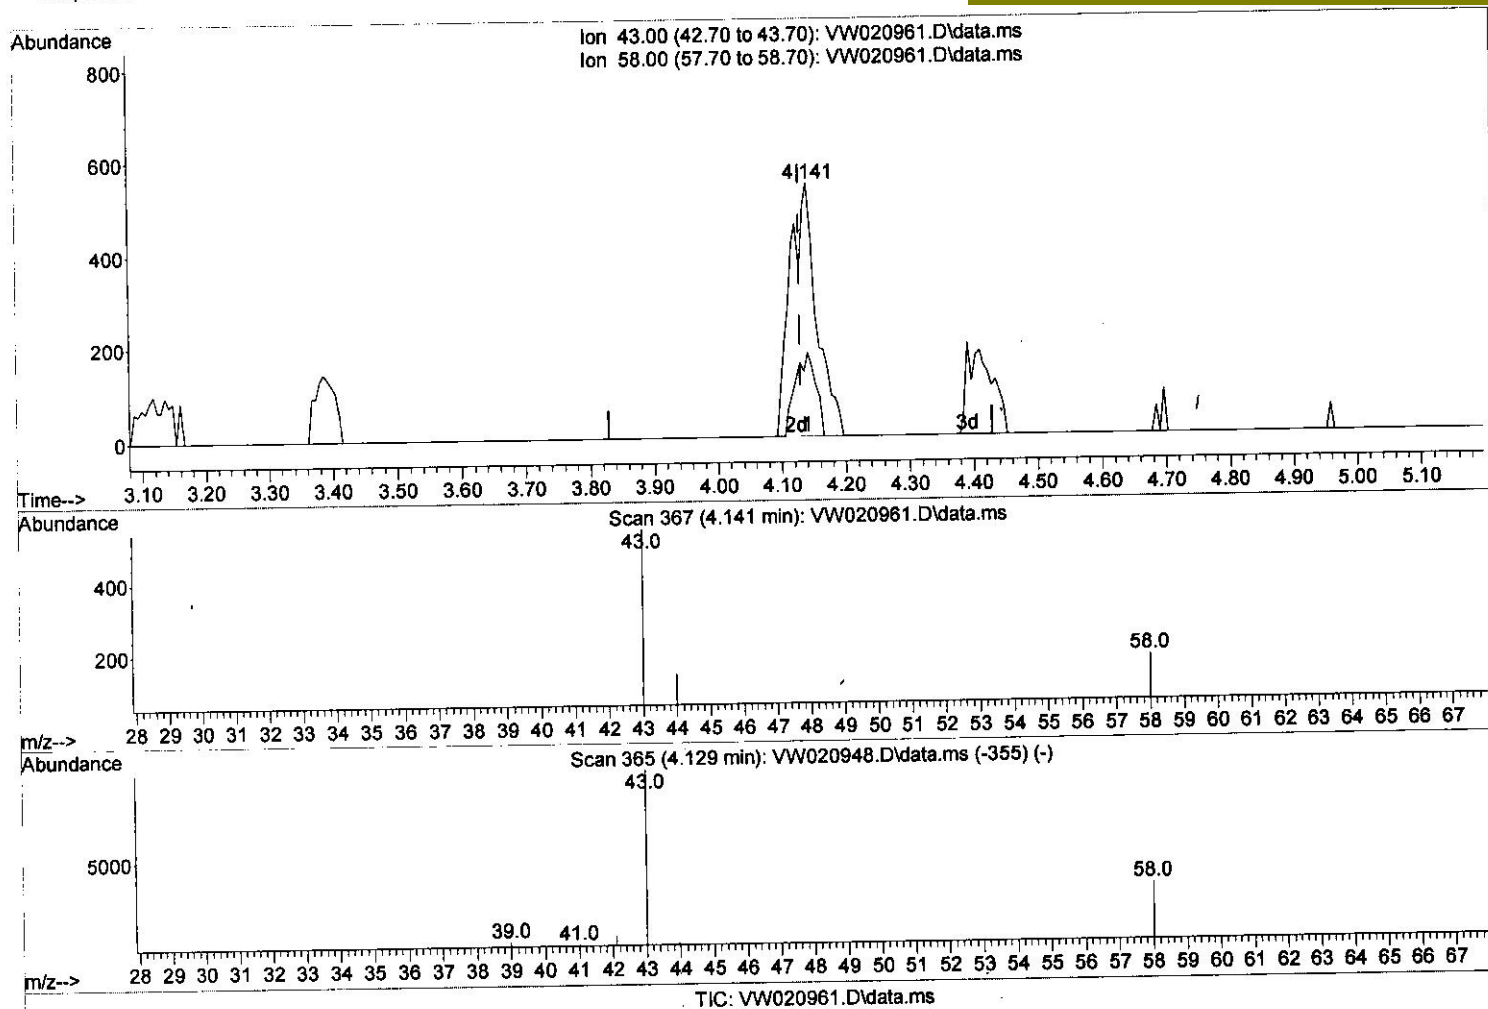

(13) Acetone (T)

4.141min (+ 0.012) 4.97 ug/L

response 1559

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	25.40
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
 Data File : VW020961.D
 Acq On : 26 Nov 2021 16:39
 Operator : SY/VA
 Sample : M4833-22
 Misc : 5.87g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 ESQN9

Quant Time: Nov 27 00:59:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 27 00:54:15 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 11/28/2021
 Supervised By : Mahesh Dadoda 11/29/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	121338	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.627	117	98979	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	36862	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	25439	18.074	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	72.280%	
7) Chloroethane-d5	2.885	69	17279	19.035	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	76.160%	
11) 1,1-Dichloroethene-d2	4.013	63	31127	11.430	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	45.720%	
21) 2-Butanone-d5	7.079	46	12666	36.055	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	72.100%	
24) Chloroform-d	7.652	84	59188	19.359	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	77.440%	
26) 1,2-Dichloroethane-d4	8.305	65	32826	21.153	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	84.600%	
32) Benzene-d6	8.274	84	106423	20.400	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	81.600%	
36) 1,2-Dichloropropane-d6	9.274	67	33243	22.378	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	89.520%	
41) Toluene-d8	10.323	98	97586	18.847	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	75.400%	
43) trans-1,3-Dichloroprop...	10.579	79	13303	18.946	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	75.800%	
47) 2-Hexanone-d5	10.920	63	11561	46.925	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	93.840%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	28472	25.020	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	100.080%	
66) 1,2-Dichlorobenzene-d4	13.853	152	26975	20.532	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	82.120%	

Target Compounds
 13) Acetone 4.141 43 1559m } 4.970 ug/L Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed