

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
 Data File : VW020955.D
 Acq On : 26 Nov 2021 14:14
 Operator : SY/VA
 Sample : M4833-13
 Misc : 6.21g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQN0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
 Supervised By :Mahesh Dadoda 11/29/2021

Quant Time: Nov 27 00:57:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 27 00:54:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	119710	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	100072	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	42573	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	25997	18.722	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.880%		
7) Chloroethane-d5	2.885	69	16588	18.523	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.080%		
11) 1,1-Dichloroethene-d2	4.013	63	31630	11.773	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	47.080%		
21) 2-Butanone-d5	7.080	46	15151	43.715	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	87.420%		
24) Chloroform-d	7.653	84	60957	20.209	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	80.840%		
26) 1,2-Dichloroethane-d4	8.305	65	33557	21.918	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	87.680%		
32) Benzene-d6	8.275	84	113474	21.515	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.040%		
36) 1,2-Dichloropropane-d6	9.274	67	34285	22.828	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.320%		
41) Toluene-d8	10.323	98	103359	19.744	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	78.960%		
43) trans-1,3-Dichloroprop...	10.579	79	14723	20.740	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	82.960%		
47) 2-Hexanone-d5	10.921	63	12742	51.153	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.300%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	28377	24.664	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	98.640%		
66) 1,2-Dichlorobenzene-d4	13.853	152	32421	21.367	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	85.480%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	1652m	5.339	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
Data File : VW020955.D
Acq On : 26 Nov 2021 14:14
Operator : SY/VA
Sample : M4833-13
Misc : 6.21g/10.0mL/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
ESQN0

Quant Time: Nov 27 00:57:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 27 00:54:15 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 11/28/2021
Supervised By :Mahesh Dadoda 11/29/2021

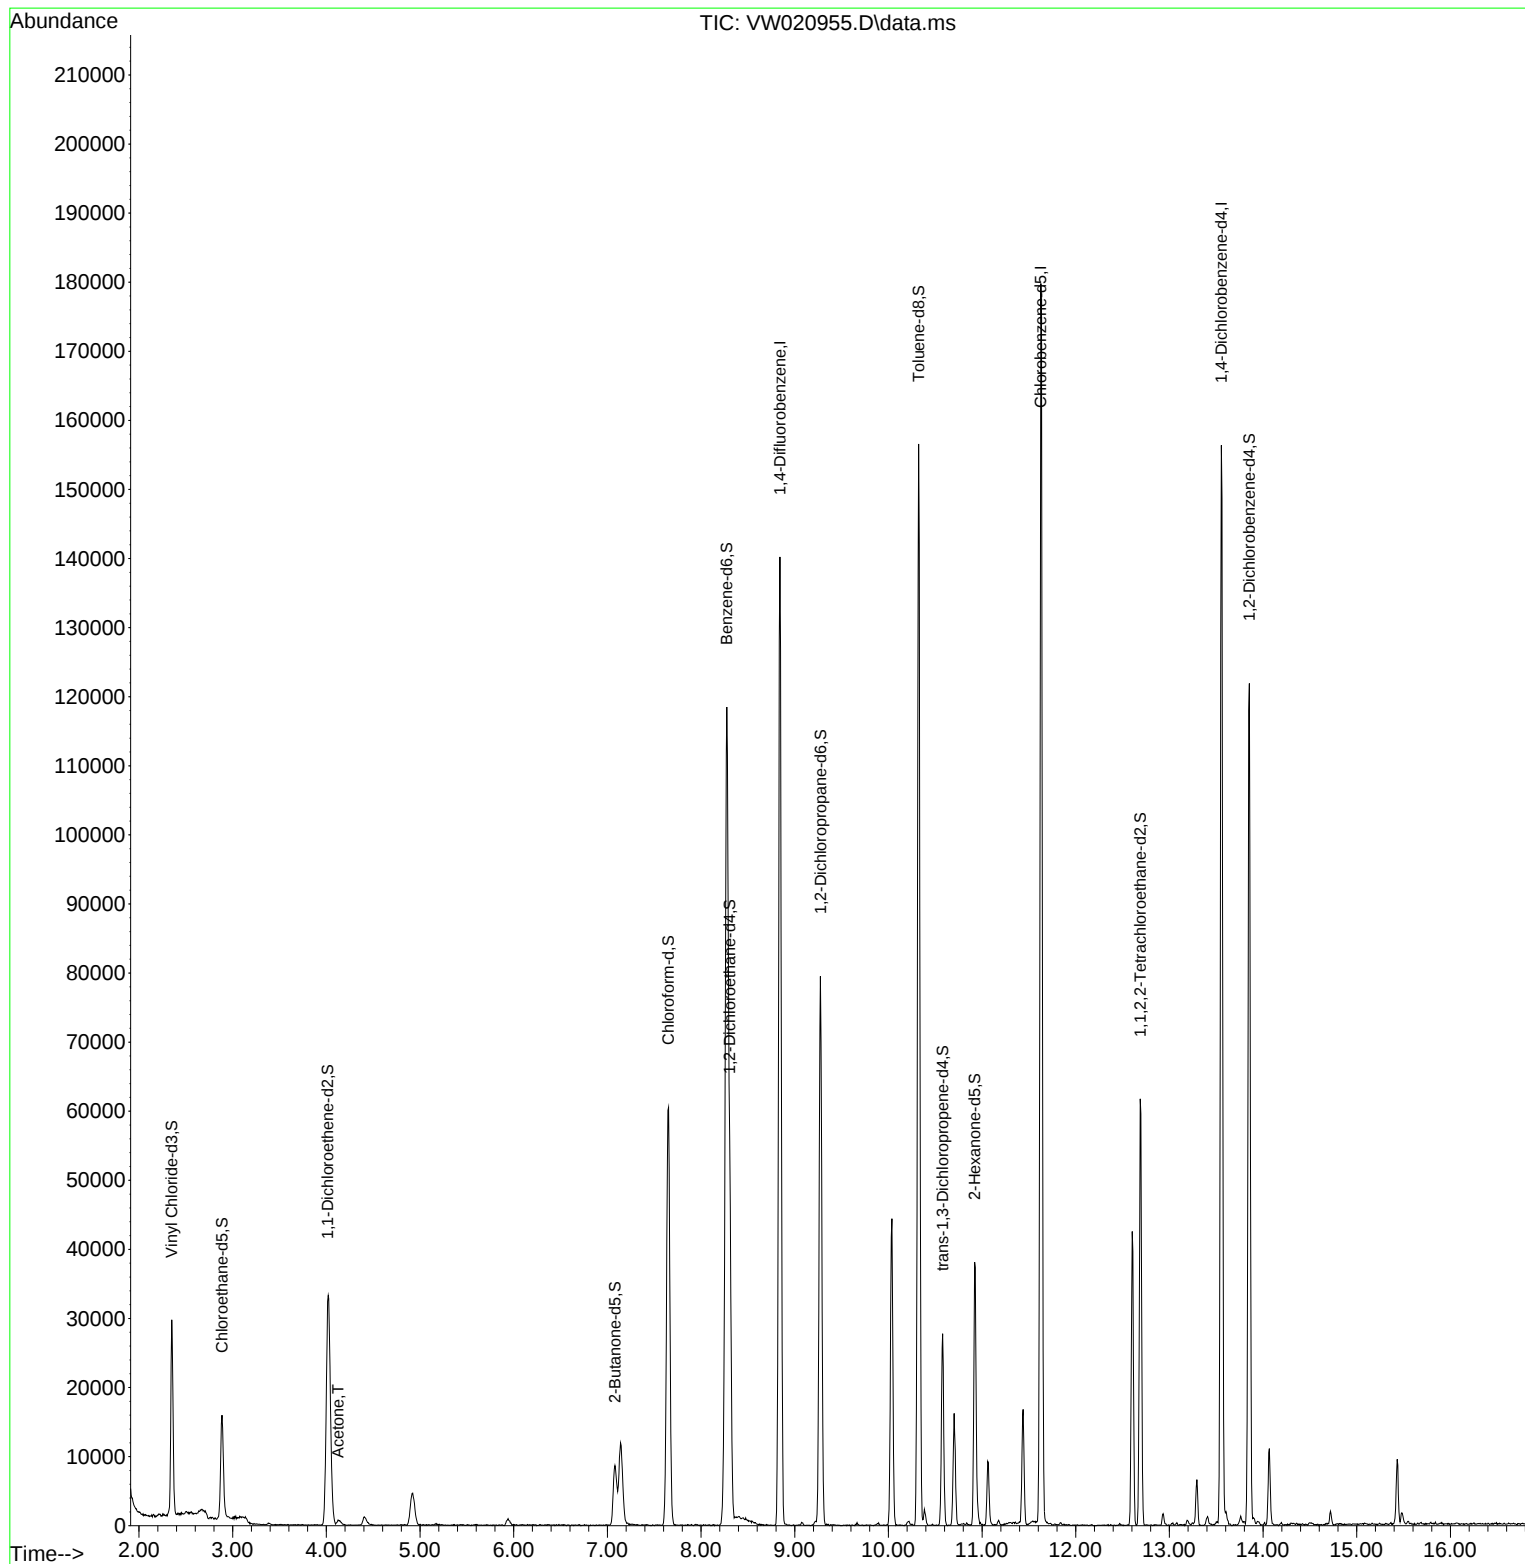

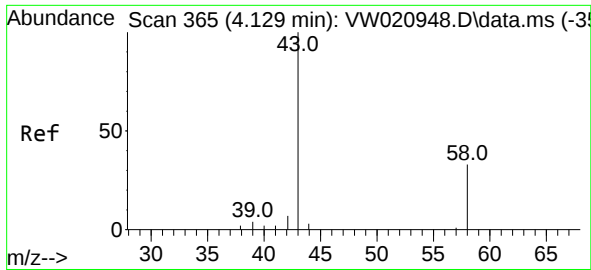

#13
 Acetone
 Concen: 5.339 ug/L m
 RT: 4.123 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW020955.D
 Acq: 26 Nov 2021 14:14

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQN0

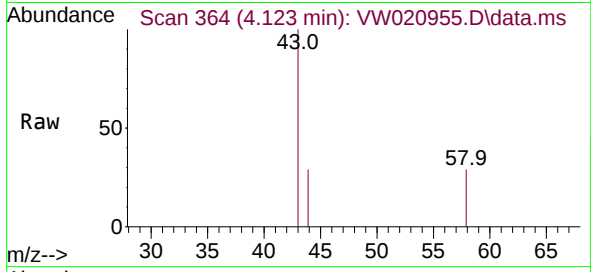

Tgt Ion: 43 Resp: 1652
 Ion Ratio Lower Upper
 43 100
 58 18.5 0.0 52.8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
 Supervised By :Mahesh Dadoda 11/29/2021

