

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
 Data File : VW020957.D
 Acq On : 26 Nov 2021 15:03
 Operator : SY/VA
 Sample : M4833-07
 Misc : 6.36g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQM7

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
 Supervised By :Mahesh Dadoda 11/29/2021

Quant Time: Nov 27 00:58:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 27 00:54:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	127082	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.633	117	103969	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	41520	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.348	65	29746	20.179	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.720%		
7) Chloroethane-d5	2.885	69	21009	22.098	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.400%		
11) 1,1-Dichloroethene-d2	4.013	63	37096	13.007	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	52.040%		
21) 2-Butanone-d5	7.073	46	16964	46.106	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.220%		
24) Chloroform-d	7.652	84	69733	21.778	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.120%		
26) 1,2-Dichloroethane-d4	8.305	65	37281	22.938	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.760%		
32) Benzene-d6	8.274	84	130332	23.785	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	95.120%		
36) 1,2-Dichloropropane-d6	9.274	67	38749	24.833	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	99.320%		
41) Toluene-d8	10.323	98	120789	22.209	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	88.840%		
43) trans-1,3-Dichloroprop...	10.579	79	16544	22.431	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	89.720%		
47) 2-Hexanone-d5	10.920	63	13993	54.070	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	108.140%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	30247	25.304	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	101.200%		
66) 1,2-Dichlorobenzene-d4	13.852	152	36412	24.605	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.440%		
Target Compounds					Qvalue	
13) Acetone	4.141	43	1785m	5.434	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
Data File : VW020957.D
Acq On : 26 Nov 2021 15:03
Operator : SY/VA
Sample : M4833-07
Misc : 6.36g/10.0mL/MSVOA_W/SOIL
ALS Vial : 12 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
ESQM7

Quant Time: Nov 27 00:58:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 27 00:54:15 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 11/28/2021
Supervised By :Mahesh Dadoda 11/29/2021

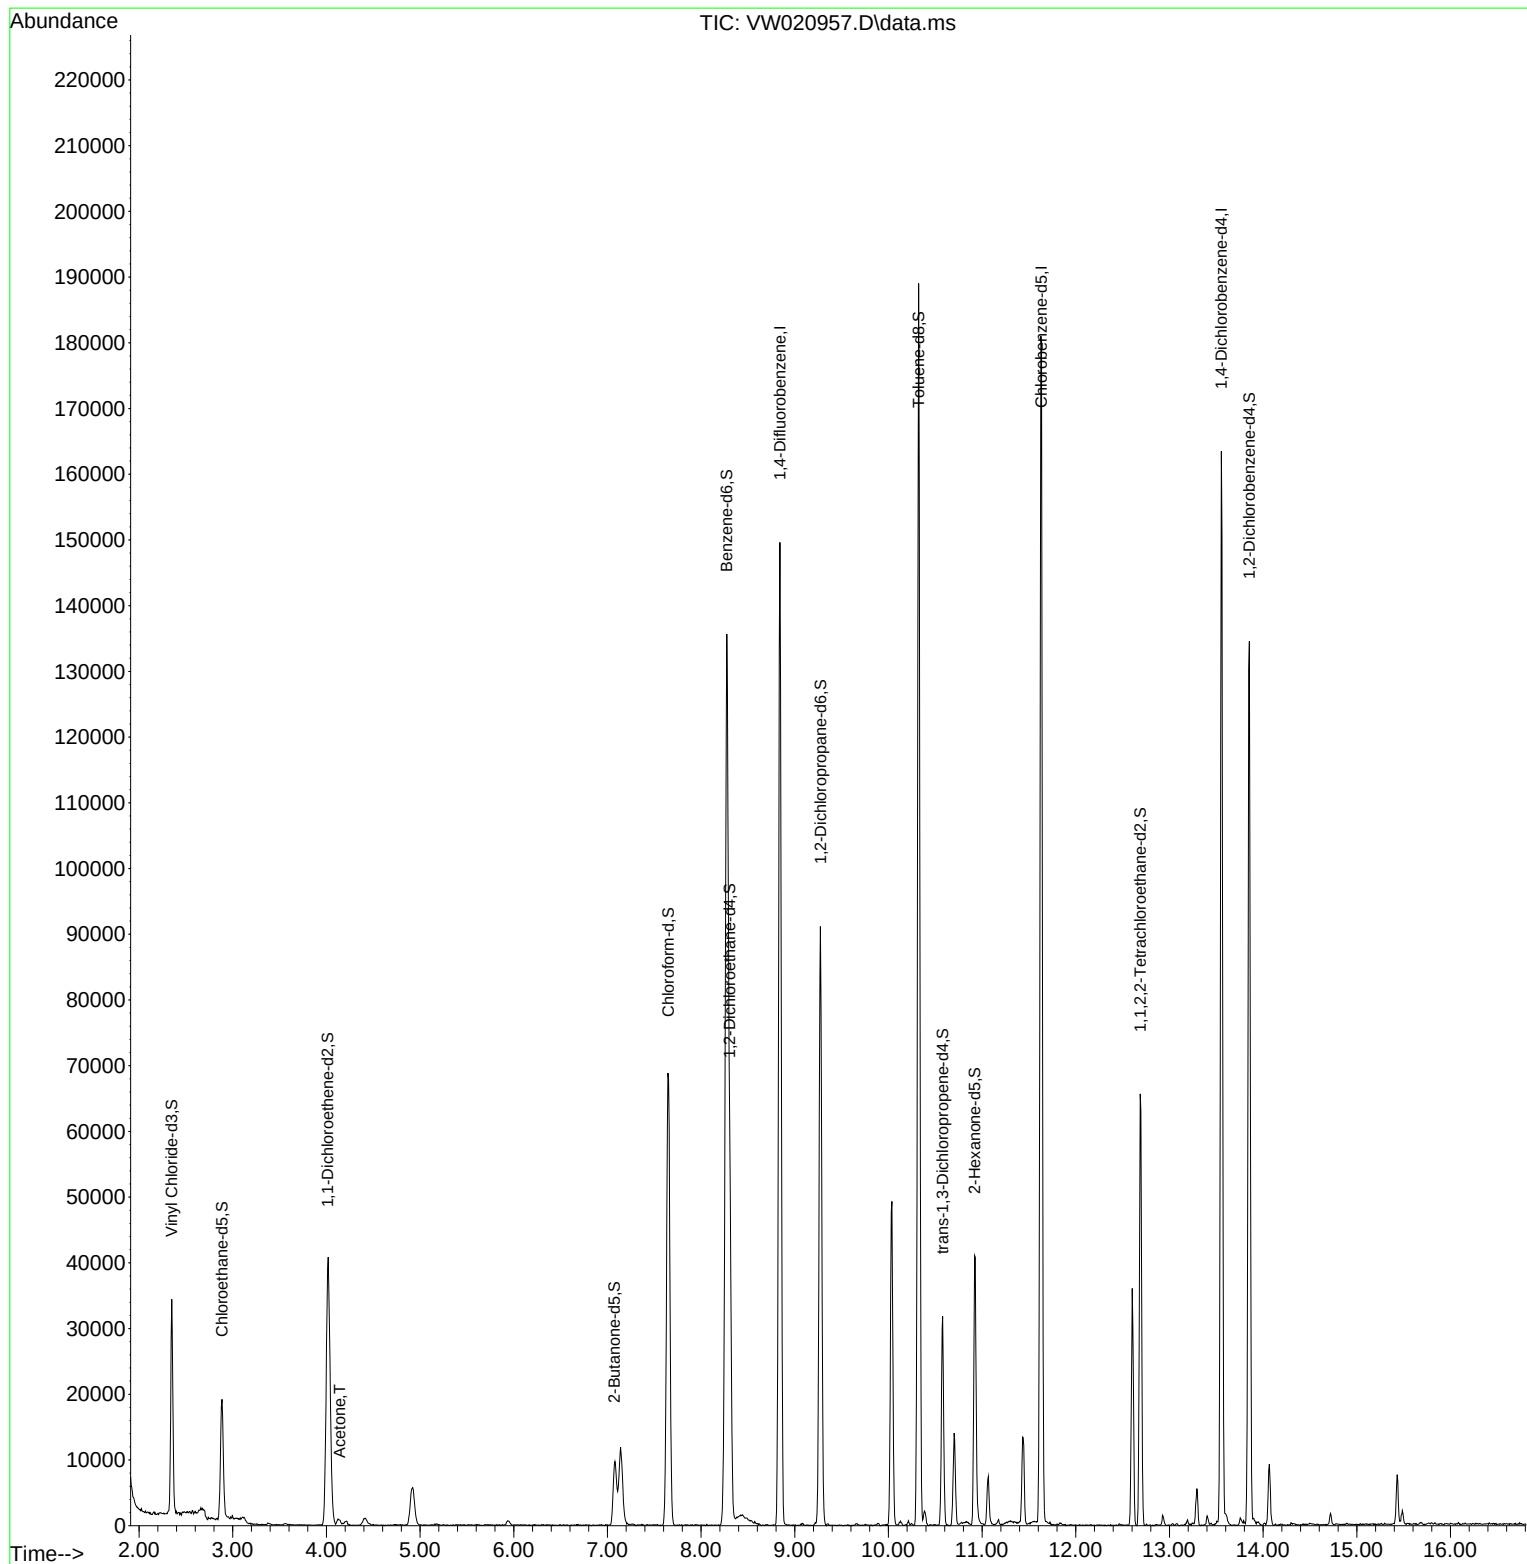

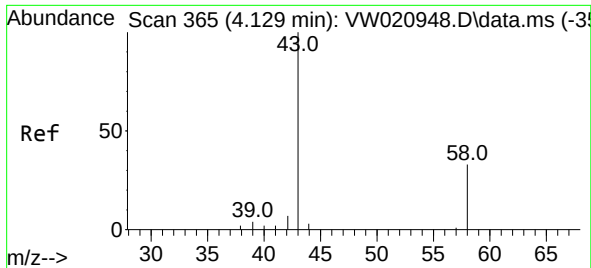

#13
 Acetone
 Concen: 5.434 ug/L m
 RT: 4.141 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW020957.D
 Acq: 26 Nov 2021 15:03

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQM7

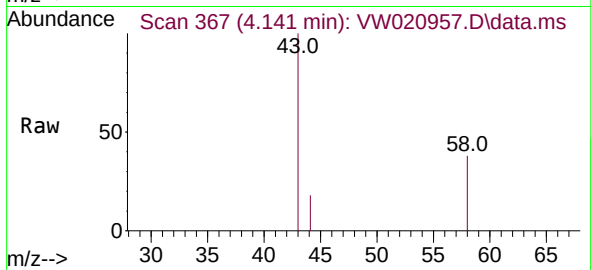

Tgt Ion: 43 Resp: 178
 Ion Ratio Lower Upper
 43 100
 58 31.7 0.0 52.8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
 Supervised By :Mahesh Dadoda 11/29/2021

