

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
 Data File : VW020959.D
 Acq On : 26 Nov 2021 15:51
 Operator : SY/VA
 Sample : M4833-14
 Misc : 4.71g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQN2

Quant Time: Nov 27 00:58:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 27 00:54:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	130797	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	101575	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	43249	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	27852	18.358	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.440%
7) Chloroethane-d5	2.885	69	18900	19.315	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.280%
11) 1,1-Dichloroethene-d2	4.013	63	34068	11.606	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.440%
21) 2-Butanone-d5	7.080	46	14930	39.426	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.860%
24) Chloroform-d	7.653	84	63843	19.372	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.480%
26) 1,2-Dichloroethane-d4	8.305	65	35908	21.466	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.880%
32) Benzene-d6	8.275	84	116855	21.828	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.320%
36) 1,2-Dichloropropane-d6	9.274	67	35670	23.398	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.600%
41) Toluene-d8	10.323	98	108077	20.340	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.360%
43) trans-1,3-Dichloroprop...	10.579	79	14560	20.207	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.840%
47) 2-Hexanone-d5	10.921	63	11978	47.375	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.740%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	30460	26.083	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	31847	20.660	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.640%
Target Compounds					Qvalue	
13) Acetone	4.135	43	1256	3.715	ug/L	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
Data File : VW020959.D
Acq On : 26 Nov 2021 15:51
Operator : SY/VA
Sample : M4833-14
Misc : 4.71g/10.0mL/MSVOA_W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ESQN2

Quant Time: Nov 27 00:58:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 27 00:54:15 2021
Response via : Initial Calibration

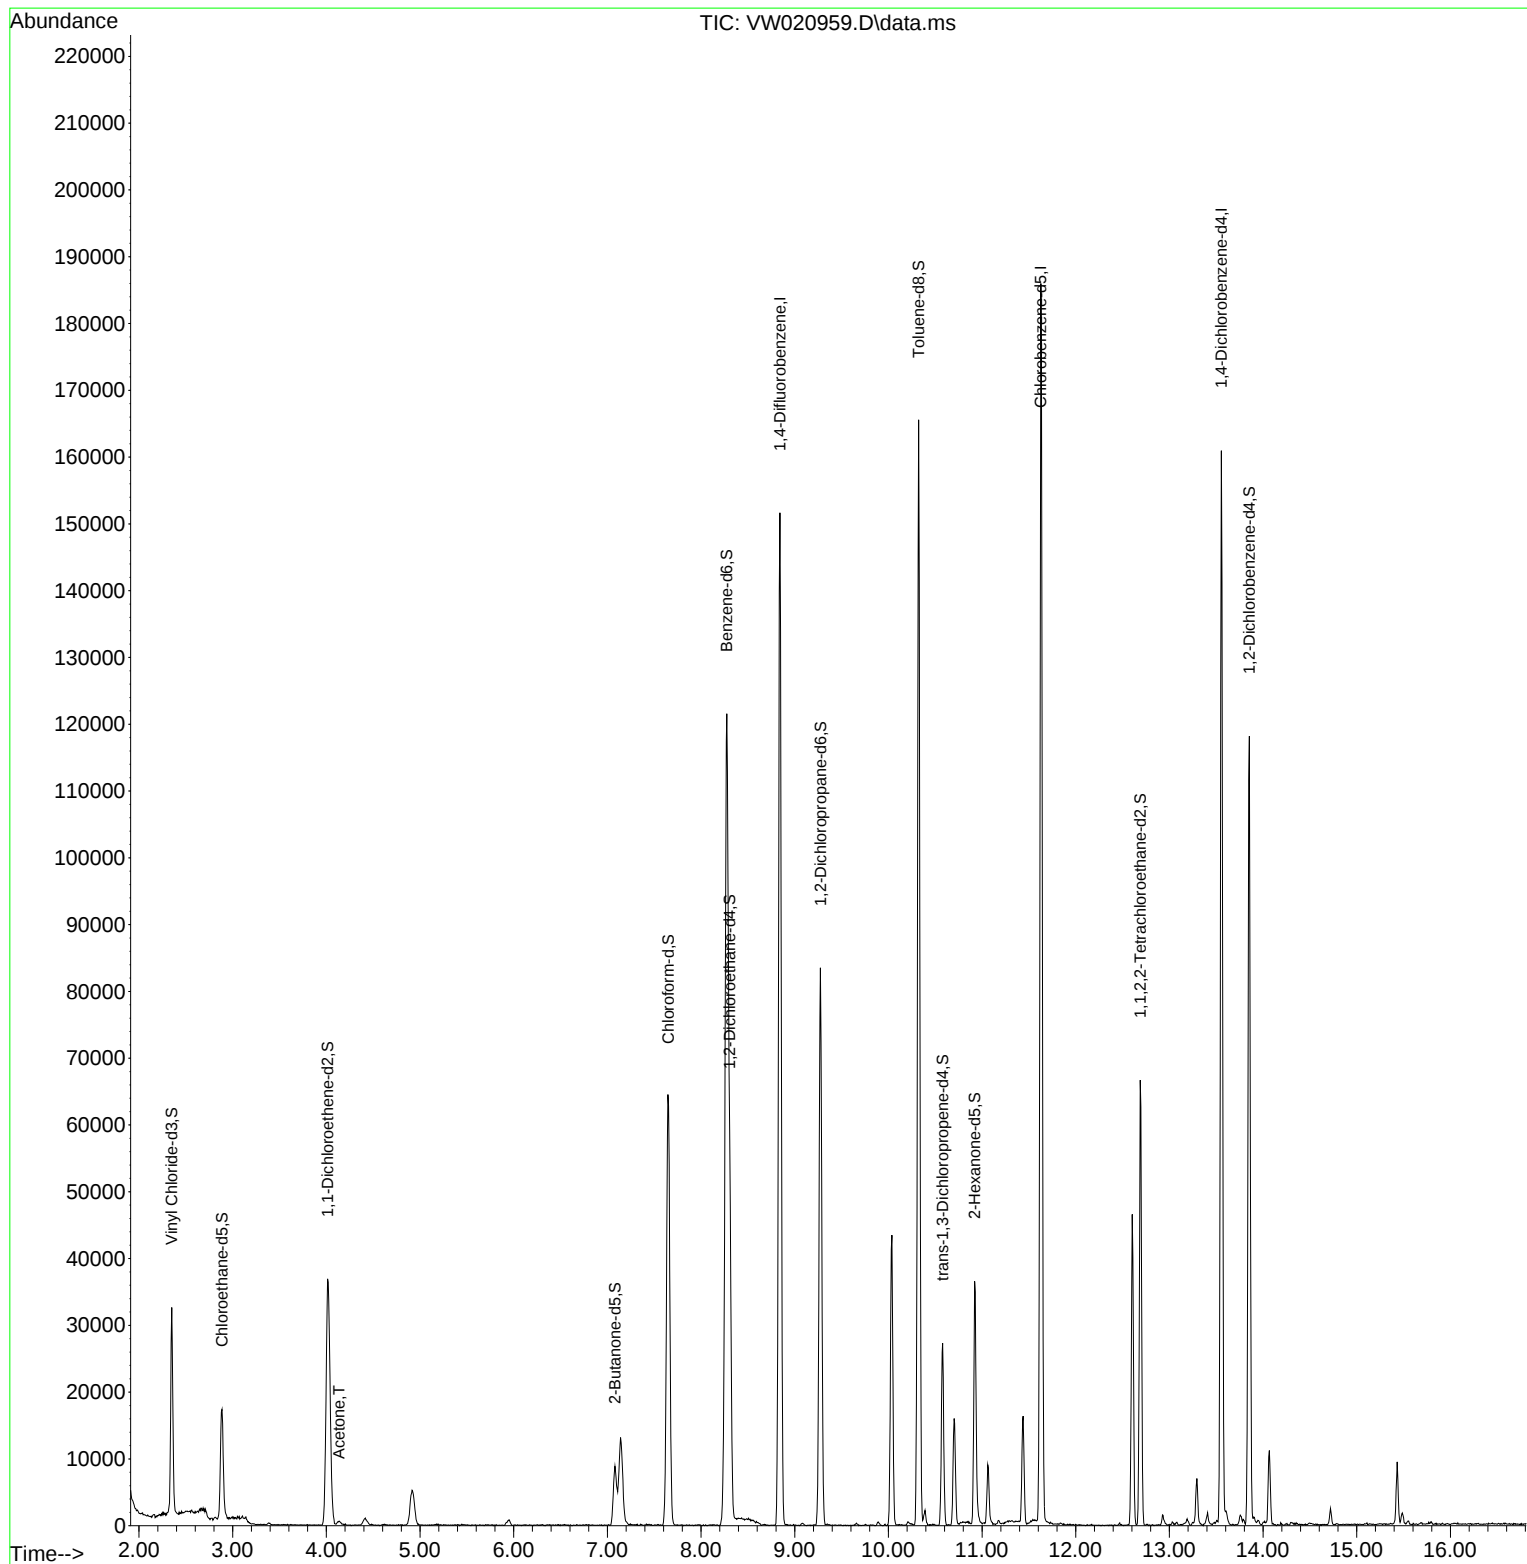

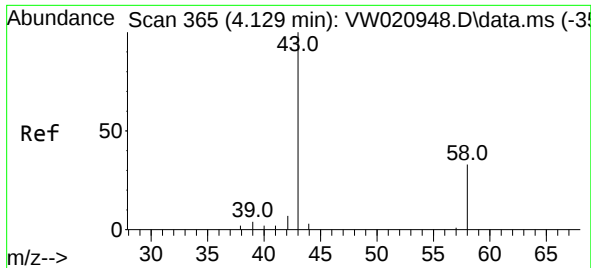

#13

Acetone

Concen: 3.715 ug/L

RT: 4.135 min Scan# 30

Delta R.T. 0.006 min

Lab File: VW020959.D


Acq: 26 Nov 2021 15:51

Instrument :

MSVOA_W

ClientSampleId :

ESQ2

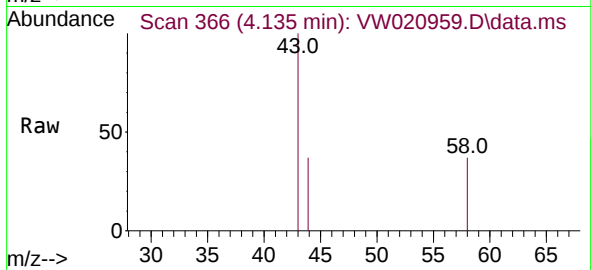

Tgt Ion: 43 Resp: 1256

Ion Ratio Lower Upper

43 100

58 15.6 0.0 52.8

