

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
 Data File : VW020960.D
 Acq On : 26 Nov 2021 16:15
 Operator : SY/VA
 Sample : M4833-20
 Misc : 6.29g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQN7

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
 Supervised By :Mahesh Dadoda 11/29/2021

Quant Time: Nov 27 00:58:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 27 00:54:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	115949	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	92863	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	33894	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	25470	18.938	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.760%		
7) Chloroethane-d5	2.885	69	17292	19.935	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.760%		
11) 1,1-Dichloroethene-d2	4.013	63	30905	11.876	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	47.520%		
21) 2-Butanone-d5	7.080	46	15888	47.328	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.660%		
24) Chloroform-d	7.653	84	56397	19.304	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	77.200%		
26) 1,2-Dichloroethane-d4	8.305	65	32419	21.862	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	87.440%		
32) Benzene-d6	8.275	84	105446	21.544	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.160%		
36) 1,2-Dichloropropane-d6	9.275	67	32040	22.989	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.960%		
41) Toluene-d8	10.323	98	92159	18.971	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	75.880%		
43) trans-1,3-Dichloroprop...	10.579	79	13808	20.961	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.840%		
47) 2-Hexanone-d5	10.921	63	12955	56.046	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	112.100%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	27366	25.632	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	102.520%		
66) 1,2-Dichlorobenzene-d4	13.853	152	24794	20.524	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	82.080%		
Target Compounds					Qvalue	
13) Acetone	4.135	43	1914m	6.386	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
Data File : VW020960.D
Acq On : 26 Nov 2021 16:15
Operator : SY/VA
Sample : M4833-20
Misc : 6.29g/10.0mL/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
ESQN7

Quant Time: Nov 27 00:58:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 27 00:54:15 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 11/28/2021
Supervised By :Mahesh Dadoda 11/29/2021

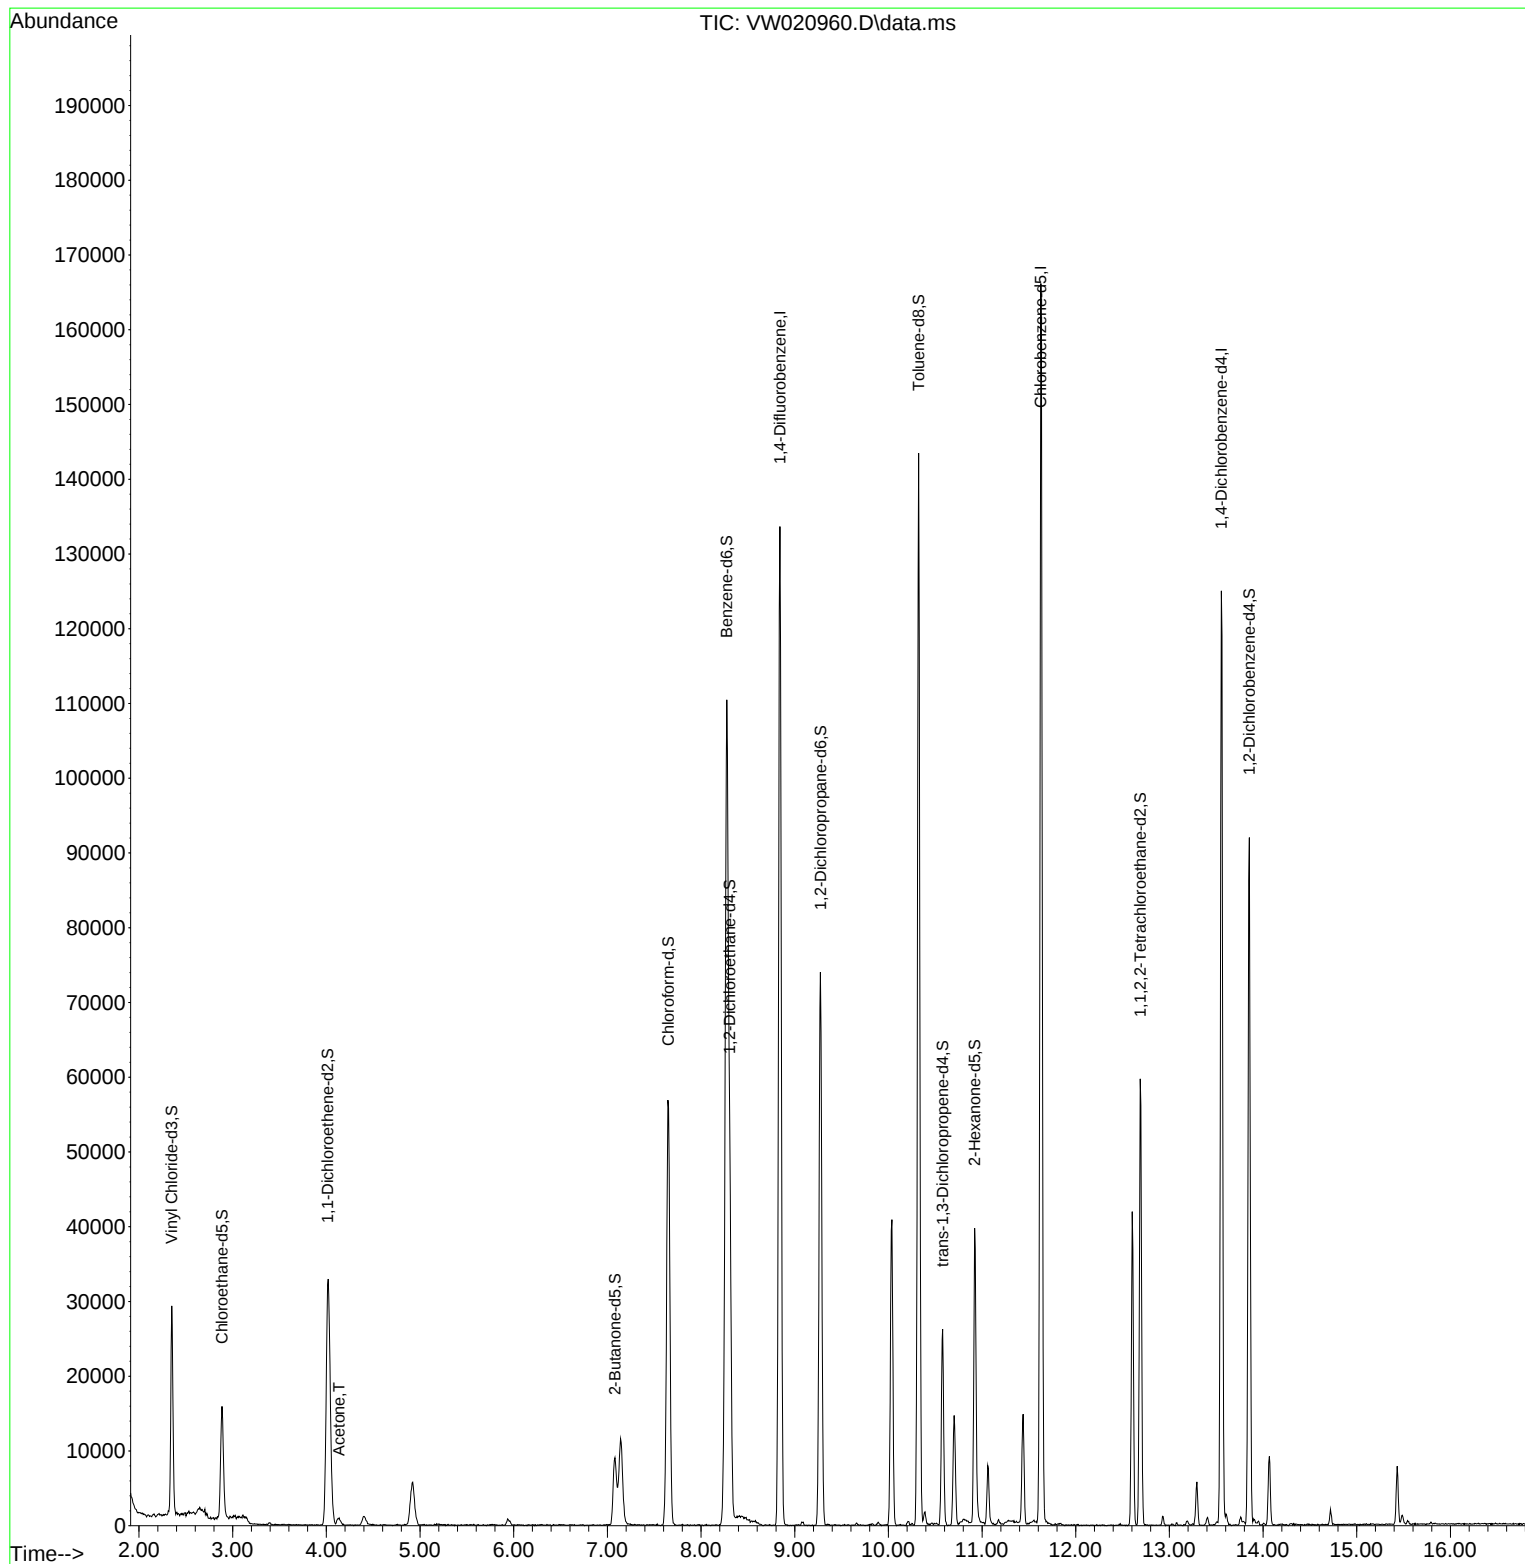

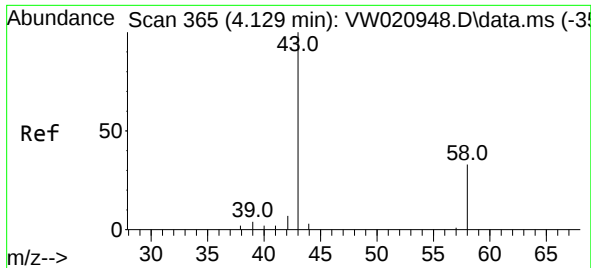

#13
 Acetone
 Concen: 6.386 ug/L m
 RT: 4.135 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW020960.D
 Acq: 26 Nov 2021 16:15

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQN7

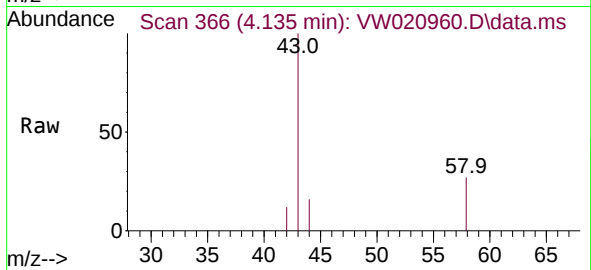

Tgt Ion: 43 Resp: 1914
 Ion Ratio Lower Upper
 43 100
 58 21.7 0.0 52.8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
 Supervised By :Mahesh Dadoda 11/29/2021

