

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
 Data File : VW020961.D
 Acq On : 26 Nov 2021 16:39
 Operator : SY/VA
 Sample : M4833-22
 Misc : 5.87g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQN9

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
 Supervised By :Mahesh Dadoda 11/29/2021

Quant Time: Nov 27 00:59:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 27 00:54:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	121338	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.627	117	98979	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	36862	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	25439	18.074	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.280%		
7) Chloroethane-d5	2.885	69	17279	19.035	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	76.160%		
11) 1,1-Dichloroethene-d2	4.013	63	31127	11.430	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	45.720%		
21) 2-Butanone-d5	7.079	46	12666	36.055	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	72.100%		
24) Chloroform-d	7.652	84	59188	19.359	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	77.440%		
26) 1,2-Dichloroethane-d4	8.305	65	32826	21.153	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	84.600%		
32) Benzene-d6	8.274	84	106423	20.400	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	81.600%		
36) 1,2-Dichloropropane-d6	9.274	67	33243	22.378	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	89.520%		
41) Toluene-d8	10.323	98	97586	18.847	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	75.400%		
43) trans-1,3-Dichloroprop...	10.579	79	13303	18.946	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	75.800%		
47) 2-Hexanone-d5	10.920	63	11561	46.925	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.840%		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	28472	25.020	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	100.080%		
66) 1,2-Dichlorobenzene-d4	13.853	152	26975	20.532	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	82.120%		
Target Compounds					Qvalue	
13) Acetone	4.141	43	1559m	4.970	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
Data File : VW020961.D
Acq On : 26 Nov 2021 16:39
Operator : SY/VA
Sample : M4833-22
Misc : 5.87g/10.0mL/MSVOA_W/SOIL
ALS Vial : 16 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
ESQN9

Quant Time: Nov 27 00:59:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 27 00:54:15 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
Supervised By :Mahesh Dadoda 11/29/2021

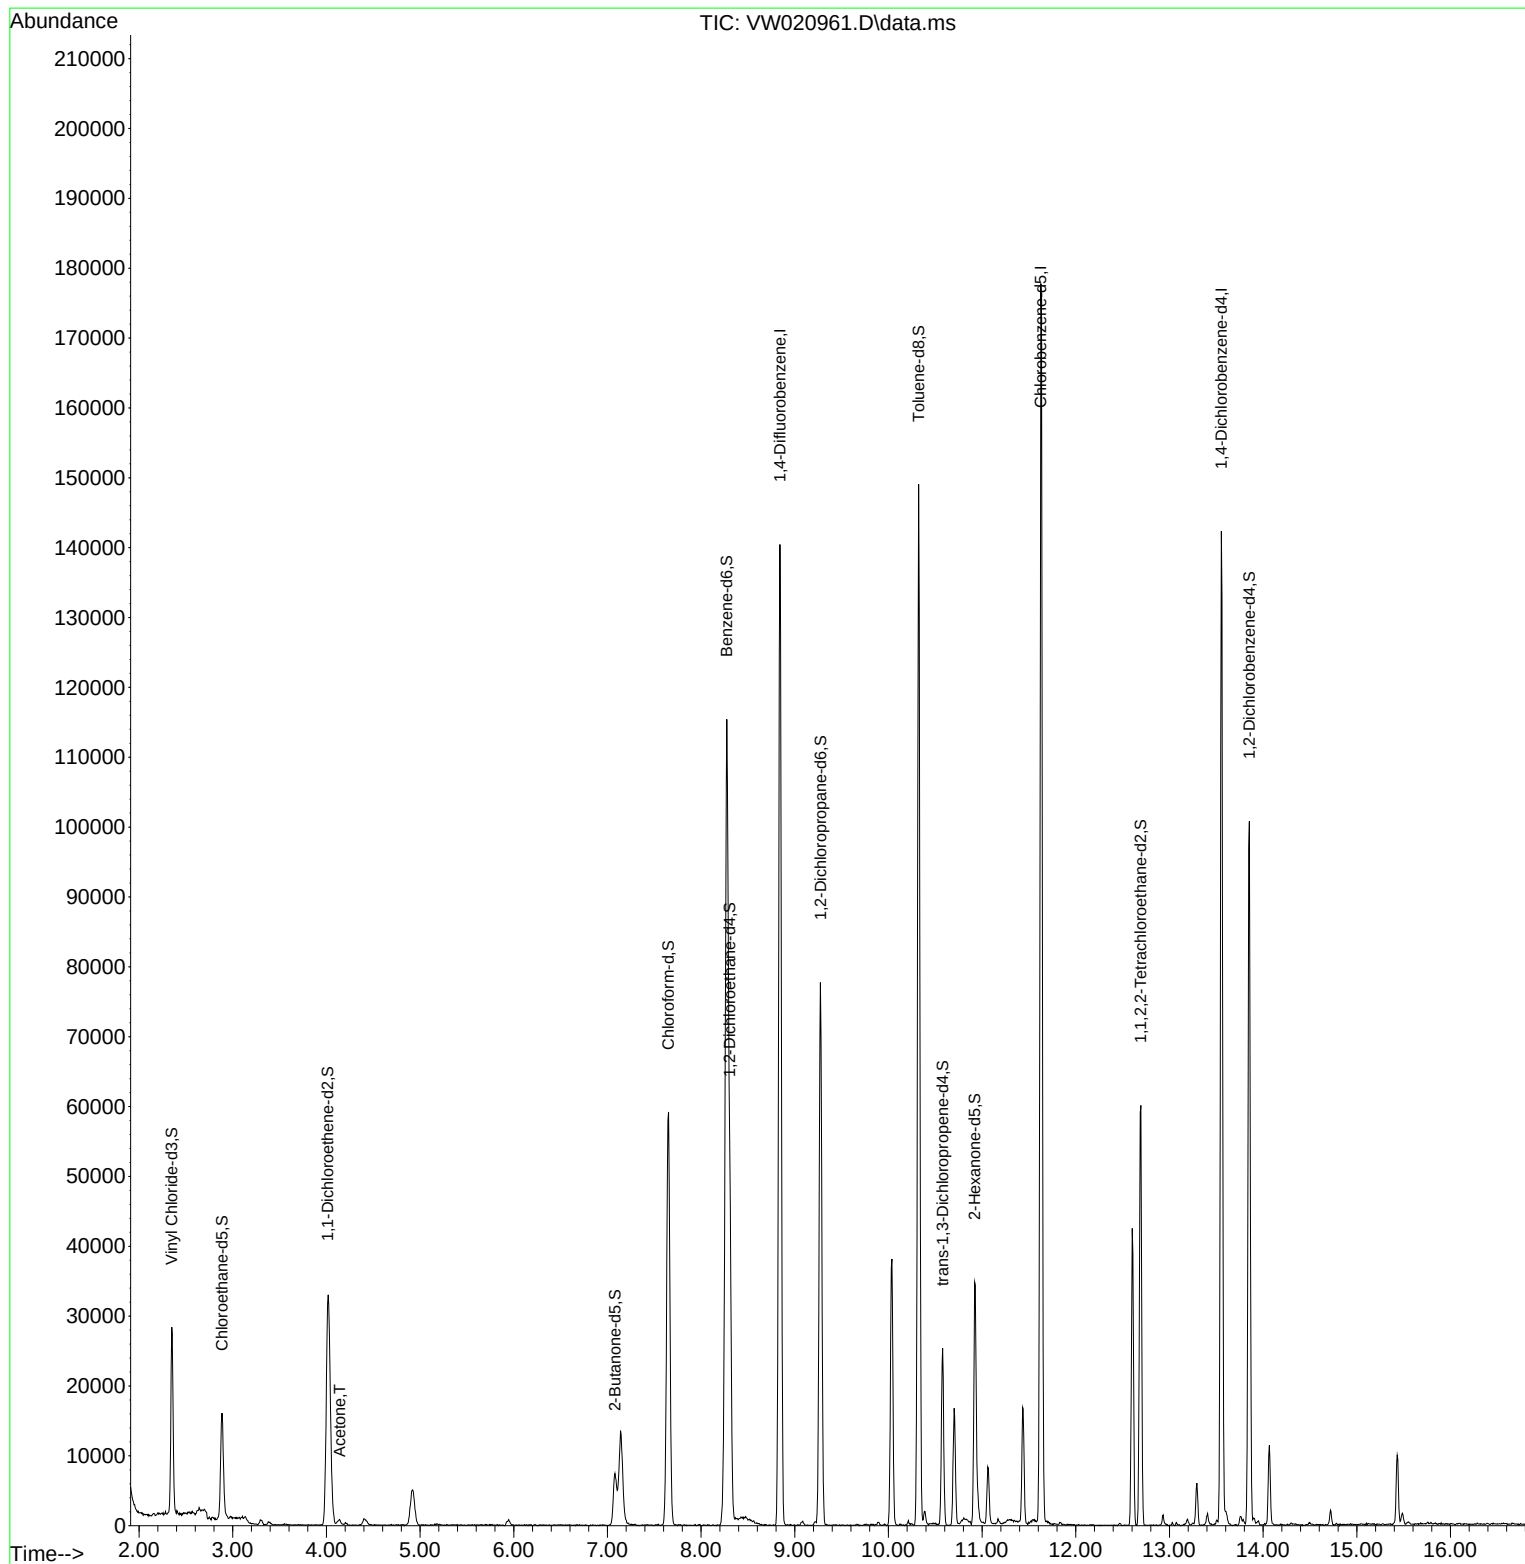

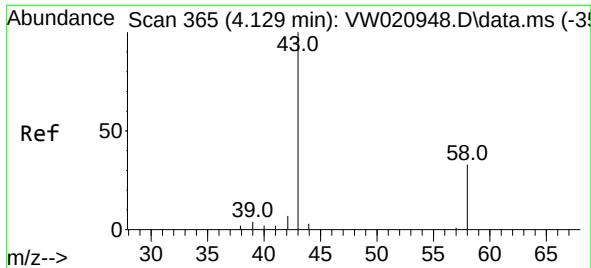

#13
 Acetone
 Concen: 4.970 ug/L m
 RT: 4.141 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW020961.D
 Acq: 26 Nov 2021 16:39

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQN9

Tgt Ion: 43 Resp: 155
 Ion Ratio Lower Upper
 43 100
 58 25.4 0.0 52.8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
 Supervised By :Mahesh Dadoda 11/29/2021

