

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
 Data File : VW020963.D
 Acq On : 26 Nov 2021 17:27
 Operator : SY/VA
 Sample : M4833-18
 Misc : 5.68g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQN4

Quant Time: Nov 27 00:59:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 27 00:54:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	118654	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	98367	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	42308	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	25287	18.373	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	73.480%		
7) Chloroethane-d5	2.885	69	18081	20.369	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.480%		
11) 1,1-Dichloroethene-d2	4.019	63	32464	12.191	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	48.760%		
21) 2-Butanone-d5	7.080	46	13314	38.756	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	77.520%		
24) Chloroform-d	7.653	84	58634	19.612	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	78.440%		
26) 1,2-Dichloroethane-d4	8.305	65	32571	21.463	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	85.840%		
32) Benzene-d6	8.275	84	108870	20.999	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	84.000%		
36) 1,2-Dichloropropane-d6	9.274	67	33831	22.916	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.680%		
41) Toluene-d8	10.323	98	101308	19.688	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	78.760%		
43) trans-1,3-Dichloroprop...	10.579	79	13456	19.283	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.120%		
47) 2-Hexanone-d5	10.920	63	11321	46.236	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.480%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	26707	23.615	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.440%		
66) 1,2-Dichlorobenzene-d4	13.853	152	31287	20.748	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	83.000%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	3151	10.273	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
Data File : VW020963.D
Acq On : 26 Nov 2021 17:27
Operator : SY/VA
Sample : M4833-18
Misc : 5.68g/10.0mL/MSVOA_W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ESQN4

Quant Time: Nov 27 00:59:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 27 00:54:15 2021
Response via : Initial Calibration

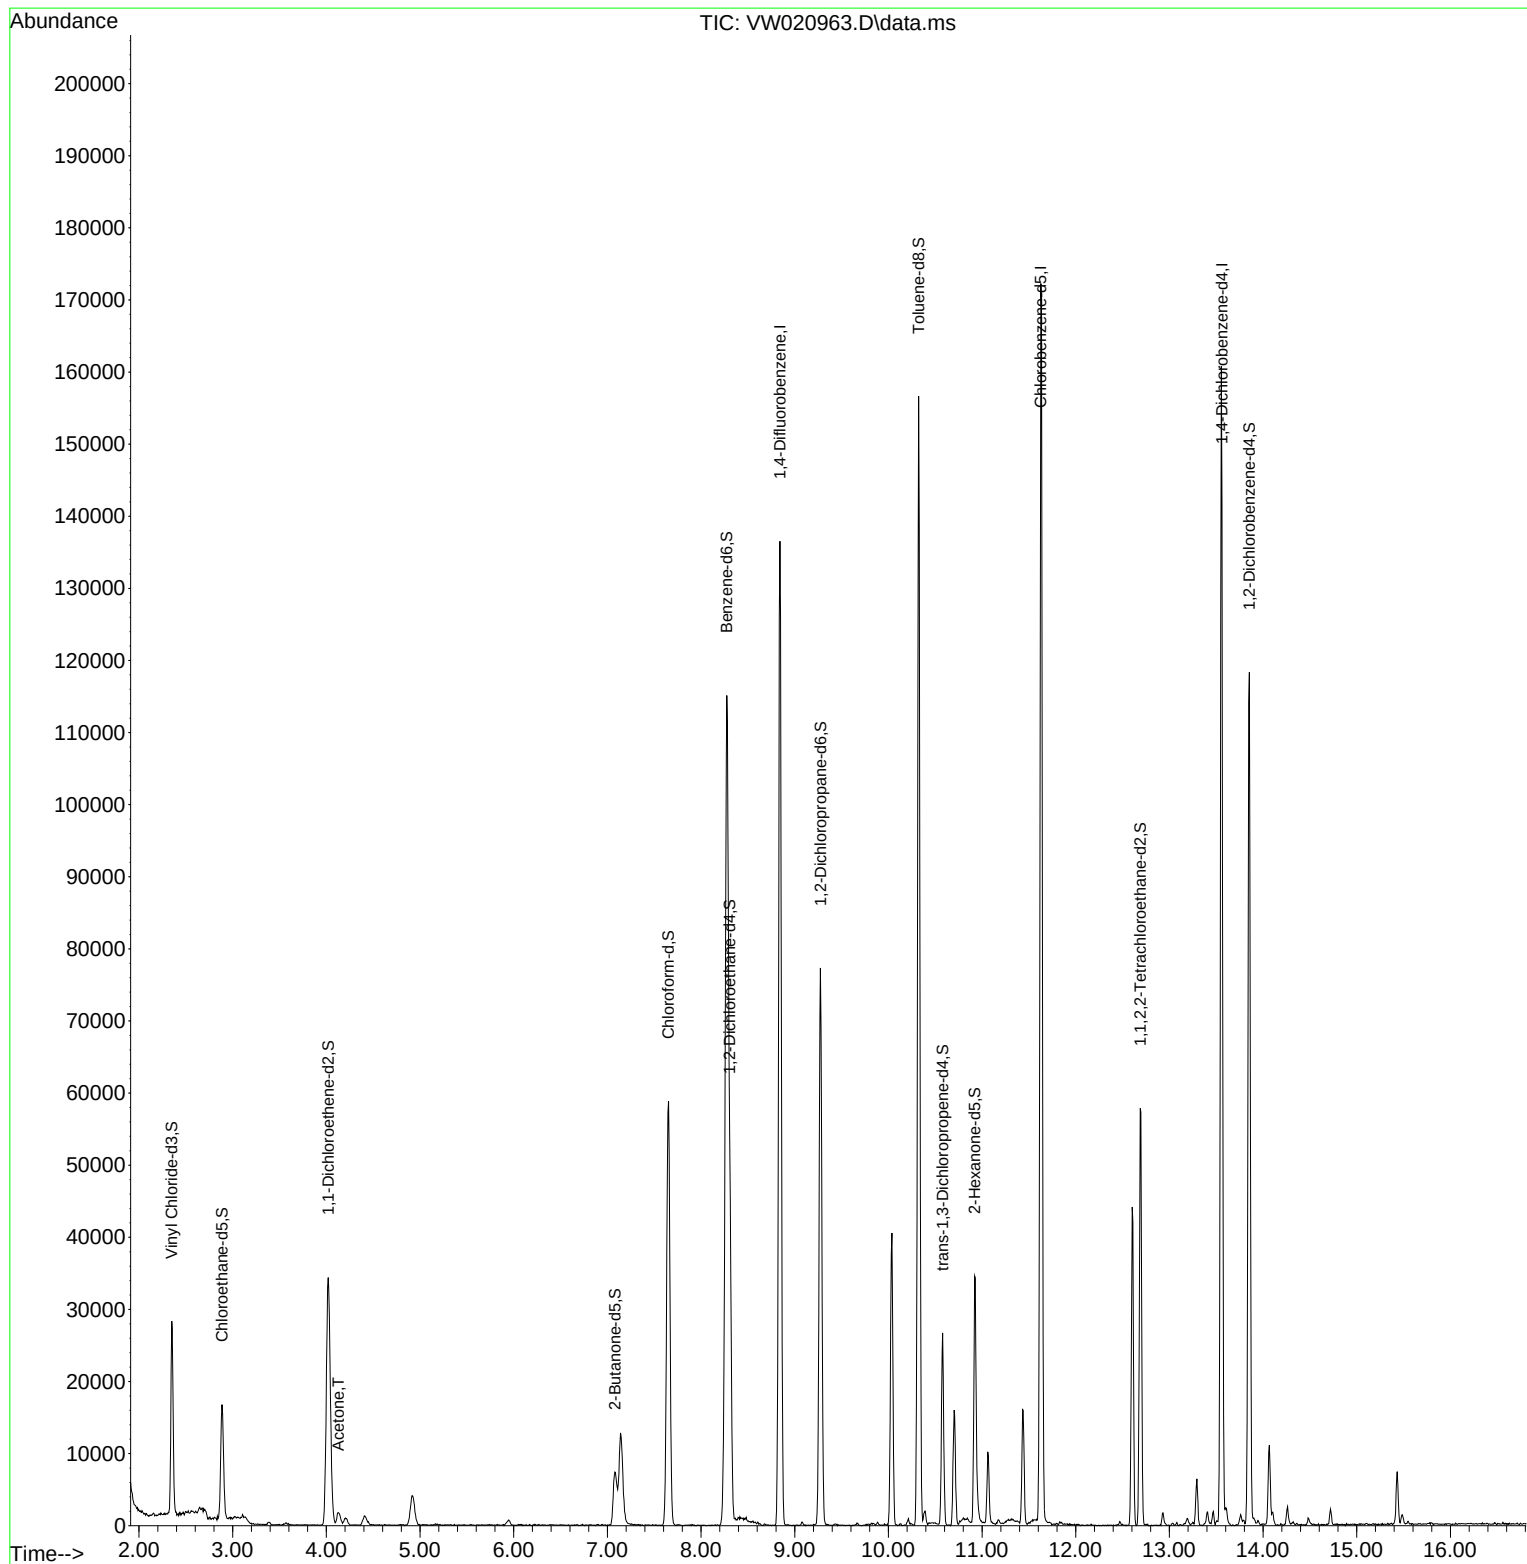

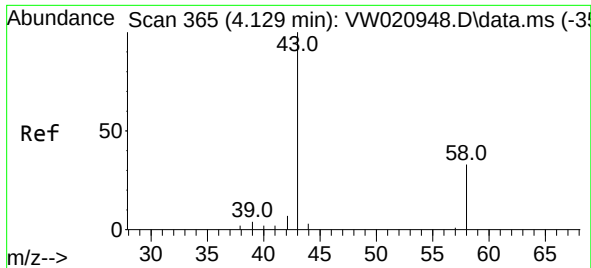

#13
 Acetone
 Concen: 10.273 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW020963.D
 Acq: 26 Nov 2021 17:27

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQN4

Tgt Ion: 43 Resp: 3151
 Ion Ratio Lower Upper
 43 100
 58 18.4 0.0 52.8

