

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
 Data File : VW020964.D
 Acq On : 26 Nov 2021 17:51
 Operator : SY/VA
 Sample : M4833-23
 Misc : 5.73g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQP0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
 Supervised By :Mahesh Dadoda 11/29/2021

Quant Time: Nov 27 00:59:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 27 00:54:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	124096	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.633	117	101307	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	40770	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.348	65	25896	17.990	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.960%		
7) Chloroethane-d5	2.885	69	18784	20.233	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.920%		
11) 1,1-Dichloroethene-d2	4.019	63	33242	11.936	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	47.760%		
21) 2-Butanone-d5	7.079	46	12599	35.067	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	70.140%		
24) Chloroform-d	7.646	84	61199	19.572	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	78.280%		
26) 1,2-Dichloroethane-d4	8.305	65	33315	20.991	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	83.960%		
32) Benzene-d6	8.274	84	113138	21.189	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	84.760%		
36) 1,2-Dichloropropane-d6	9.274	67	34281	22.547	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	90.200%		
41) Toluene-d8	10.323	98	101261	19.107	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	76.440%		
43) trans-1,3-Dichloroprop...	10.579	79	13595	18.917	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	75.680%		
47) 2-Hexanone-d5	10.920	63	10872	43.114	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.220%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	27119	23.283	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.120%		
66) 1,2-Dichlorobenzene-d4	13.852	152	30082	20.702	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	82.800%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	1253m	3.906	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112621\
Data File : VW020964.D
Acq On : 26 Nov 2021 17:51
Operator : SY/VA
Sample : M4833-23
Misc : 5.73g/10.0mL/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
ESQP0

Quant Time: Nov 27 00:59:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 27 00:54:15 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
Supervised By :Mahesh Dadoda 11/29/2021

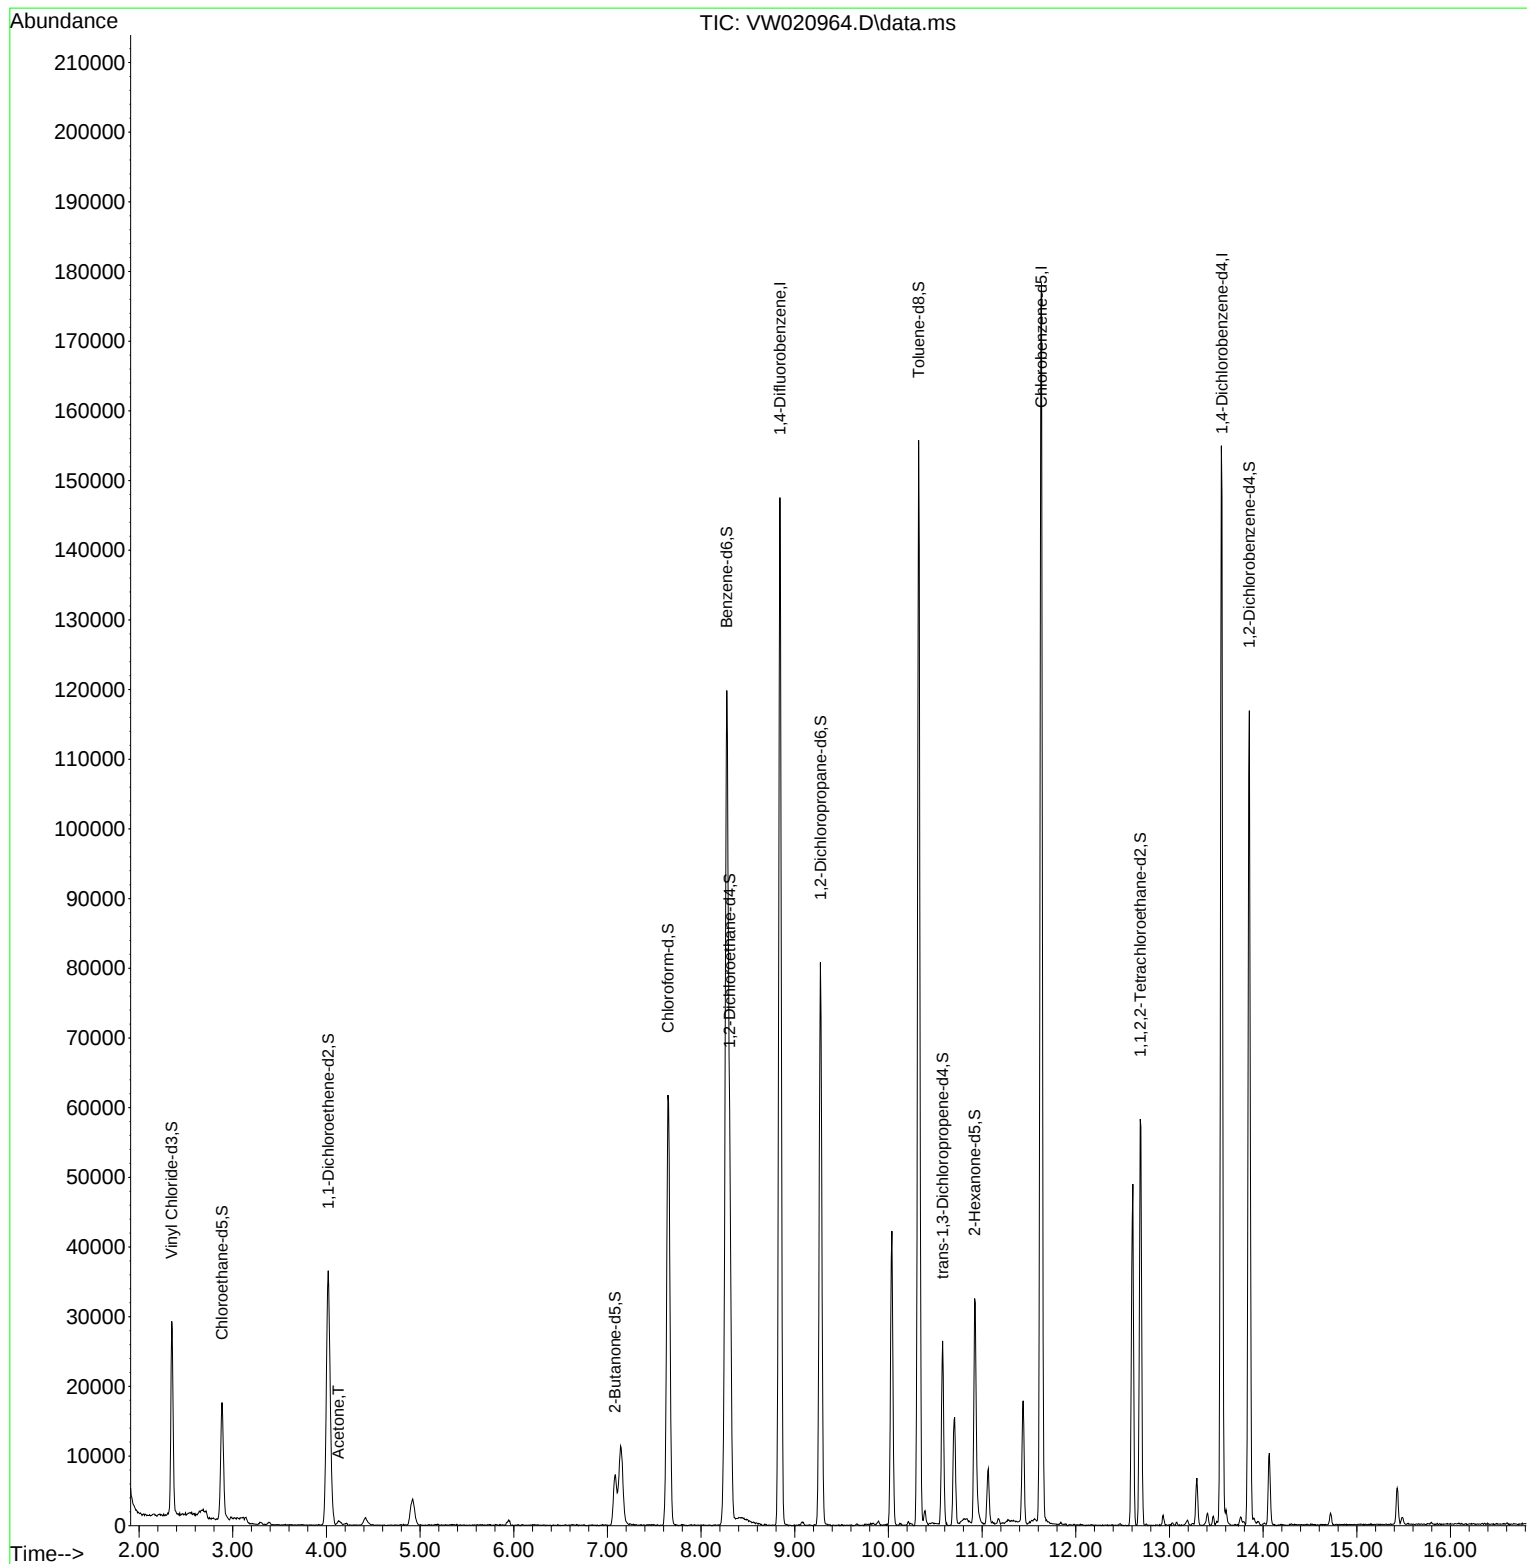

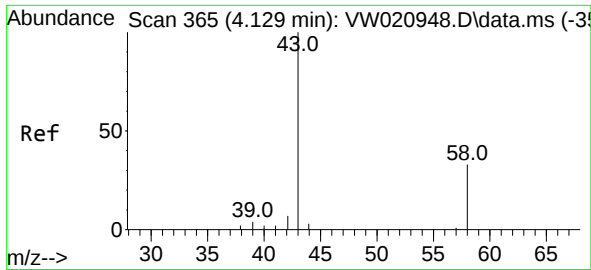

#13
Acetone
Concen: 3.906 ug/L m
RT: 4.129 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW020964.D
Acq: 26 Nov 2021 17:51

Instrument :
MSVOA_W
ClientSampleId :
ESQP0

Tgt Ion: 43 Resp: 125
Ion Ratio Lower Upper
43 100
58 27.3 0.0 52.8

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 11/28/2021
Supervised By :Mahesh Dadoda 11/29/2021

