


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW112818\
Data File : VW007103.D
Acq On : 28 Nov 2018 09:40
Operator : VAY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W112118S.M
Title : SW846 8260
Last Update : Wed Nov 21 03:23:02 2018

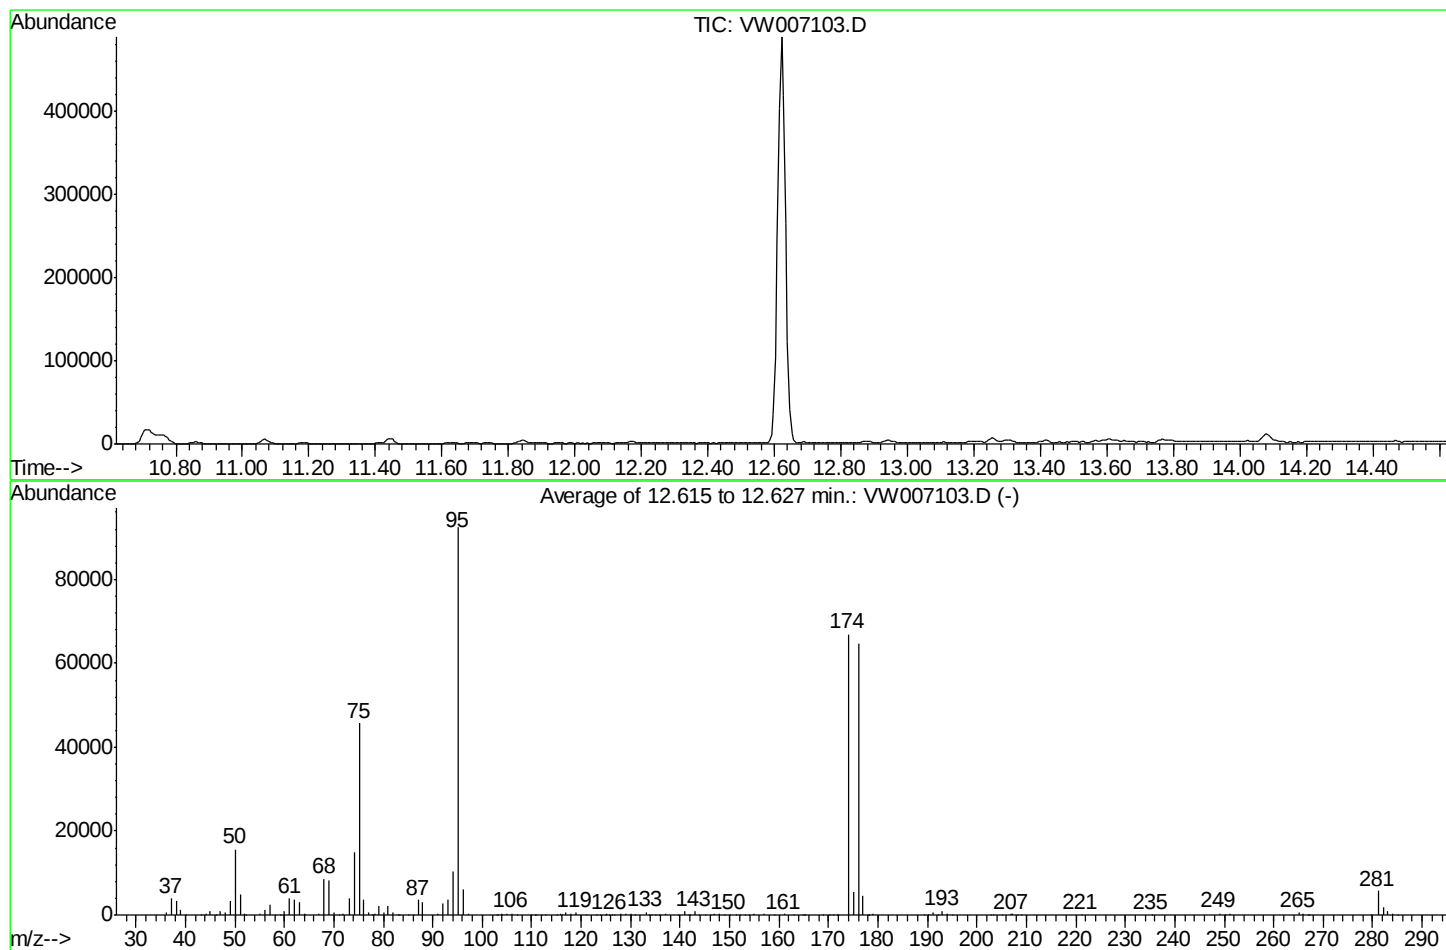

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	15724	PASS
75	95	30	60	49.4	45645	PASS
95	95	100	100	100.0	92421	PASS
96	95	5	9	6.7	6153	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.3	66864	PASS
175	174	5	9	8.3	5549	PASS
176	174	95	101	96.8	64744	PASS
177	176	5	9	7.1	4605	PASS