

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
 Data File : VW014173.D
 Acq On : 29 Nov 2019 11:36
 Operator : SY/VA
 Sample : K6064-03
 Misc : 6.10G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 30 04:13:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 30 04:10:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	352670	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	341193	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	182833	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	90393	16.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.28%
7) Chloroethane-d5	2.89	69	90454	19.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.32%
10) 1,1-Dichloroethene-d2	4.01	63	162198	14.05	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.20%
20) 2-Butanone-d5	7.07	46	76712	46.93	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.86%
24) Chloroform-d	7.65	84	273580	25.23	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.92%
26) 1,2-Dichloroethane-d4	8.31	65	139972	25.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.68%
29) Benzene-d6	8.27	84	549493	22.70	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.80%
33) 1,2-Dichloropropane-d6	9.27	67	173577	24.48	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.92%
37) Toluene-d8	10.32	98	501125	21.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.32%
38) trans-1,3-Dichloropropene-	10.57	79	63130	20.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.16%
39) 2-Hexanone-d5	10.92	63	57530	42.78	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.56%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	129708	24.22	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.88%
61) 1,2-Dichlorobenzene-d4	13.85	152	184789	25.16	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.64%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.55	75	18499	4.759 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW112919\
Data File : VW014173.D
Acq On : 29 Nov 2019 11:36
Operator : SY/VA
Sample : K6064-03
Misc : 6.10G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 30 04:13:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 30 04:10:38 2019
Response via : Initial Calibration

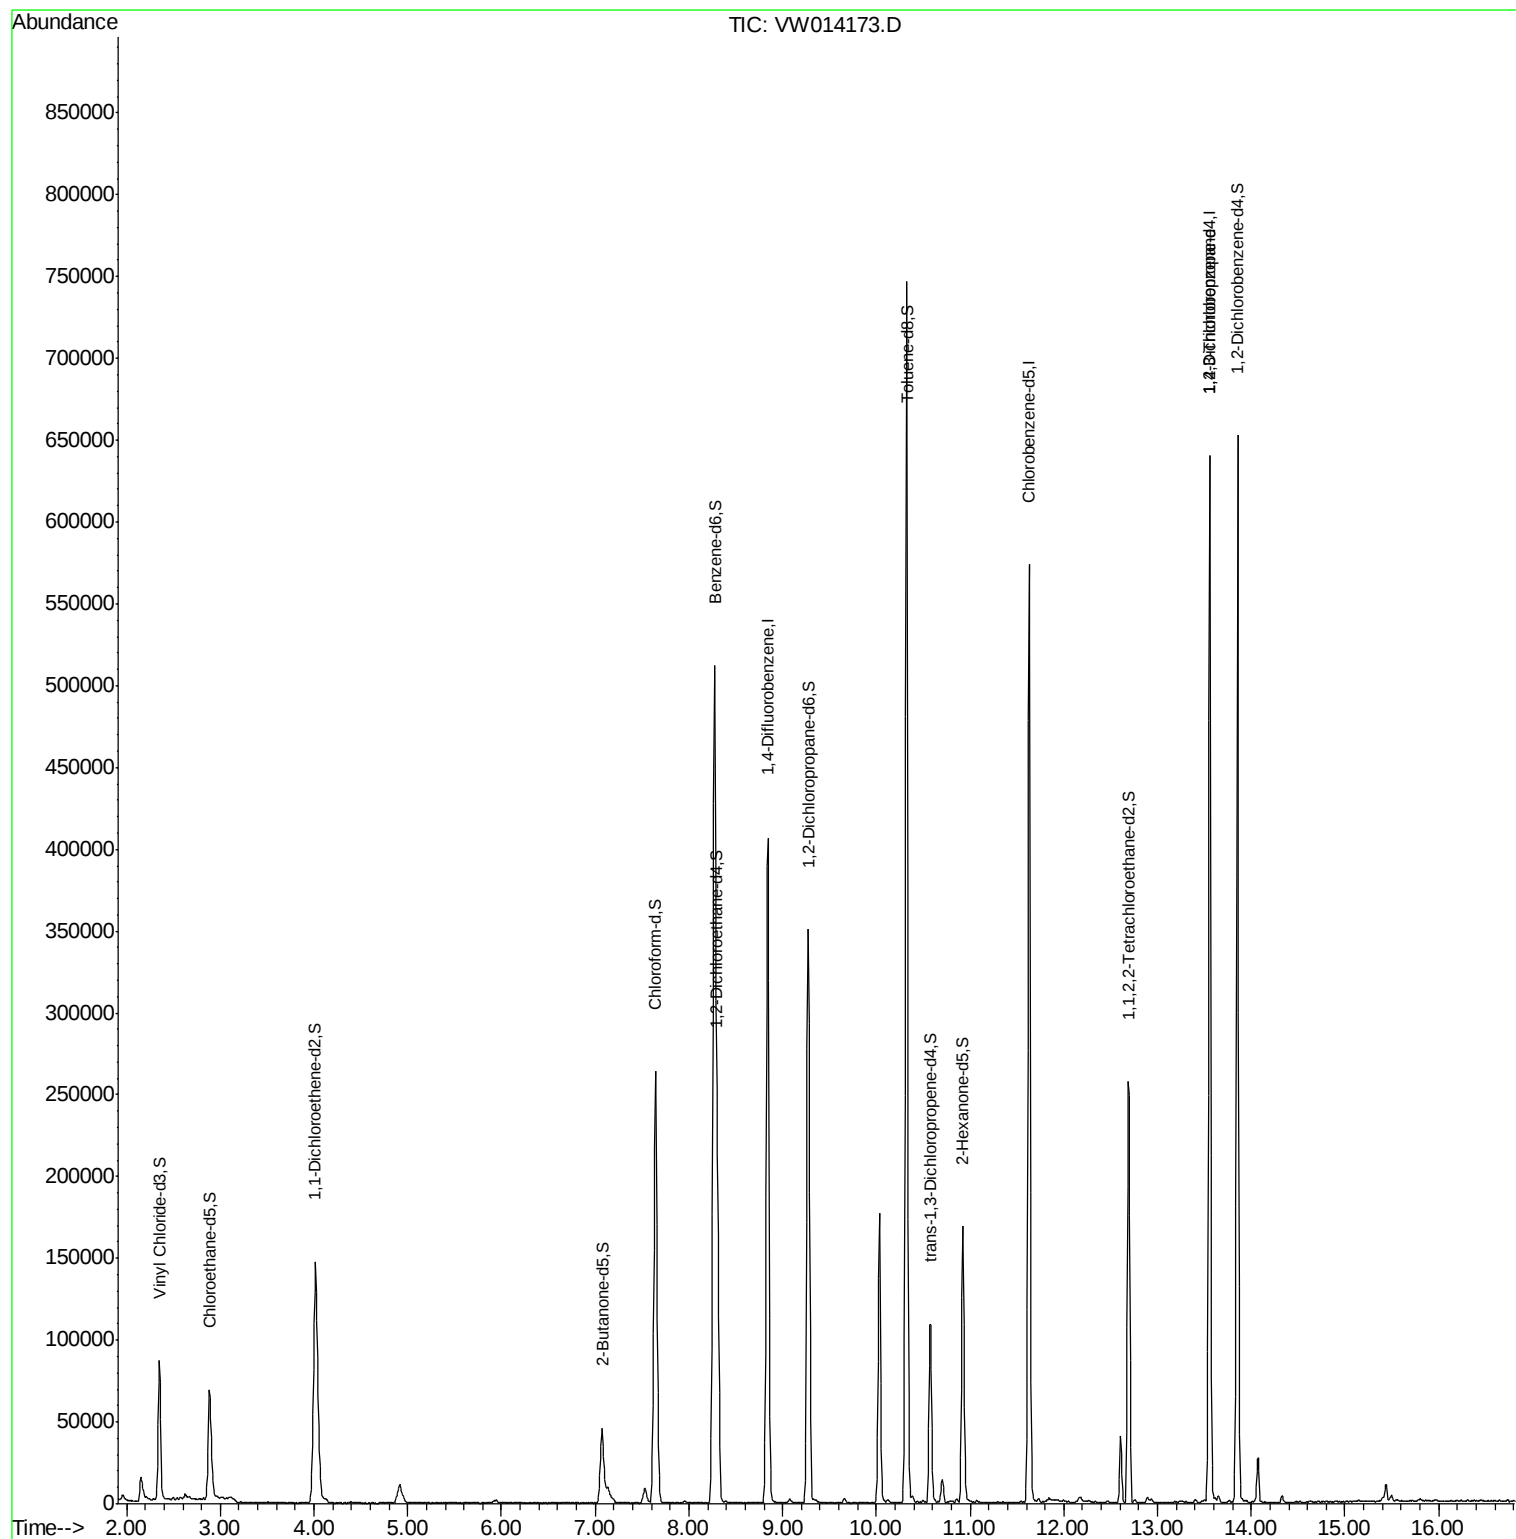

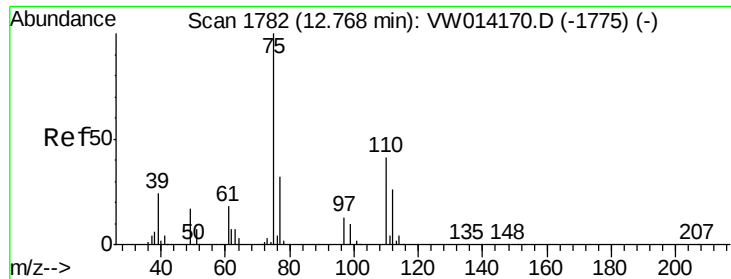

#59

1,2,3-Trichloropropane

Concen: 4.759 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW014173.D

Acq: 29 Nov 2019 11:36

Instrument :

MSVOA_W

ClientSampleId :

Tot Ion: 75 Resp: 18499

Ion Ratio Lower Upper

75 100

77 38.5 25.9 38.9

