

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
 Data File : VW014177.D
 Acq On : 29 Nov 2019 13:21
 Operator : SY/VA
 Sample : K6089-06
 Misc : 5.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 30 04:13:31 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 30 04:10:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	279458	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	257414	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	112122	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	73672	16.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.08%
7) Chloroethane-d5	2.89	69	74111	20.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.00%
10) 1,1-Dichloroethene-d2	4.01	63	126576	13.83	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.32%
20) 2-Butanone-d5	7.07	46	79218	61.16	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.32%
24) Chloroform-d	7.65	84	217281	25.29	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.16%
26) 1,2-Dichloroethane-d4	8.30	65	121115	28.04	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	112.16%
29) Benzene-d6	8.27	84	424707	23.25	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.00%
33) 1,2-Dichloropropane-d6	9.27	67	139804	26.13	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.52%
37) Toluene-d8	10.32	98	368103	21.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.00%
38) trans-1,3-Dichloropropene-	10.58	79	50253	21.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.72%
39) 2-Hexanone-d5	10.92	63	57792	56.96	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.92%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	116298	28.79	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	115.16%
61) 1,2-Dichlorobenzene-d4	13.85	152	115419	25.62	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.48%

Target Compounds


					Ovalue
35) Trichloroethene	8.84	95	8148	1.618 ug/L #	2
42) cis-1,3-Dichloropropene	10.03	75	2868	0.400 ug/L #	73
59) 1,2,3-Trichloropropane	13.55	75	11464	3.909 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW112919\
Data File : VW014177.D
Acq On : 29 Nov 2019 13:21
Operator : SY/VA
Sample : K6089-06
Misc : 5.36G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 30 04:13:31 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 30 04:10:38 2019
Response via : Initial Calibration




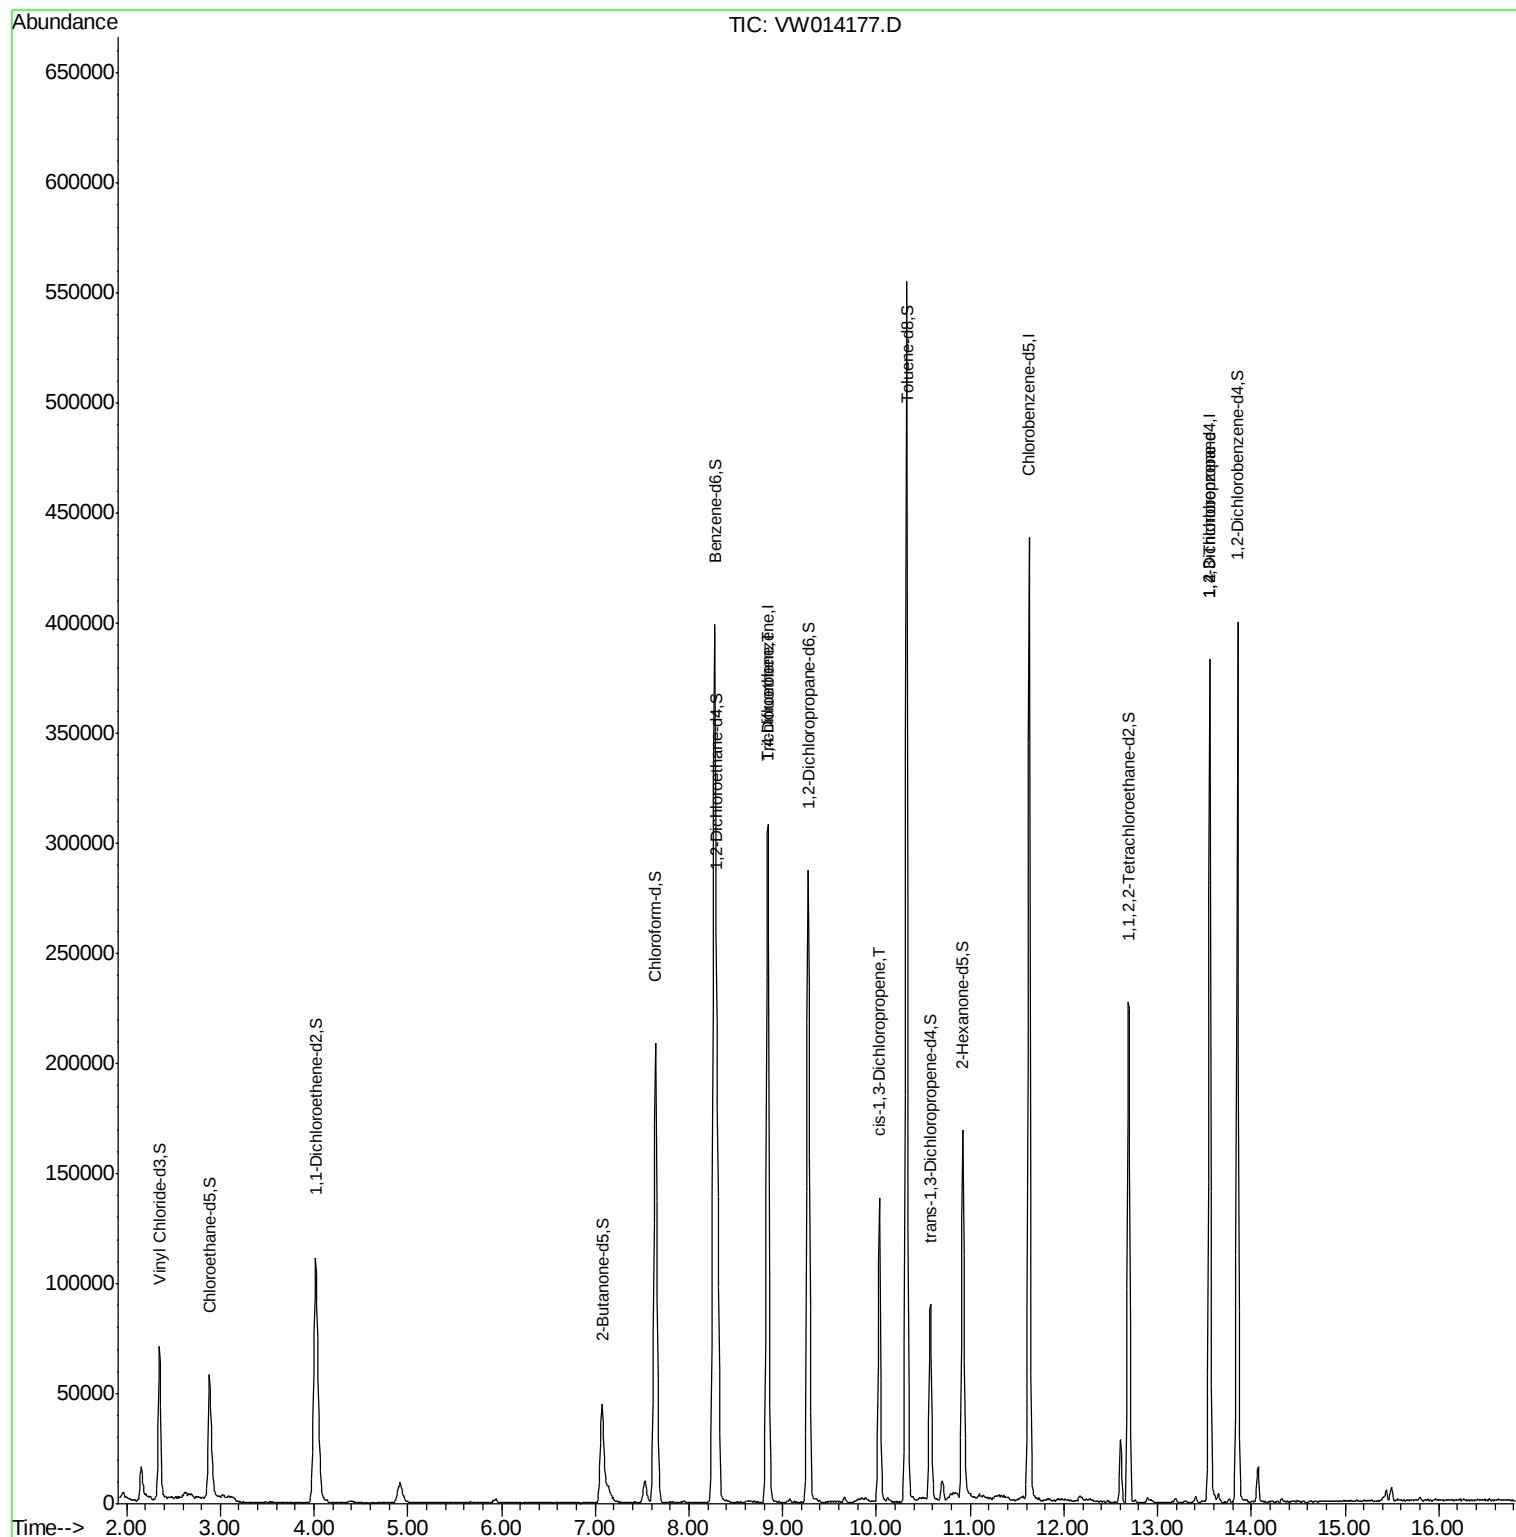


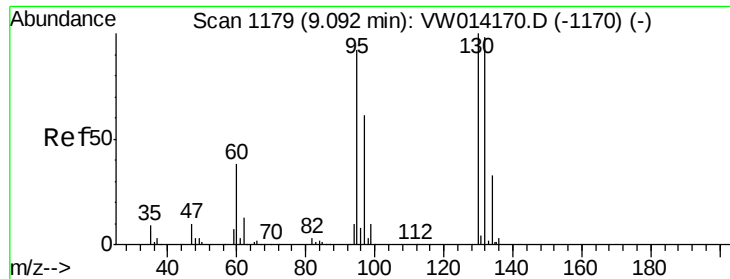

#35
 Trichloroethene
 Concen: 1.618 ug/L
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.25 min
 Lab File: VW014177.D
 Acq: 29 Nov 2019 13:21




Instrument :
 MSVOA_W
 ClientSampleId :


Tot Ion: 95 Resp: 8148
 Ion Ratio Lower Upper
 95 100
 97 0.6 45.1 83.9#
 132 0.0 73.7 136.9#
 130 0.0 76.6 142.2#

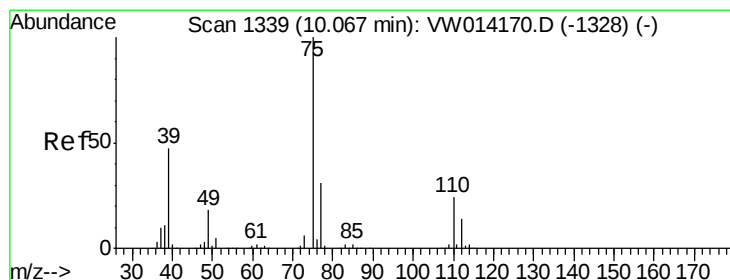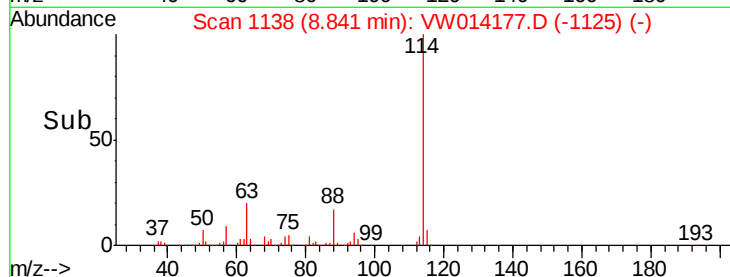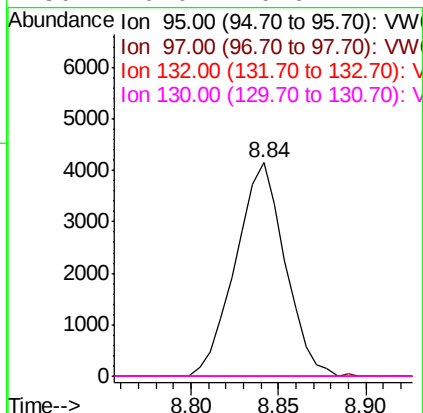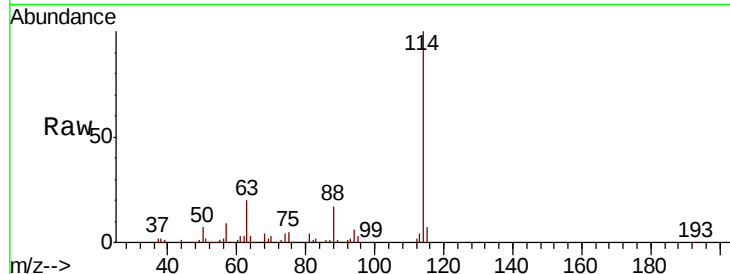

#42
 cis-1,3-Dichloropropene
 Concen: 0.400 ug/L
 RT: 10.03 min Scan# 1333
 Delta R.T. -0.04 min
 Lab File: VW014177.D
 Acq: 29 Nov 2019 13:21

Tgt Ion: 75 Resp: 2868
 Ion Ratio Lower Upper
 75 100
 77 46.5 22.1 41.1#

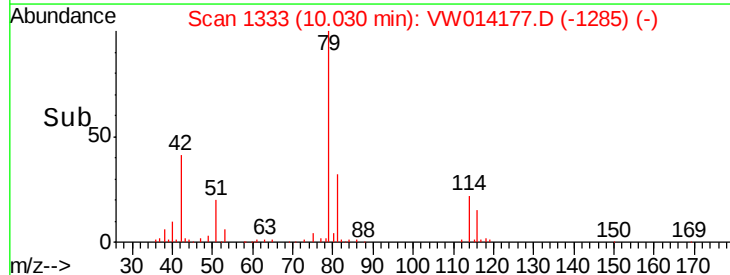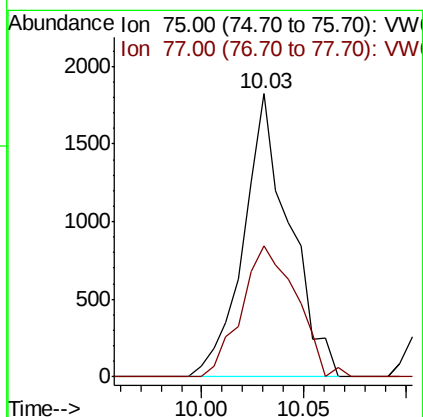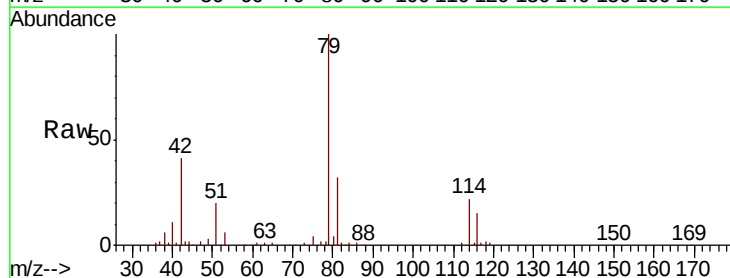

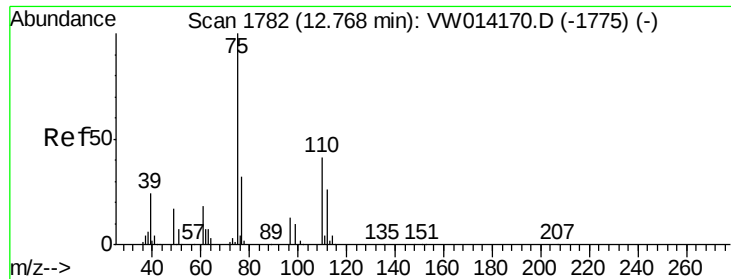

#59

1,2,3-Trichloropropane

Concen: 3.909 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW014177.D

Acq: 29 Nov 2019 13:21

Instrument :

MSVOA_W

ClientSampleId :

Tot Ion: 75 Resp: 11464

Ion Ratio Lower Upper

75 100

77 37.2 25.9 38.9

