

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
 Data File : VW014183.D
 Acq On : 29 Nov 2019 15:59
 Operator : SY/VA
 Sample : K6089-13
 Misc : 4.86G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 C0BR1

Manual Integrations
APPROVED

apatel
 12/2/2019 3:19:34 PM

Quant Time: Nov 30 04:14:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 30 04:10:38 2019
 Response via : Initial Calibration

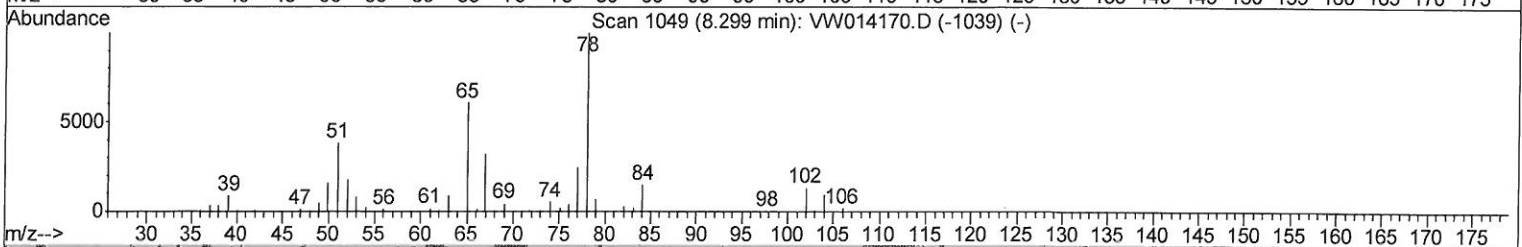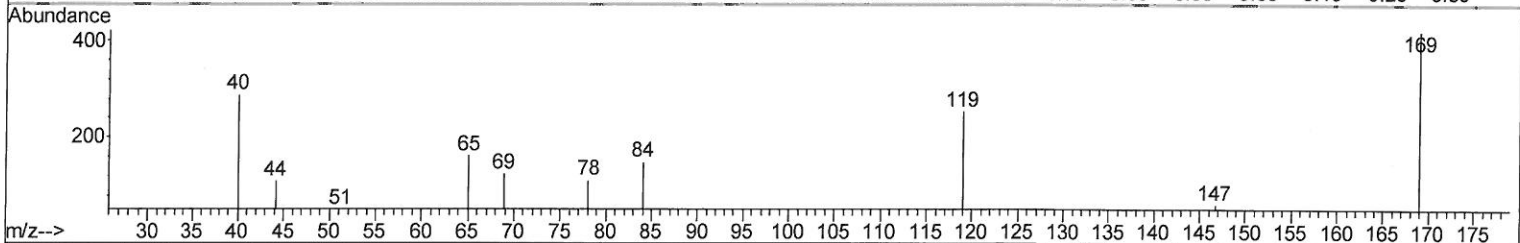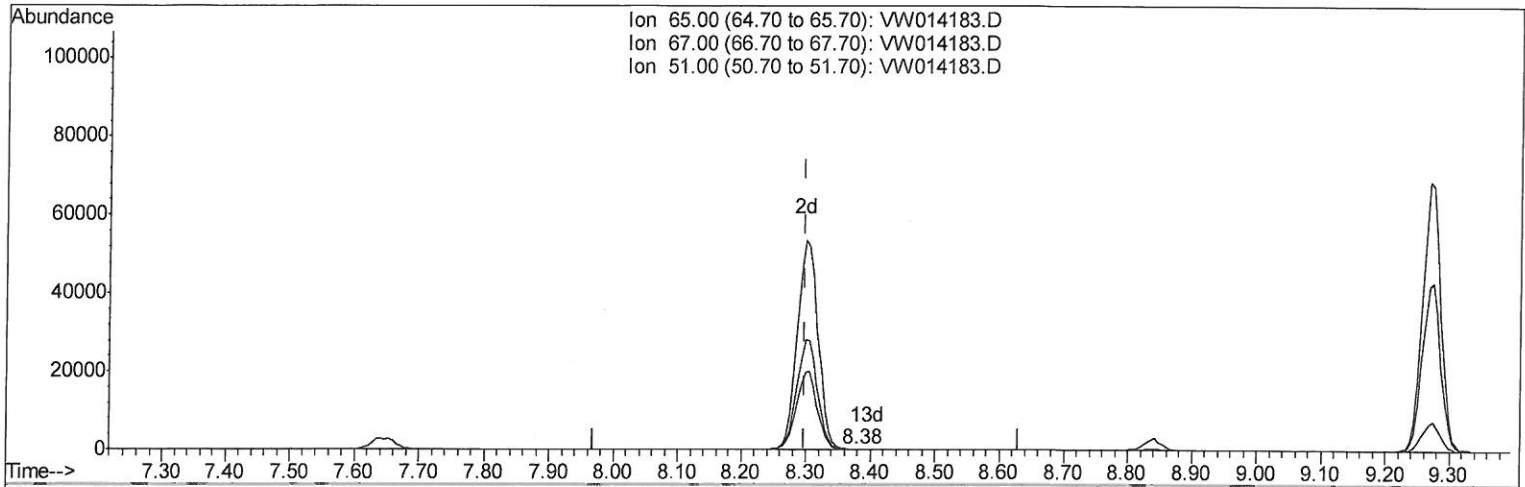

TIC: VW014183.D

(26) 1,2-Dichloroethane-d4 (S)

8.378min (+0.079) 0.03ug/L

response 159

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	45.91
51.00	107.20	129.56
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
 Data File : VW014183.D
 Acq On : 29 Nov 2019 15:59
 Operator : SY/VA
 Sample : K6089-13
 Misc : 4.86G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BR1

Manual Integrations
 APPROVED

apatel
 12/2/2019 3:19:34 PM

Quant Time: Nov 30 04:14:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 30 04:10:38 2019
 Response via : Initial Calibration

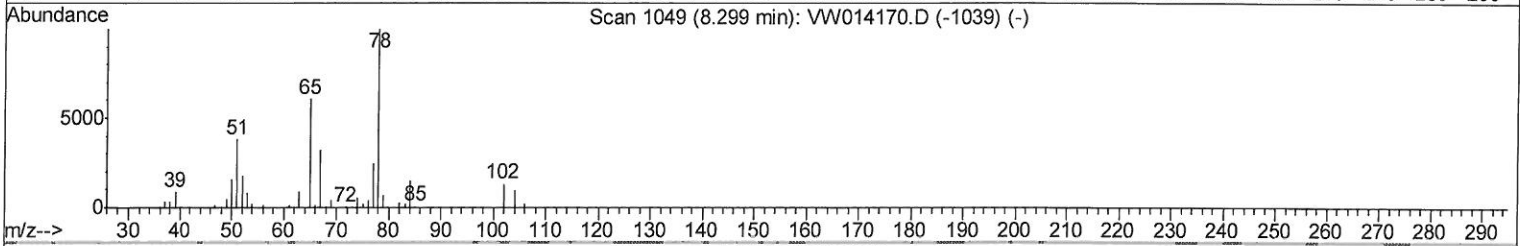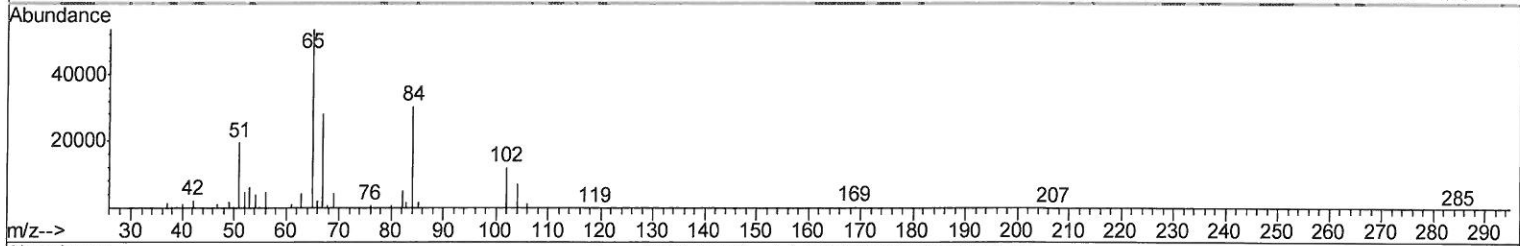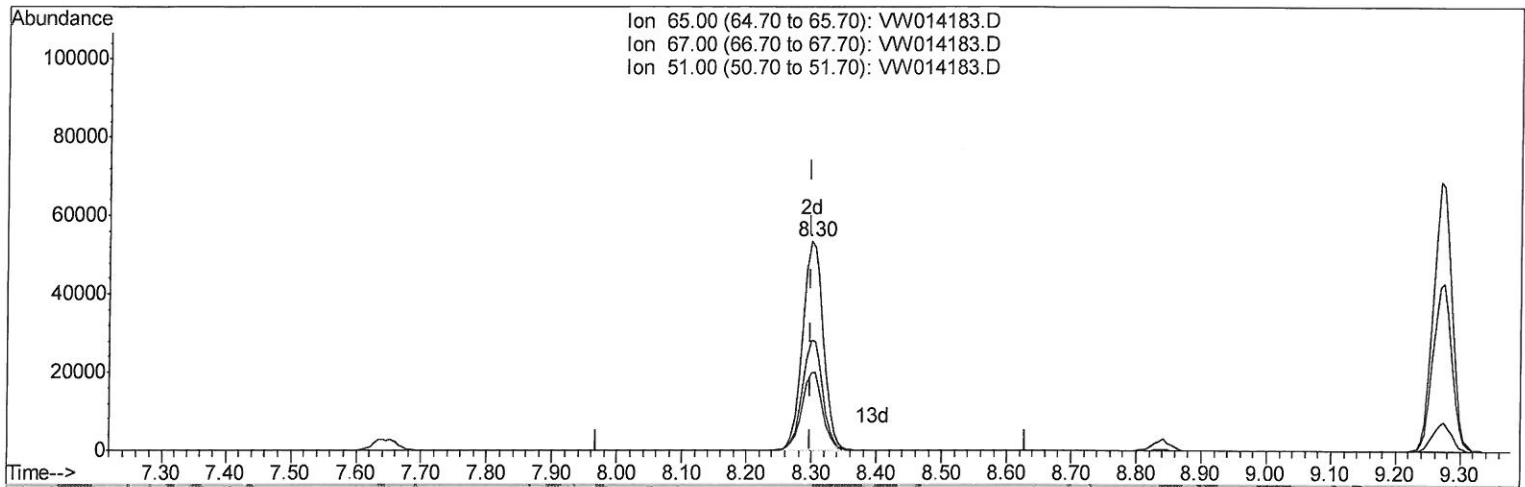

TIC: VW014183.D

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.000) 23.34ug/L m

12/04/19 Sy

response 119606

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	0.06#
51.00	107.20	0.17#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
 Data File : VW014183.D
 Acq On : 29 Nov 2019 15:59
 Operator : SY/VA
 Sample : K6089-13
 Misc : 4.86G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BR1

Manual Integrations
 APPROVED

apatel
 12/2/2019 3:19:34 PM

Quant Time: Nov 30 06:01:00 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 30 04:10:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	331472	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	324251	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	163073	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	69271	13.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.40%
7) Chloroethane-d5	2.88	69	71567	16.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.76%
10) 1,1-Dichloroethene-d2	4.01	63	124965	11.51	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.04%
20) 2-Butanone-d5	7.07	46	75179	48.93	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.86%
24) Chloroform-d	7.64	84	215617	21.16	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.64%
26) 1,2-Dichloroethane-d4	8.30	65	119606m	23.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.36%
29) Benzene-d6	8.27	84	425280	18.49	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.96%
33) 1,2-Dichloropropane-d6	9.27	67	137009	20.33	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.32%
37) Toluene-d8	10.32	98	377472	17.30	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	69.20%
38) trans-1,3-Dichloropropene-	10.57	79	51499	17.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.36%
39) 2-Hexanone-d5	10.92	63	58857	46.05	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.10%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	121931	23.96	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.84%
61) 1,2-Dichlorobenzene-d4	13.85	152	138791	21.18	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.72%

12/04/19 Sg

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
21) 2-Butanone	7.17	43	4302	2.142	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
Data File : VW014183.D
Acq On : 29 Nov 2019 15:59
Operator : SY/VA
Sample : K6089-13
Misc : 4.86G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
C0BR1

Manual Integrations
APPROVED

apatel
12/2/2019 3:19:34 PM

Quant Time: Nov 30 06:01:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 30 04:10:38 2019
Response via : Initial Calibration

