

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
 Data File : VW014185.D
 Acq On : 29 Nov 2019 16:52
 Operator : SY/VA
 Sample : K6089-15
 Misc : 2.92G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BR3

Manual Integrations
 APPROVED

apatel
 12/2/2019 3:19:25 PM

Quant Time: Nov 30 04:14:19 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 30 04:10:38 2019
 Response via : Initial Calibration

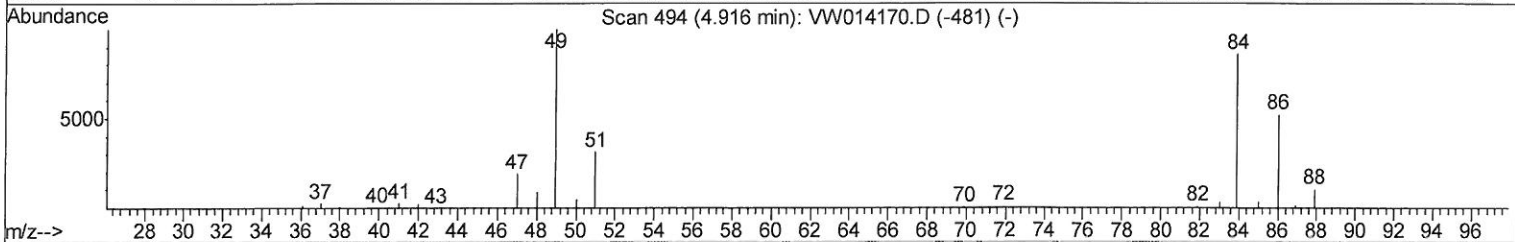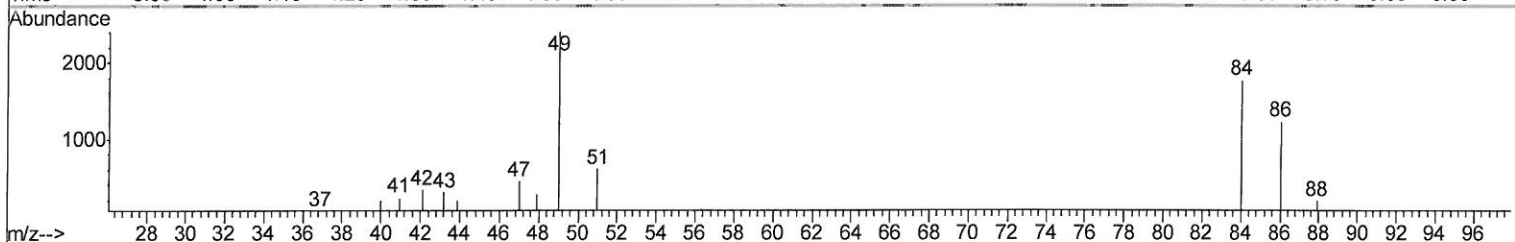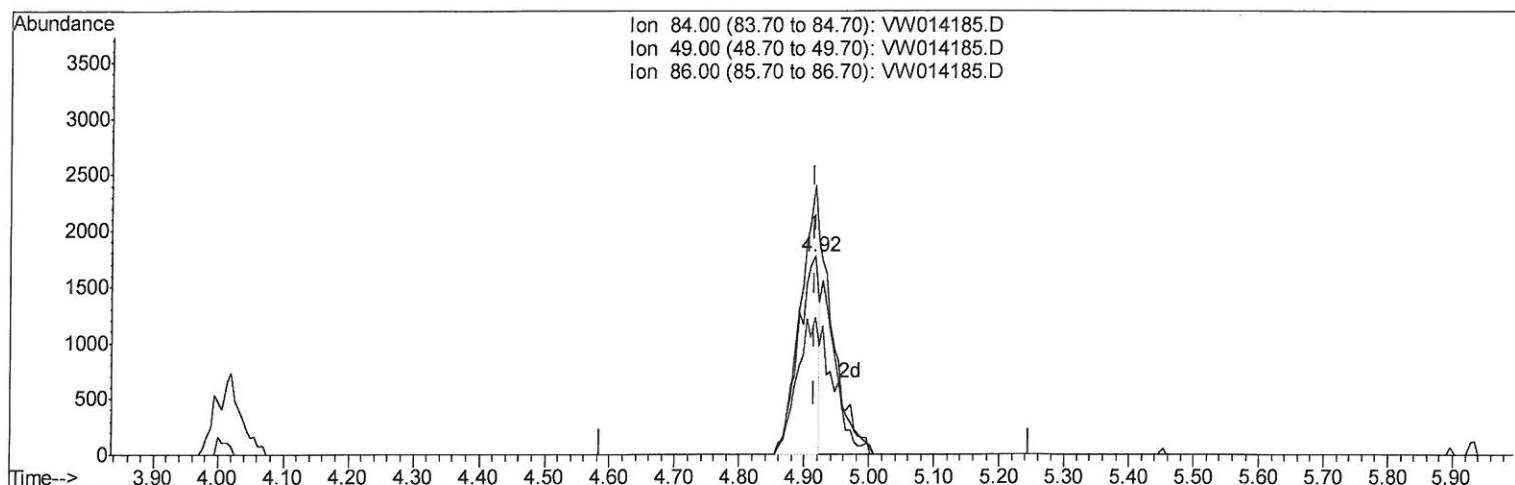

(16) Methylene chloride (T)

4.915min (-0.000) 2.09ug/L

response 3915

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	135.80
86.00	62.40	69.23
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
 Data File : VW014185.D
 Acq On : 29 Nov 2019 16:52
 Operator : SY/VA
 Sample : K6089-15
 Misc : 2.92G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BR3

Manual Integrations
 APPROVED

apatel
 12/2/2019 3:19:25 PM

Quant Time: Nov 30 04:14:19 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 30 04:10:38 2019
 Response via : Initial Calibration

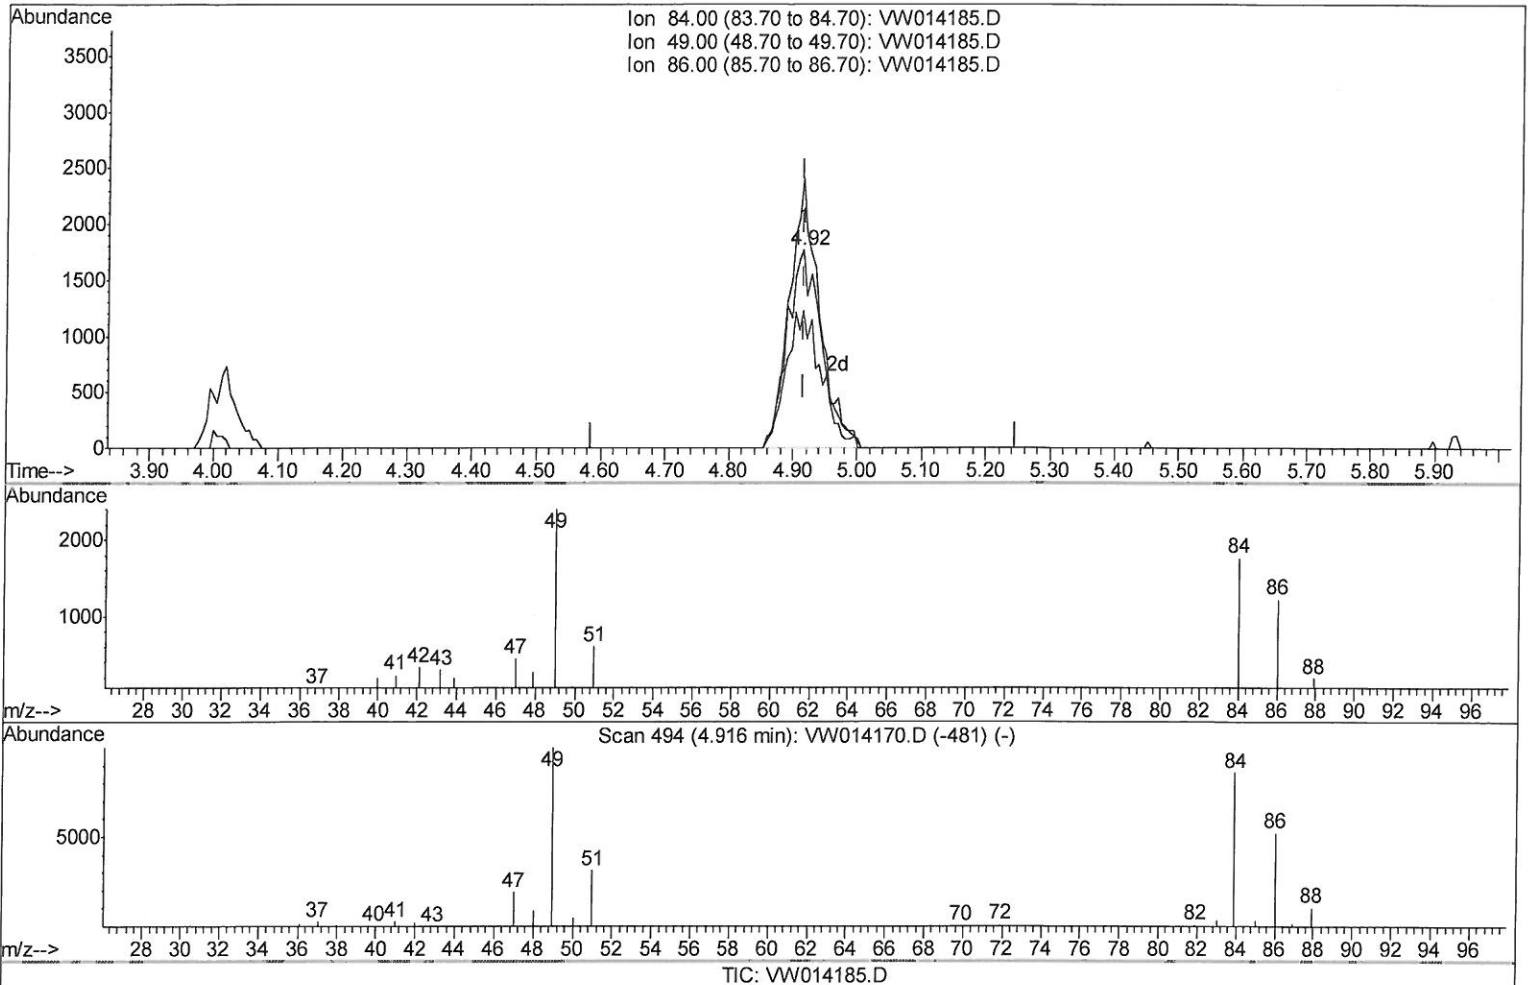

(16) Methylene chloride (T)

4.915min (-0.000) 3.55ug/L m

response 6659

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	135.80
86.00	62.40	69.23
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
 Data File : VW014185.D
 Acq On : 29 Nov 2019 16:52
 Operator : SY/VA
 Sample : K6089-15
 Misc : 2.92G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 C0BR3

Manual Integrations
 APPROVED

apatel
 12/2/2019 3:19:25 PM

Quant Time: Nov 30 04:14:19 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 30 04:10:38 2019
 Response via : Initial Calibration

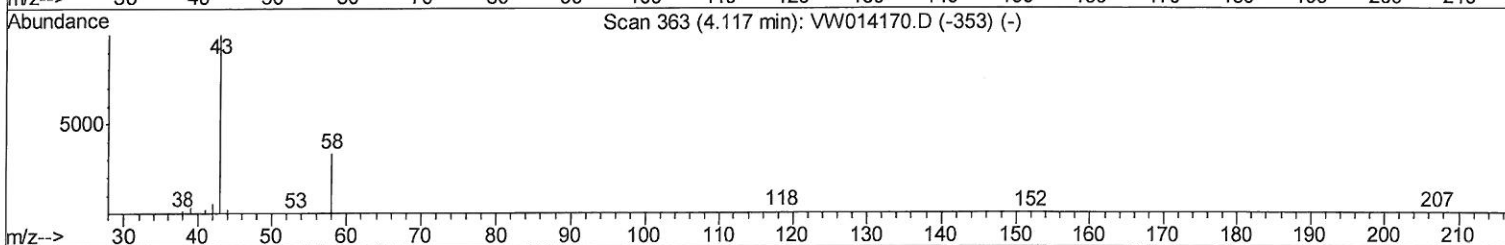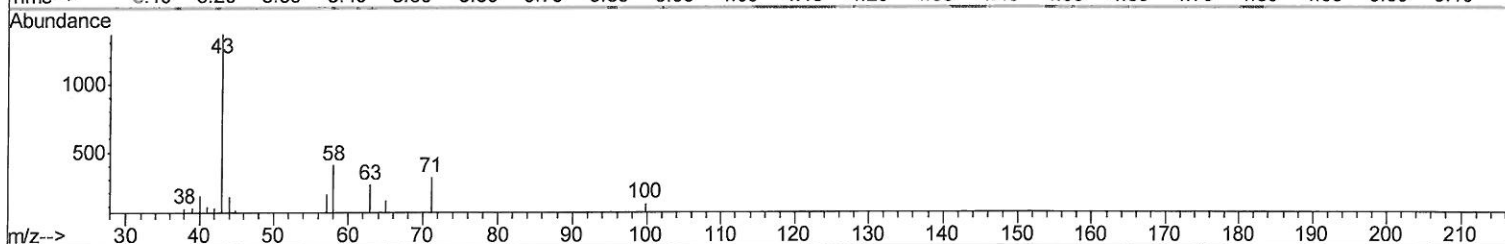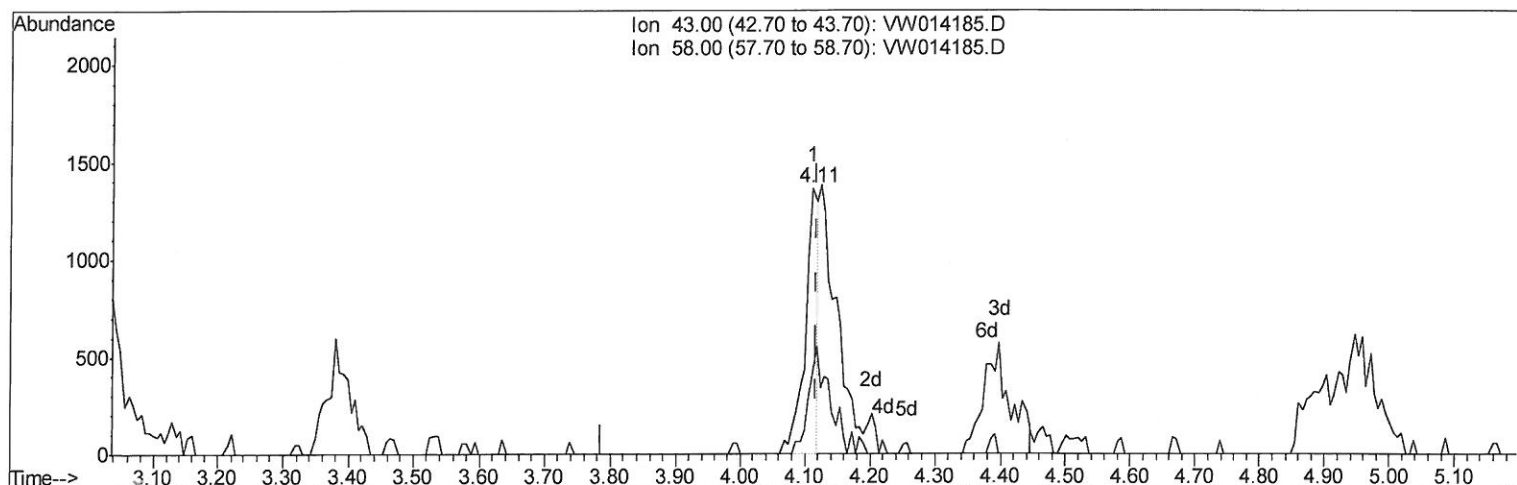

TIC: VW014185.D

(13) Acetone (T)

4.111min (-0.006) 3.92ug/L

response 1802

Ion	Exp%	Act%
43.00	100	100
58.00	32.70	36.85
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
Data File : VW014185.D
Acq On : 29 Nov 2019 16:52
Operator : SY/VA
Sample : K6089-15
Misc : 2.92G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BR3

Manual Integrations
APPROVED

apatel
12/2/2019 3:19:25 PM

Quant Time: Nov 30 04:14:19 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 30 04:10:38 2019
Response via : Initial Calibration

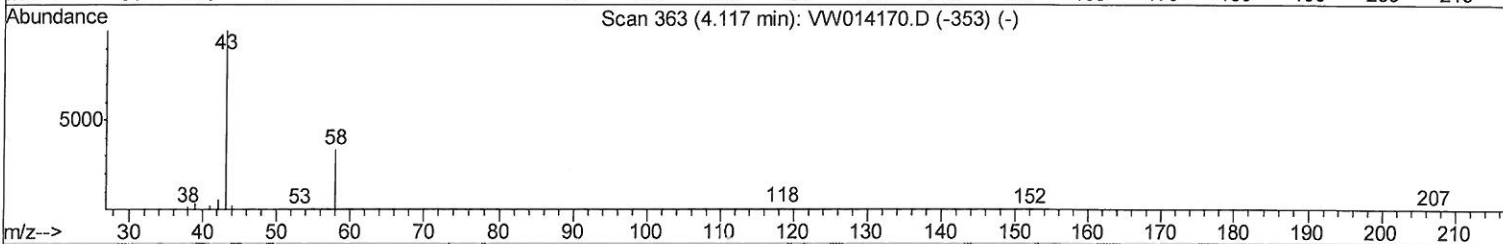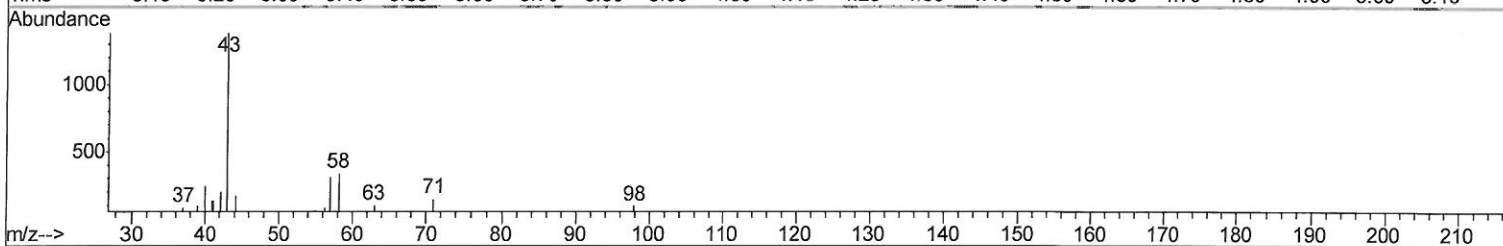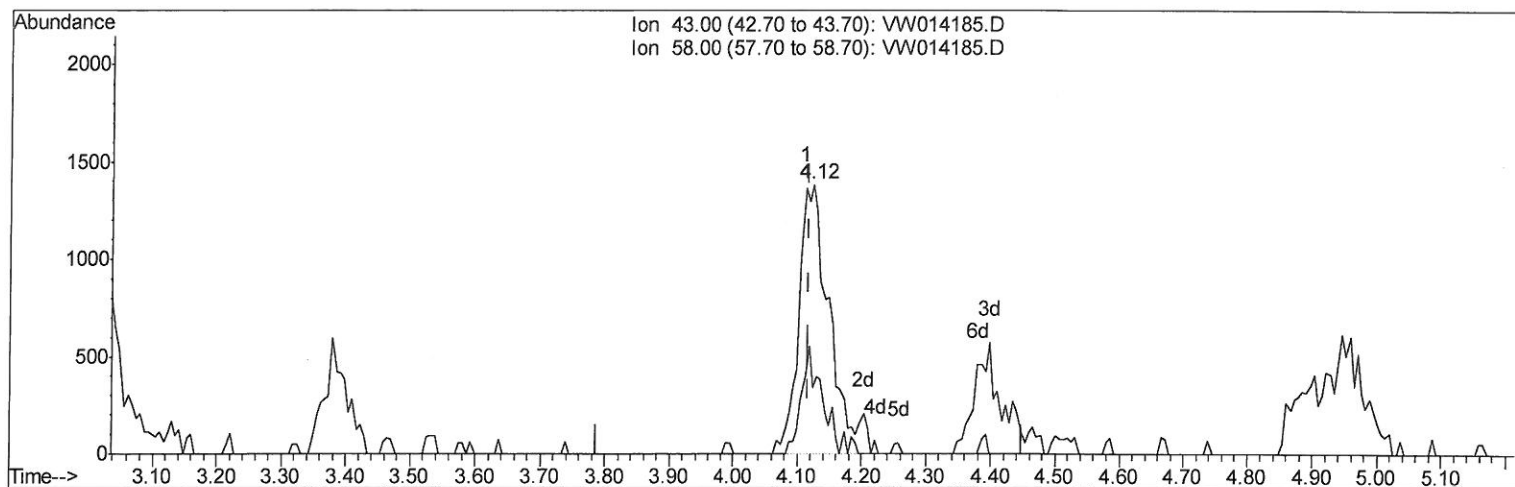

TIC: VW014185.D

(13) Acetone (T)

4.123min (+0.006) 9.99ug/L m

response 4588

Ion	Exp%	Act%
43.00	100	100
58.00	32.70	14.47
0.00	0.00	0.00
0.00	0.00	0.00

12/04/19 sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
 Data File : VW014185.D
 Acq On : 29 Nov 2019 16:52
 Operator : SY/VA
 Sample : K6089-15
 Misc : 2.92G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 C0BR3

Manual Integrations
 APPROVED

apatel
 12/2/2019 3:19:25 PM

Quant Time: Nov 30 06:09:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Nov 30 04:10:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	97400	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	28870	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	2969	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	48809	31.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	125.64%
7) Chloroethane-d5	2.89	69	54702	43.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	173.68%#
10) 1,1-Dichloroethene-d2	4.02	63	66749	20.93	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	83.72%
20) 2-Butanone-d5	7.07	46	47992	106.30	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	212.60%#
24) Chloroform-d	7.65	84	140221	46.82	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	187.28%#
26) 1,2-Dichloroethane-d4	8.31	65	56880	37.78	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	151.12%#
29) Benzene-d6	8.27	84	223897	109.30	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	437.20%#
33) 1,2-Dichloropropane-d6	9.27	67	78630	131.04	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	524.16%#
37) Toluene-d8	10.32	98	79037	40.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	162.76%#
38) trans-1,3-Dichloropropene-	10.57	79	6181	24.05	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.20%
39) 2-Hexanone-d5	10.93	63	12963	113.92	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	227.84%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	35371	78.06	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	312.24%#
61) 1,2-Dichlorobenzene-d4	13.85	152	4072	34.14	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	136.56%#

Target Compounds

					Ovalue	
13) Acetone	4.12	43	4588m	9.987	ug/L	98
16) Methylene chloride	4.92	84	6659m	3.551	ug/L	94
30) Cyclohexane	7.95	56	5606	6.068	ug/L	90
36) Methylcyclohexane	9.34	83	10704	10.568	ug/L	94
44) Toluene	10.39	91	9723	4.211	ug/L	90
54) m,p-Xylene	11.83	106	1668	1.694	ug/L	94
55) o-xylene	12.16	106	1719	1.864	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112919\
Data File : VW014185.D
Acq On : 29 Nov 2019 16:52
Operator : SY/VA
Sample : K6089-15
Misc : 2.92G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BR3

Manual Integrations
APPROVED

apatel
12/2/2019 3:19:25 PM

Quant Time: Nov 30 06:09:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Sat Nov 30 04:10:38 2019
Response via : Initial Calibration

