


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW112919\
 Data File : VW014169.D
 Acq On : 29 Nov 2019 08:48
 Operator : SY/VA
 Sample : BFB30
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB30

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Title : VOC Analysis
 Last Update : Sat Nov 30 04:10:38 2019

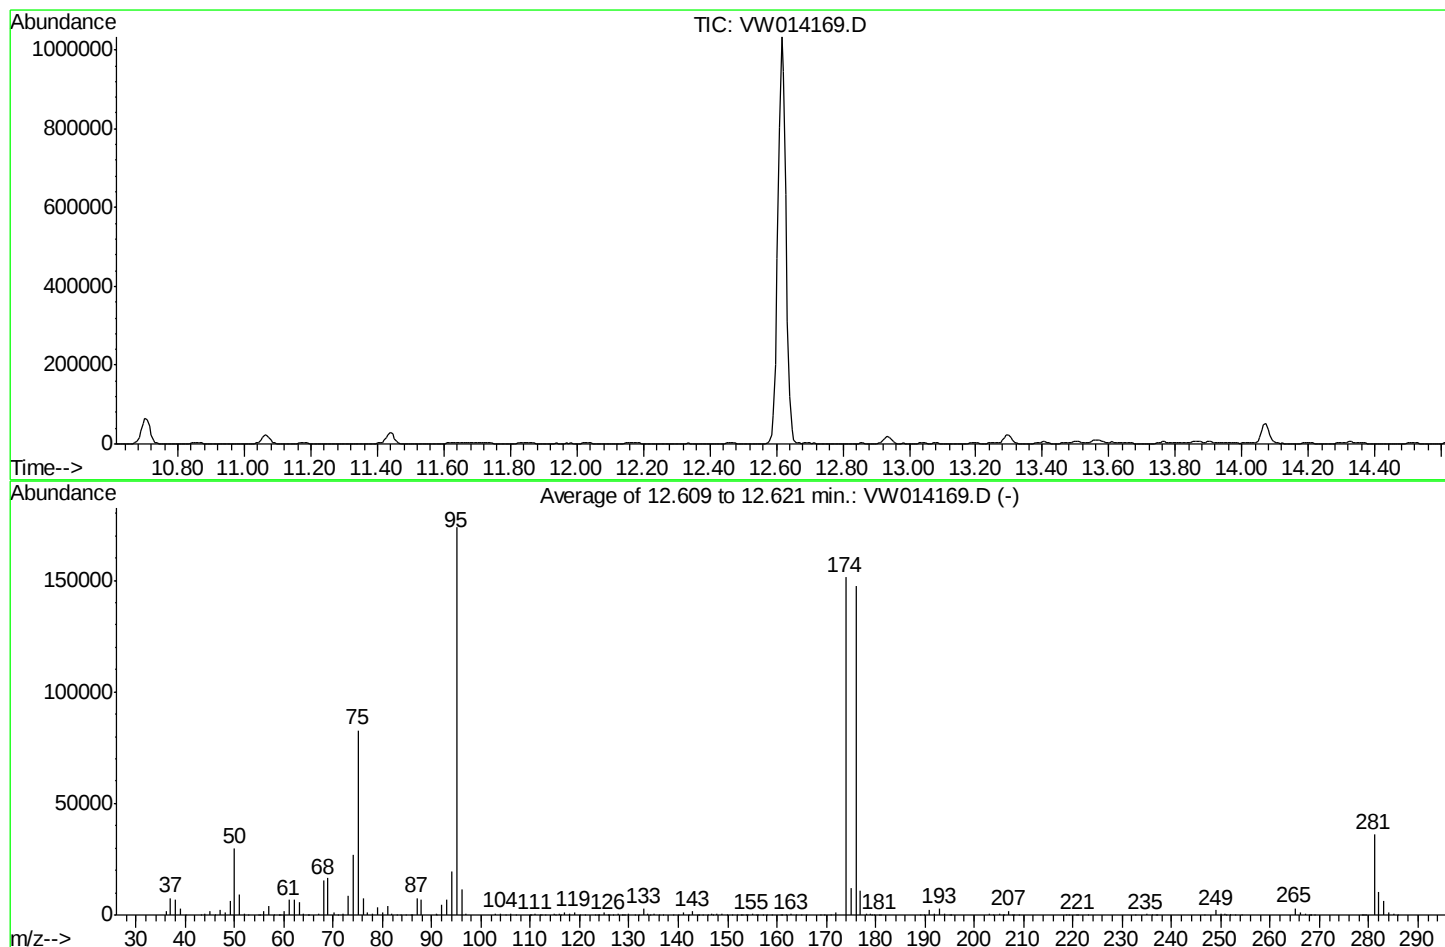

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	29701	PASS
75	95	30	80	47.7	82874	PASS
95	95	100	100	100.0	173802	PASS
96	95	5	9	6.5	11292	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.2	151469	PASS
175	174	5	9	8.0	12146	PASS
176	174	95	101	97.3	147368	PASS
177	176	5	9	7.4	10880	PASS

m/z	Abundance
36.10	1647.0
37.10	6983.0
38.10	6137.0
39.10	2233.0
40.10	323.0
43.00	144.0
44.00	658.0
45.00	1511.0
46.10	142.0
47.10	1784.0
48.10	913.0
49.10	5374.0
50.00	26248.0
51.00	8543.0
52.00	401.0
52.80	113.0
54.90	235.0
55.20	255.0
56.00	1741.0
57.00	3746.0
58.10	228.0
59.00	371.0
60.10	1303.0
61.00	6190.0
62.00	6319.0
63.00	4790.0
64.00	604.0
64.90	660.0
67.00	421.0
68.00	12563.0
69.00	15094.0
70.00	1028.0
71.00	112.0
72.10	685.0
73.00	8184.0
74.00	23296.0
75.00	71144.0
76.00	6421.0
77.00	1179.0
77.90	483.0
78.90	3361.0
80.00	852.0
81.00	3559.0
82.00	842.0
83.60	113.0
84.80	62.0
87.00	6568.0
88.00	5513.0
90.90	329.0
92.10	3685.0
93.00	5828.0
94.00	15595.0
95.00	147968.0
96.00	10074.0
97.00	315.0
103.00	737.0
104.00	631.0
104.90	301.0
105.90	403.0
107.00	171.0
110.10	474.0
110.90	302.0
111.90	178.0
112.20	173.0
114.90	391.0
115.20	362.0
115.90	440.0
116.90	918.0
117.90	727.0
118.90	1246.0
120.10	89.0
121.10	101.0
125.00	1217.0
125.80	656.0
127.90	575.0
128.80	196.0
129.80	485.0
131.10	215.0
132.00	170.0
133.00	3753.0
133.80	781.0
134.30	473.0
135.00	412.0
136.90	353.0
139.00	80.0
140.90	1077.0
141.90	179.0
142.90	1289.0
144.10	84.0
144.90	299.0
145.90	288.0
146.80	472.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

147.10	504.0
147.80	475.0
148.90	438.0
149.90	136.0
151.00	99.0
152.00	52.0
152.70	64.0
153.70	68.0
155.00	414.0
155.80	80.0
157.10	188.0
159.00	230.0
160.80	338.0
161.90	114.0
162.90	774.0
163.90	111.0
165.10	341.0
165.90	55.0
168.80	84.0
171.00	197.0
171.90	890.0
173.90	113800.0
175.00	9279.0
175.90	114424.0
177.00	8508.0
178.00	523.0
178.80	624.0
179.90	126.0
180.80	74.0
181.10	69.0
189.10	432.0
191.00	3159.0
192.00	841.0
193.00	3370.0
194.00	795.0
195.00	470.0
203.10	326.0
203.90	194.0
205.00	733.0
205.90	277.0
207.00	2116.0
208.10	535.0
209.00	273.0
218.70	71.0
219.20	163.0
221.10	113.0
223.10	56.0
232.70	65.0
235.00	611.0
236.10	149.0
249.00	2779.0
250.00	856.0
250.90	1262.0
251.80	304.0
253.00	267.0
265.00	4132.0
266.00	1164.0
267.10	1088.0
267.90	147.0
268.30	163.0
269.00	112.0
278.60	188.0
279.30	334.0
281.10	42968.0
282.10	13427.0
283.00	6780.0
284.00	1753.0
285.10	751.0
285.80	127.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

m/z	Abundance
36.00	1514.0
37.00	8639.0
38.10	7935.0
39.00	3205.0
39.90	364.0
41.10	72.0
43.10	202.0
44.00	949.0
45.10	1874.0
45.90	142.0
47.10	2382.0
48.00	1134.0
49.10	7291.0
50.00	33256.0
51.10	10538.0
52.10	563.0
52.80	56.0
55.00	461.0
56.00	2238.0
57.00	4542.0
58.10	291.0
58.80	183.0
59.20	285.0
60.00	2046.0
61.00	7356.0
62.10	7861.0
63.10	6424.0
64.00	770.0
65.10	477.0
67.00	547.0
68.00	17936.0
69.00	18936.0
70.00	1416.0
71.00	175.0
72.00	1050.0
73.00	9881.0
74.00	30304.0
75.00	93816.0
76.10	8130.0
77.00	932.0
78.00	730.0
79.00	3469.0
80.10	1335.0
81.00	4566.0
81.90	902.0
83.00	134.0
83.60	95.0
85.70	158.0
87.00	8889.0
88.00	8272.0
91.10	429.0
92.00	4845.0
93.10	8003.0
94.00	23552.0
95.00	195328.0
96.00	13002.0
97.00	571.0
103.00	739.0
103.90	916.0
105.00	214.0
106.00	527.0
107.10	140.0
109.80	182.0
110.20	185.0
111.00	381.0
111.90	174.0
113.00	159.0
114.90	517.0
115.90	582.0
117.00	1402.0
117.90	996.0
118.90	1312.0
120.10	91.0
123.00	56.0
123.70	59.0
125.00	1023.0
126.10	190.0
126.80	244.0
127.80	685.0
128.90	428.0
129.90	561.0
131.20	179.0
131.90	115.0
133.10	2820.0
133.80	554.0
135.00	631.0
136.10	54.0
137.00	370.0
139.00	85.0
139.90	114.0
140.90	1380.0
142.00	180.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

142.90	1747.0
144.00	132.0
144.80	323.0
145.70	265.0
146.90	421.0
147.90	546.0
148.90	291.0
149.90	337.0
152.00	78.0
152.80	127.0
154.00	129.0
154.90	546.0
155.80	122.0
156.90	355.0
159.00	271.0
160.80	297.0
161.90	148.0
162.80	602.0
164.90	330.0
168.90	51.0
170.90	224.0
171.90	1074.0
173.90	165504.0
175.00	13674.0
176.00	162304.0
177.00	11686.0
178.10	762.0
178.90	539.0
179.70	86.0
189.10	274.0
190.00	85.0
191.00	2636.0
192.00	666.0
193.00	3051.0
194.00	500.0
195.20	346.0
203.00	355.0
204.00	149.0
205.10	690.0
206.10	174.0
207.00	2126.0
207.90	362.0
209.10	337.0
218.70	106.0
221.00	200.0
234.90	502.0
235.90	85.0
236.80	123.0
246.80	76.0
249.10	2141.0
249.90	508.0
251.20	782.0
252.00	262.0
253.00	96.0
254.20	56.0
265.10	3225.0
266.10	756.0
267.10	925.0
268.00	267.0
268.90	53.0
278.90	236.0
281.10	39736.0
282.10	10442.0
283.00	7162.0
284.10	1337.0
285.20	320.0
285.70	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

m/z	Abundance
36.00	1727.0
37.10	7615.0
38.10	6442.0
39.10	2495.0
39.90	253.0
41.90	60.0
43.00	141.0
44.00	743.0
45.00	1492.0
45.90	51.0
47.00	2642.0
48.00	1068.0
49.10	6106.0
50.00	29600.0
51.10	9241.0
51.90	409.0
55.00	270.0
56.00	2161.0
57.00	3535.0
57.90	201.0
58.80	290.0
59.90	1722.0
61.00	6877.0
62.00	6812.0
63.00	5403.0
64.00	538.0
65.00	401.0
67.10	659.0
68.00	16250.0
69.00	15709.0
70.10	1279.0
71.00	98.0
72.10	871.0
73.00	7222.0
74.10	27936.0
75.00	83664.0
76.00	7180.0
77.00	1104.0
77.90	679.0
79.00	3487.0
80.00	1185.0
81.00	3563.0
81.80	660.0
82.90	138.0
85.90	394.0
86.90	7676.0
87.90	6549.0
91.00	530.0
92.00	4872.0
93.00	6413.0
94.00	20280.0
95.00	178112.0
96.00	10802.0
96.90	278.0
102.90	448.0
103.90	852.0
104.80	168.0
105.80	395.0
107.10	106.0
109.80	185.0
110.90	288.0
112.30	80.0
113.00	106.0
115.00	257.0
116.10	646.0
116.90	928.0
117.90	725.0
119.00	1180.0
123.90	165.0
124.80	464.0
124.90	458.0
125.90	212.0
126.80	157.0
128.00	721.0
128.60	299.0
129.10	195.0
130.00	653.0
131.00	288.0
132.00	92.0
133.20	1302.0
133.80	427.0
134.90	350.0
137.00	183.0
138.90	67.0
139.90	96.0
141.00	1478.0
141.90	225.0
142.90	1561.0
143.80	160.0
144.90	253.0
145.90	353.0
146.80	239.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

147.90	634.0
148.90	220.0
149.80	247.0
152.00	121.0
152.70	71.0
153.10	61.0
154.00	144.0
154.90	420.0
156.00	79.0
157.10	343.0
158.00	52.0
158.90	184.0
161.00	241.0
163.00	231.0
164.90	207.0
168.90	96.0
169.70	77.0
172.00	858.0
173.90	175104.0
175.00	13486.0
175.90	165376.0
176.90	12448.0
178.10	511.0
179.10	282.0
179.70	79.0
189.00	83.0
189.90	57.0
191.00	1397.0
191.80	307.0
193.00	1501.0
193.90	248.0
195.00	152.0
203.00	397.0
205.00	584.0
206.00	176.0
207.00	1283.0
207.70	247.0
209.10	277.0
218.80	70.0
220.80	110.0
235.00	215.0
237.10	108.0
249.00	1550.0
250.00	354.0
250.90	713.0
251.90	198.0
252.90	151.0
265.00	1857.0
266.00	758.0
267.00	428.0
268.10	107.0
278.50	65.0
279.10	166.0
279.50	170.0
281.10	25784.0
282.00	6732.0
283.10	4846.0
284.00	862.0
285.10	267.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30

Scan 1749 (12.567 min): VW014169.D
BFB30

m/z	Abundance
36.10	148.0
40.10	312.0
41.10	98.0
41.90	61.0
43.10	64.0
44.00	274.0
54.90	84.0
56.00	115.0
281.10	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB30