

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112921\
 Data File : VW020976.D
 Acq On : 29 Nov 2021 12:09
 Operator : SY/VA
 Sample : M4839-04
 Misc : 5.68g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQP5

Quant Time: Nov 30 00:56:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 30 00:55:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	113068	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	99488	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	45618	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	21863	16.670	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.680%
7) Chloroethane-d5	2.891	69	15886	18.781	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.120%
11) 1,1-Dichloroethene-d2	4.019	63	31332	12.347	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.400%
21) 2-Butanone-d5	7.080	46	13698	41.844	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.680%
24) Chloroform-d	7.653	84	55912	19.626	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.520%
26) 1,2-Dichloroethane-d4	8.305	65	29595	20.466	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.880%
32) Benzene-d6	8.274	84	104698	19.967	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.880%
36) 1,2-Dichloropropane-d6	9.274	67	31298	20.961	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.840%
41) Toluene-d8	10.323	98	96555	18.553	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.200%
43) trans-1,3-Dichloroprop...	10.579	79	13625	19.306	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.240%
47) 2-Hexanone-d5	10.926	63	10542	42.570	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.140%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	25125	21.966	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.880%
66) 1,2-Dichlorobenzene-d4	13.859	152	31731	19.516	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.080%
Target Compounds						
13) Acetone	4.123	43	3658	12.516	ug/L	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112921\
Data File : VW020976.D
Acq On : 29 Nov 2021 12:09
Operator : SY/VA
Sample : M4839-04
Misc : 5.68g/10.0mL/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ESQP5

Quant Time: Nov 30 00:56:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 30 00:55:38 2021
Response via : Initial Calibration

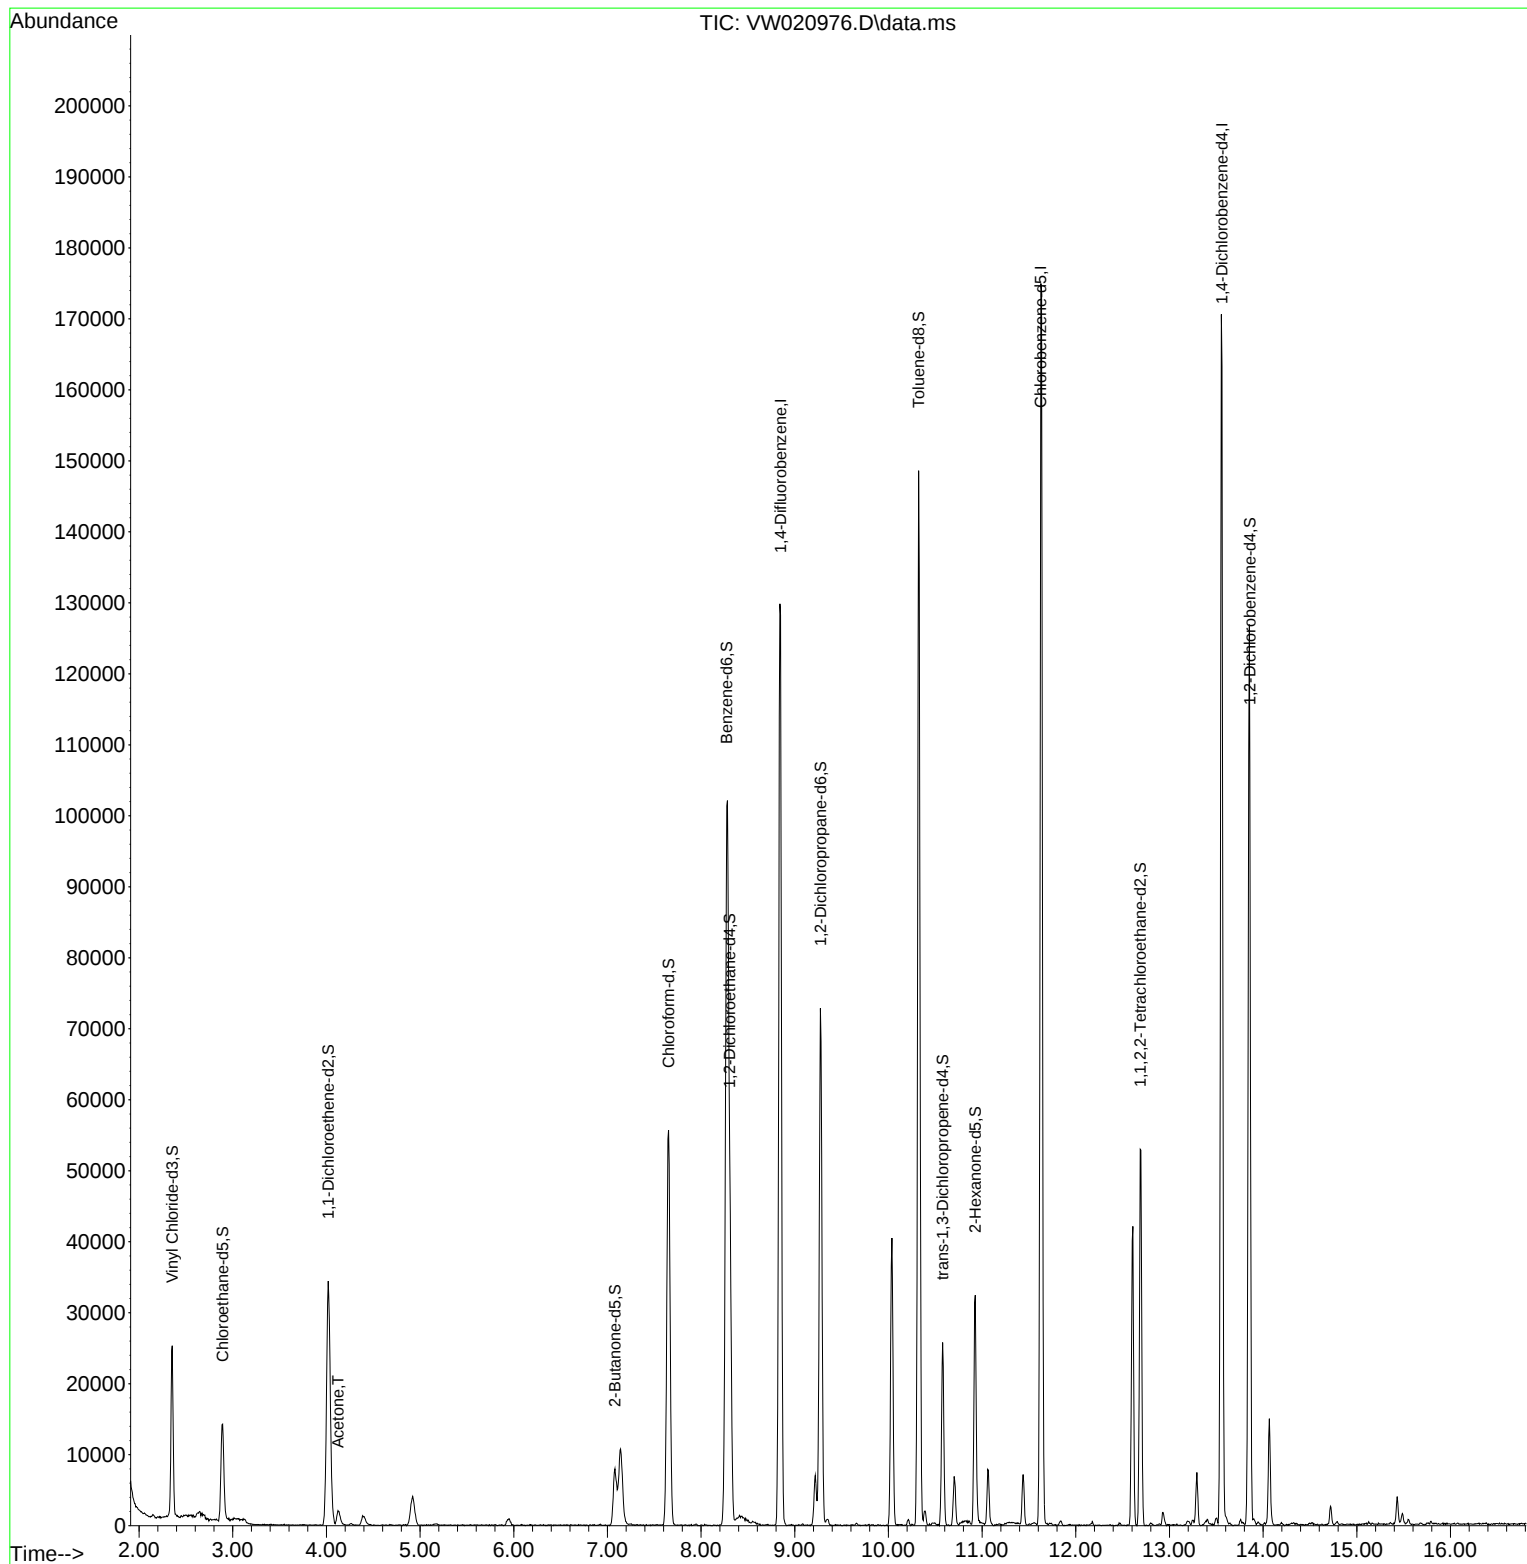

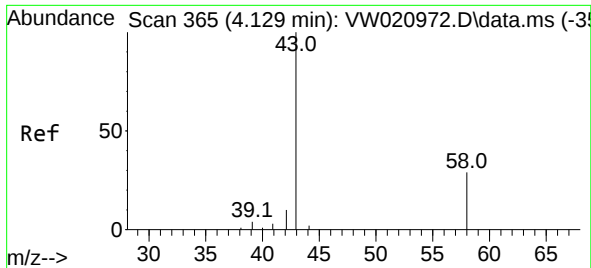

#13
 Acetone
 Concen: 12.516 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW020976.D
 Acq: 29 Nov 2021 12:09

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQP5

Tgt Ion: 43 Resp: 3658
 Ion Ratio Lower Upper
 43 100
 58 16.6 0.0 52.8

