
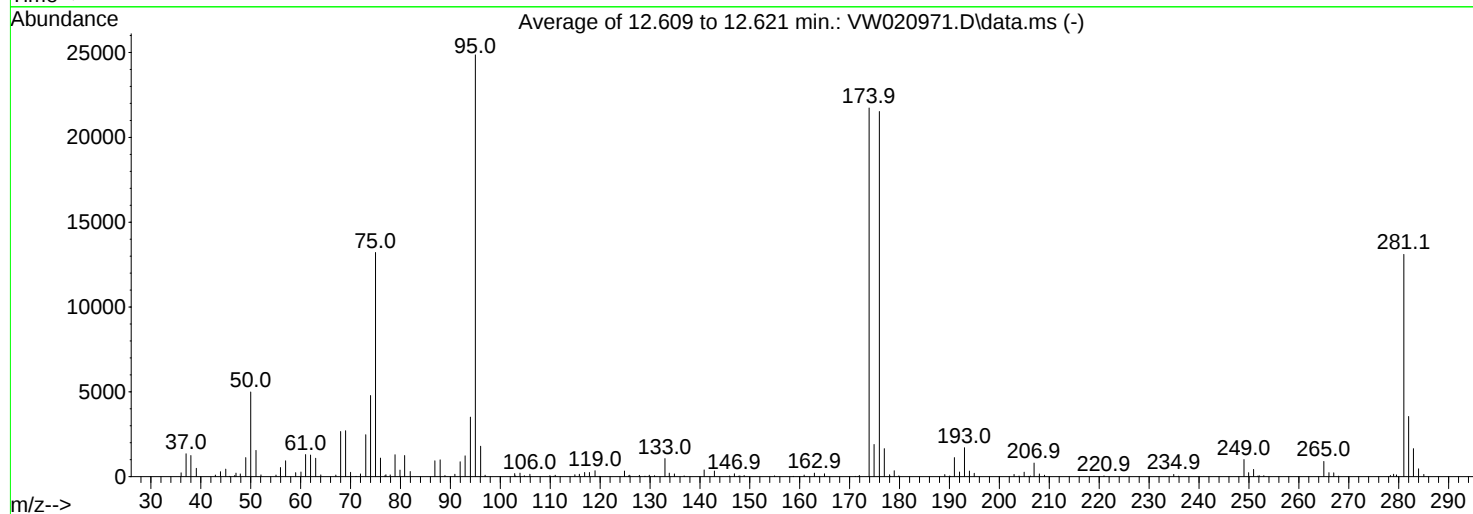


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112921\
 Data File : VW020971.D
 Acq On : 29 Nov 2021 08:40
 Operator : SY/VA
 Sample : BFB466
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB466

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Title : SFAM01.0
 Last Update : Wed Dec 01 00:01:42 2021

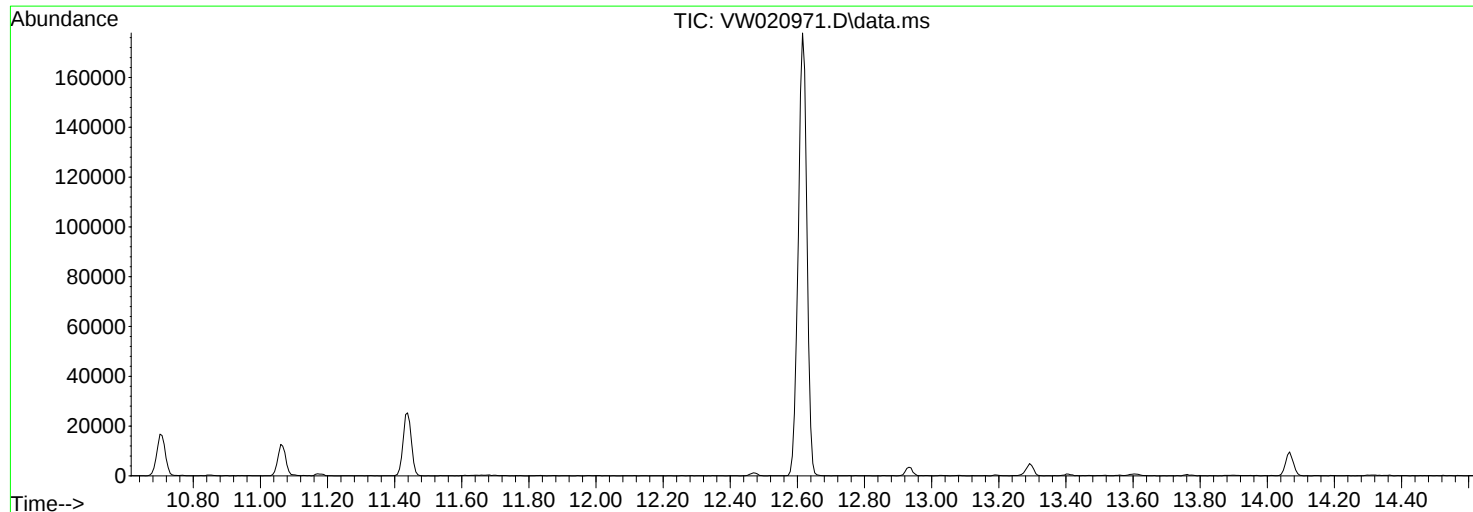

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	4987	PASS
75	95	30	80	53.2	13218	PASS
95	95	100	100	100.0	24864	PASS
96	95	5	9	7.2	1795	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.4	21733	PASS
175	174	5	9	8.7	1900	PASS
176	174	95	105	99.0	21526	PASS
177	176	5	10	7.7	1651	PASS

m/z	Abundance
40.00	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

m/z	Abundance
36.00	204.0
37.00	1173.0
38.00	1116.0
39.10	485.0
42.90	162.0
43.90	312.0
45.00	505.0
45.80	56.0
46.80	188.0
47.20	143.0
47.90	145.0
49.00	884.0
50.00	3928.0
51.00	1287.0
52.00	92.0
55.00	98.0
56.00	492.0
57.00	808.0
59.00	380.0
60.10	269.0
61.00	1229.0
62.00	1155.0
63.00	842.0
64.20	92.0
67.00	71.0
68.00	2055.0
69.00	2136.0
70.00	214.0
72.10	135.0
73.10	3001.0
74.00	4012.0
75.00	11085.0
76.00	867.0
76.90	159.0
78.10	119.0
78.90	1079.0
79.90	329.0
80.80	1045.0
81.90	306.0
86.90	698.0
88.00	862.0
89.00	106.0
90.90	144.0
92.00	727.0
93.00	977.0
94.00	2682.0
95.00	20392.0
96.10	1566.0
96.90	86.0
102.90	371.0
104.00	201.0
104.80	92.0
105.90	105.0
110.00	102.0
111.00	129.0
115.00	151.0
115.90	130.0
116.90	259.0
117.90	318.0
119.00	464.0
124.90	553.0
125.70	140.0
126.10	106.0
130.90	53.0
133.00	1609.0
133.80	395.0
134.90	176.0
136.80	69.0
140.90	335.0
142.90	238.0
145.90	53.0
146.90	249.0
148.00	77.0
148.90	115.0
160.90	118.0
162.90	262.0
163.90	56.0
165.00	286.0
171.70	68.0
172.10	61.0
173.90	16800.0
174.90	1504.0
176.00	15137.0
176.90	1407.0
178.00	234.0
178.90	517.0
179.90	66.0
189.00	203.0
190.00	111.0
191.00	1591.0
192.00	378.0
193.00	2521.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

194.00	499.0
194.90	247.0
203.00	215.0
204.00	64.0
205.00	427.0
206.20	105.0
206.90	1012.0
208.00	199.0
209.10	135.0
221.00	87.0
235.00	167.0
235.90	80.0
249.00	1544.0
250.00	381.0
250.90	635.0
251.80	110.0
252.10	103.0
253.00	101.0
265.00	1004.0
266.00	397.0
267.00	352.0
268.00	75.0
278.30	125.0
279.00	215.0
281.10	18032.0
282.00	5603.0
283.00	1940.0
284.00	730.0
285.00	236.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

m/z	Abundance
36.00	269.0
37.00	1552.0
38.00	1455.0
39.10	528.0
40.20	63.0
42.90	66.0
44.00	319.0
45.00	485.0
47.00	288.0
47.90	156.0
49.00	1246.0
50.00	5717.0
51.10	1630.0
52.00	109.0
55.10	95.0
56.00	570.0
57.00	983.0
59.00	176.0
60.00	286.0
61.00	1451.0
62.00	1294.0
63.00	1258.0
64.00	140.0
67.10	104.0
68.00	3088.0
69.00	3170.0
70.00	302.0
71.10	51.0
72.00	187.0
73.10	2541.0
74.00	5187.0
75.00	14617.0
76.00	1232.0
77.10	124.0
77.90	115.0
78.90	1444.0
79.90	421.0
80.90	1372.0
82.00	269.0
86.90	977.0
87.90	995.0
88.80	83.0
90.90	131.0
91.90	916.0
93.00	1331.0
94.00	3898.0
95.00	27192.0
96.00	1995.0
97.00	92.0
102.90	176.0
103.90	193.0
104.80	69.0
106.00	182.0
109.90	82.0
111.00	121.0
114.90	83.0
115.80	145.0
116.90	224.0
117.80	239.0
119.00	357.0
119.90	53.0
124.90	304.0
125.90	75.0
128.00	74.0
129.00	77.0
129.90	109.0
130.90	56.0
133.00	1092.0
133.90	240.0
134.90	165.0
140.80	387.0
142.90	346.0
146.00	67.0
146.90	126.0
148.00	79.0
148.80	72.0
155.00	82.0
158.70	52.0
160.90	113.0
163.00	212.0
164.90	142.0
171.10	56.0
173.90	24312.0
174.90	2067.0
175.90	23488.0
177.00	1712.0
178.00	115.0
179.00	384.0
179.80	85.0
189.10	105.0
190.20	67.0
191.00	1163.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

192.00	276.0
193.00	1733.0
194.00	327.0
195.00	250.0
202.90	106.0
203.90	63.0
204.90	218.0
205.80	56.0
207.00	980.0
208.00	196.0
209.00	115.0
220.90	55.0
234.90	154.0
249.00	957.0
249.90	204.0
251.00	430.0
252.00	75.0
253.00	70.0
265.00	1093.0
266.10	167.0
267.00	214.0
278.40	78.0
279.00	143.0
279.50	154.0
281.00	12809.0
282.00	3407.0
282.90	1681.0
284.00	435.0
285.10	106.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

m/z	Abundance
36.10	204.0
37.10	1326.0
38.00	1174.0
39.10	458.0
40.10	56.0
43.00	51.0
44.00	249.0
45.00	345.0
47.10	193.0
47.90	172.0
49.00	1248.0
50.00	5317.0
51.00	1730.0
52.10	108.0
55.00	90.0
55.90	543.0
57.00	1020.0
59.10	143.0
60.10	265.0
61.00	1226.0
62.00	1386.0
63.00	1160.0
63.90	87.0
67.10	120.0
68.00	2835.0
69.00	2808.0
70.00	249.0
71.90	163.0
73.00	1878.0
74.00	5137.0
75.00	13953.0
76.00	1194.0
77.10	212.0
77.90	83.0
78.90	1356.0
79.90	399.0
80.90	1321.0
81.90	342.0
86.90	1139.0
87.90	1107.0
90.90	164.0
92.00	980.0
92.90	1363.0
94.00	3944.0
95.00	27008.0
96.00	1824.0
97.00	81.0
103.10	110.0
103.90	220.0
106.00	138.0
110.70	70.0
114.90	102.0
115.80	140.0
116.90	259.0
117.90	170.0
119.00	230.0
124.90	141.0
125.90	62.0
127.80	142.0
129.80	133.0
130.90	67.0
133.00	487.0
134.90	141.0
136.90	64.0
140.90	466.0
142.90	398.0
146.80	124.0
147.70	94.0
154.90	59.0
160.90	57.0
162.90	143.0
165.00	85.0
171.90	129.0
173.90	24088.0
174.90	2128.0
175.90	25952.0
176.90	1834.0
178.20	70.0
178.90	142.0
188.90	53.0
191.00	619.0
192.00	170.0
193.00	856.0
193.90	178.0
194.80	92.0
202.90	65.0
204.90	154.0
207.00	420.0
208.00	85.0
235.00	80.0
248.90	517.0
250.00	118.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466

251.00	201.0
265.00	602.0
266.00	142.0
266.90	107.0
278.90	58.0
279.60	163.0
281.00	8470.0
282.00	1626.0
283.00	1341.0
284.00	228.0
285.00	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB466