


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW113018\
Data File : VW007136.D
Acq On : 30 Nov 2018 10:13
Operator : SY/AP
Sample : BFB81
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB81

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM113018S.M
Title : VOC Analysis
Last Update : Fri Nov 30 15:51:51 2018

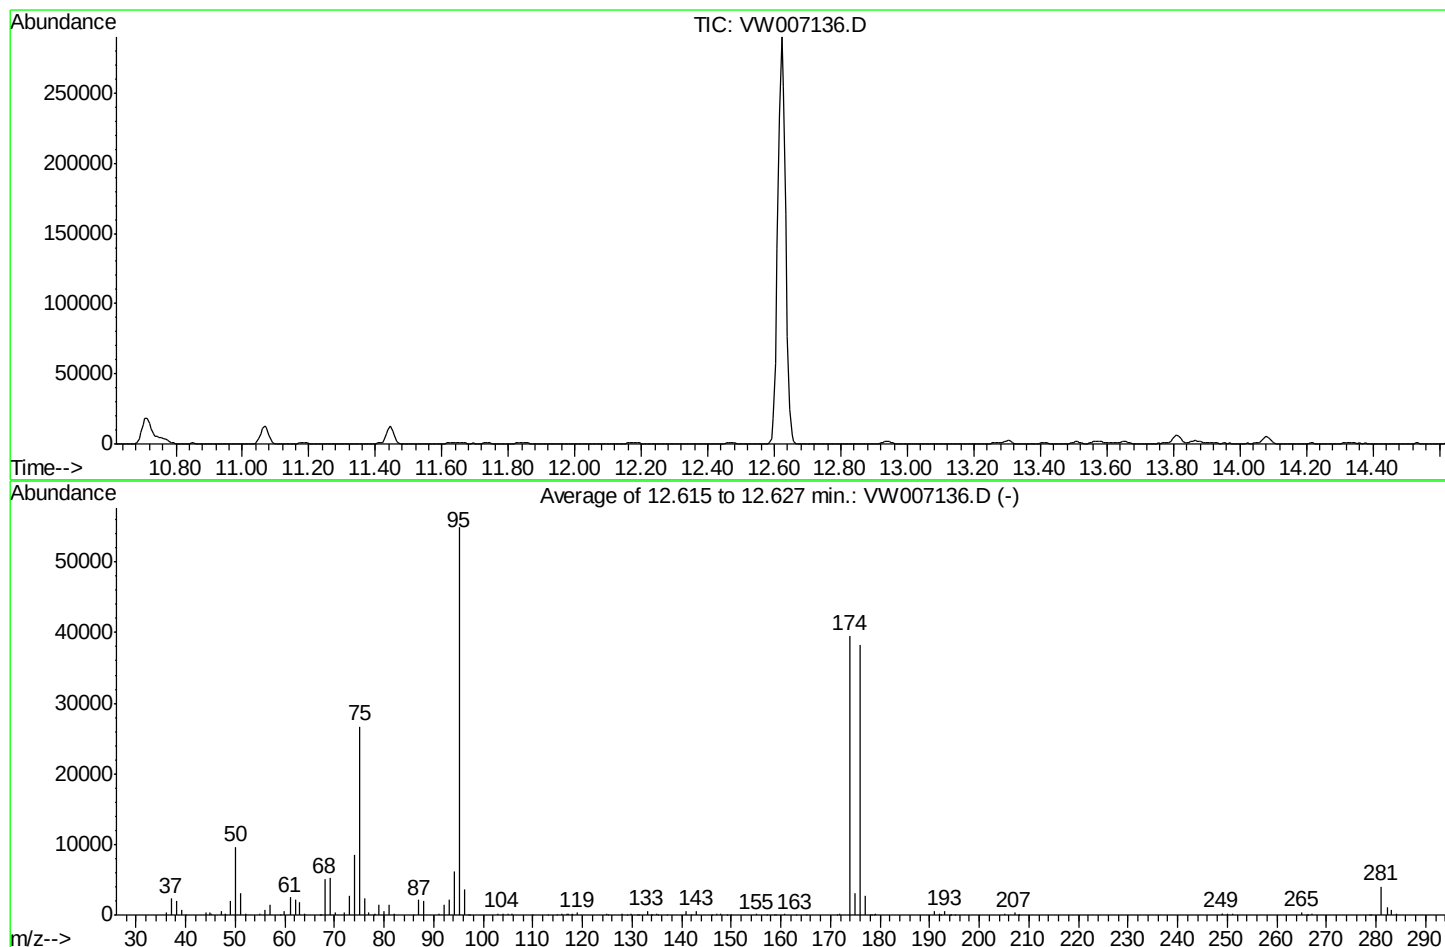

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	9662	PASS
75	95	30	80	48.5	26658	PASS
95	95	100	100	100.0	54914	PASS
96	95	5	9	6.8	3720	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.1	39602	PASS
175	174	5	9	7.6	3000	PASS
176	174	95	101	96.6	38258	PASS
177	176	5	9	7.0	2694	PASS

m/z	Abundance
36.00	389.0
37.10	2210.0
38.10	2007.0
39.10	797.0
39.90	161.0
44.00	329.0
45.00	492.0
47.10	587.0
47.90	359.0
49.00	1910.0
50.10	9181.0
51.00	2813.0
52.00	145.0
55.00	107.0
56.00	871.0
57.10	1414.0
59.00	77.0
60.00	546.0
61.10	2229.0
62.10	2121.0
63.10	1624.0
64.10	192.0
67.00	175.0
68.10	4899.0
69.00	5233.0
70.10	326.0
72.00	302.0
73.10	2986.0
74.10	7752.0
75.10	24624.0
76.00	2175.0
77.10	224.0
78.00	257.0
78.90	1204.0
80.00	466.0
81.00	1234.0
82.00	242.0
86.00	85.0
87.10	1992.0
88.00	1842.0
91.00	224.0
92.10	1334.0
93.00	1950.0
94.10	5425.0
95.10	49664.0
96.10	3441.0
97.20	130.0
103.00	167.0
103.90	161.0
104.90	90.0
105.90	250.0
110.00	101.0
113.00	87.0
114.90	87.0
116.00	165.0
116.80	314.0
117.80	267.0
118.90	305.0
124.90	189.0
128.00	166.0
128.90	91.0
129.80	174.0
131.00	127.0
133.10	625.0
133.80	167.0
134.90	84.0
137.00	63.0
141.00	449.0
141.90	89.0
143.00	527.0
146.10	55.0
147.00	129.0
148.00	126.0
149.10	78.0
155.10	142.0
161.00	112.0
163.00	114.0
171.40	86.0
172.00	148.0
174.00	33096.0
175.00	2515.0
176.00	30864.0
177.10	2213.0
178.10	107.0
179.00	190.0
191.10	590.0
192.10	228.0
193.10	693.0
194.00	129.0
195.10	96.0
205.00	123.0
207.00	386.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

207.90	53.0
248.90	327.0
250.00	158.0
251.00	129.0
265.00	442.0
266.00	174.0
267.10	127.0
278.60	70.0
281.10	4614.0
282.20	1270.0
283.10	940.0
284.20	207.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

Scan 1750 (12.573 min): VW007136.D
BFB81

m/z	Abundance
40.00	98.0
44.00	102.0
63.90	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

m/z	Abundance
36.10	386.0
37.10	2190.0
38.10	1857.0
39.10	740.0
39.90	126.0
44.00	419.0
45.20	447.0
47.10	531.0
48.10	270.0
49.10	1670.0
50.10	8580.0
51.10	2819.0
52.10	141.0
55.00	172.0
56.00	731.0
57.10	1441.0
60.00	480.0
61.00	2306.0
62.10	2070.0
63.10	1613.0
64.00	160.0
68.10	4676.0
69.10	4998.0
70.10	334.0
72.10	222.0
73.10	2427.0
74.10	8163.0
75.10	25784.0
76.10	2208.0
76.90	323.0
77.80	197.0
79.00	1363.0
80.00	570.0
80.90	1477.0
81.90	246.0
87.00	2136.0
88.00	1930.0
91.10	248.0
92.10	1363.0
93.10	2179.0
94.10	5880.0
95.10	54904.0
96.10	3526.0
96.90	59.0
103.00	96.0
103.90	254.0
105.00	93.0
105.80	153.0
112.90	55.0
115.90	165.0
117.00	417.0
117.90	234.0
118.90	320.0
125.30	107.0
128.00	146.0
128.90	70.0
129.90	174.0
130.90	94.0
133.10	363.0
133.90	60.0
134.90	109.0
136.90	111.0
140.90	538.0
142.90	595.0
145.90	89.0
146.90	67.0
147.90	115.0
149.90	85.0
155.10	87.0
156.90	139.0
159.00	122.0
160.80	80.0
171.90	201.0
174.00	41368.0
175.00	3007.0
176.00	41632.0
177.00	2556.0
177.80	68.0
178.20	58.0
179.10	65.0
191.00	321.0
192.30	98.0
193.10	318.0
194.20	90.0
204.90	76.0
207.20	236.0
208.00	71.0
248.90	249.0
250.10	90.0
251.10	170.0
265.00	289.0
266.20	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

267.00	58.0
278.90	59.0
281.10	2889.0
282.20	853.0
283.10	459.0
284.10	140.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

m/z	Abundance
36.10	526.0
37.00	2554.0
38.00	2260.0
39.10	773.0
40.00	131.0
44.00	394.0
45.00	510.0
47.10	724.0
47.80	352.0
49.00	2279.0
50.10	11225.0
51.10	3460.0
52.00	224.0
55.00	123.0
56.10	810.0
57.10	1547.0
59.10	95.0
59.90	425.0
61.10	2970.0
62.10	2576.0
63.00	2136.0
64.00	354.0
67.20	147.0
68.00	5700.0
69.10	5528.0
70.00	434.0
72.10	368.0
73.10	3026.0
74.10	9549.0
75.10	29568.0
76.00	2761.0
77.00	350.0
78.10	249.0
79.00	1544.0
80.00	484.0
81.00	1535.0
81.90	324.0
85.90	120.0
87.10	2371.0
88.00	2346.0
91.10	160.0
92.10	1857.0
93.00	2457.0
94.10	7358.0
95.10	60176.0
96.10	4195.0
96.90	80.0
103.00	110.0
103.90	264.0
104.80	116.0
105.00	95.0
105.90	165.0
113.00	58.0
114.90	157.0
115.90	209.0
117.00	379.0
118.00	143.0
119.00	413.0
124.80	159.0
125.20	137.0
128.00	285.0
128.90	105.0
129.90	298.0
131.20	92.0
133.10	650.0
134.00	130.0
134.70	102.0
135.10	100.0
137.00	107.0
140.90	584.0
141.90	75.0
143.00	760.0
146.00	72.0
147.00	103.0
148.00	126.0
149.10	67.0
150.00	73.0
155.10	163.0
157.10	117.0
158.80	64.0
159.10	66.0
160.80	124.0
165.00	63.0
171.20	88.0
174.00	44344.0
175.00	3480.0
176.00	42280.0
177.00	3313.0
177.90	100.0
178.70	79.0
179.00	65.0
191.00	542.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

192.00	125.0
193.00	626.0
194.00	135.0
195.10	78.0
205.00	148.0
207.10	302.0
208.10	84.0
249.10	374.0
250.00	115.0
251.10	124.0
265.00	519.0
266.30	117.0
267.10	120.0
278.80	61.0
281.10	4635.0
282.10	1224.0
283.10	820.0
284.10	217.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81