


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW113020\
 Data File : VW017508.D
 Acq On : 30 Nov 2020 09:12
 Operator : SY/VA
 Sample : BFB14
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB14

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Title : VOC Analysis
 Last Update : Thu Nov 26 07:23:09 2020

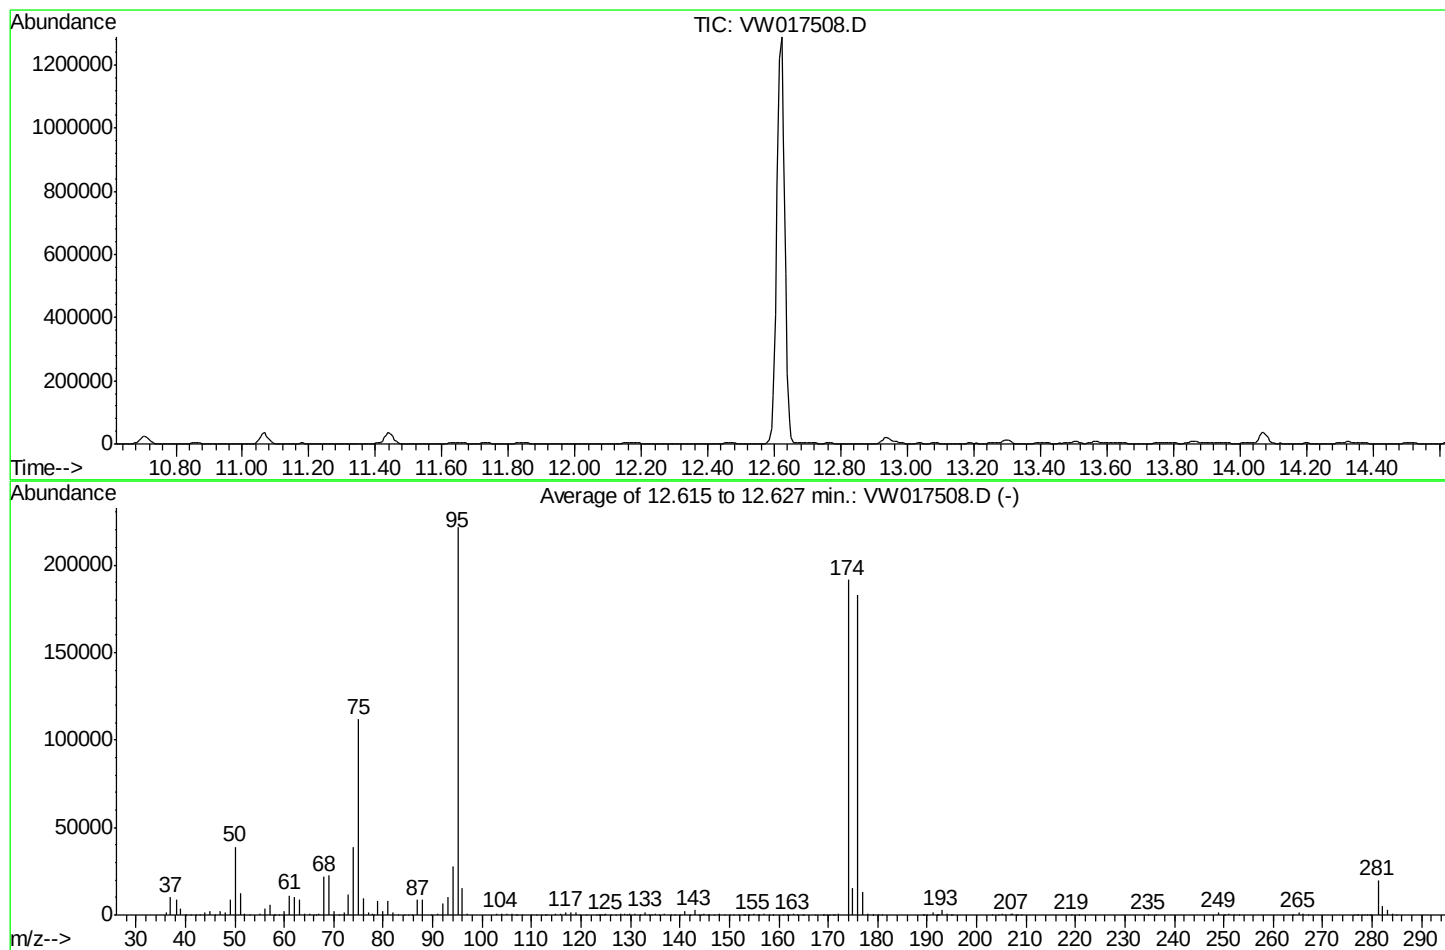

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	39104	PASS
75	95	30	80	50.4	111602	PASS
95	95	100	100	100.0	221461	PASS
96	95	5	9	6.9	15385	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.5	191552	PASS
175	174	5	9	7.9	15116	PASS
176	174	95	101	95.4	182656	PASS
177	176	5	9	7.2	13061	PASS