

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120219\
 Data File : VW014199.D
 Acq On : 02 Dec 2019 13:16
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 02 16:03:59 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Dec 02 16:00:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	280305	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	278924	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	155266	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	80400	17.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.92%
7) Chloroethane-d5	2.89	69	71558	19.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.96%
10) 1,1-Dichloroethene-d2	4.01	63	130141	14.18	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.72%
20) 2-Butanone-d5	7.07	46	80103	61.65	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	123.30%
24) Chloroform-d	7.65	84	198971	23.09	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.36%
26) 1,2-Dichloroethane-d4	8.31	65	111426	25.72	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.88%
29) Benzene-d6	8.27	84	404569	20.44	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.76%
33) 1,2-Dichloropropane-d6	9.27	67	125575	21.66	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.64%
37) Toluene-d8	10.32	98	366828	19.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.20%
38) trans-1,3-Dichloropropene-	10.57	79	53048	21.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.48%
39) 2-Hexanone-d5	10.92	63	63909	58.13	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.26%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	120064	27.43	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	109.72%
61) 1,2-Dichlorobenzene-d4	13.85	152	138307	22.17	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.68%


Target Compounds					Ovalue
13) Acetone	4.13	43	7622	5.765 ug/L	88
36) Methylcyclohexane	9.27	83	31467	3.216 ug/L #	20
59) 1,2,3-Trichloropropane	13.55	75	15807	4.975 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW120219\
Data File : VW014199.D
Acq On : 02 Dec 2019 13:16
Operator : SY/VA
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Dec 02 16:03:59 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Mon Dec 02 16:00:46 2019
Response via : Initial Calibration




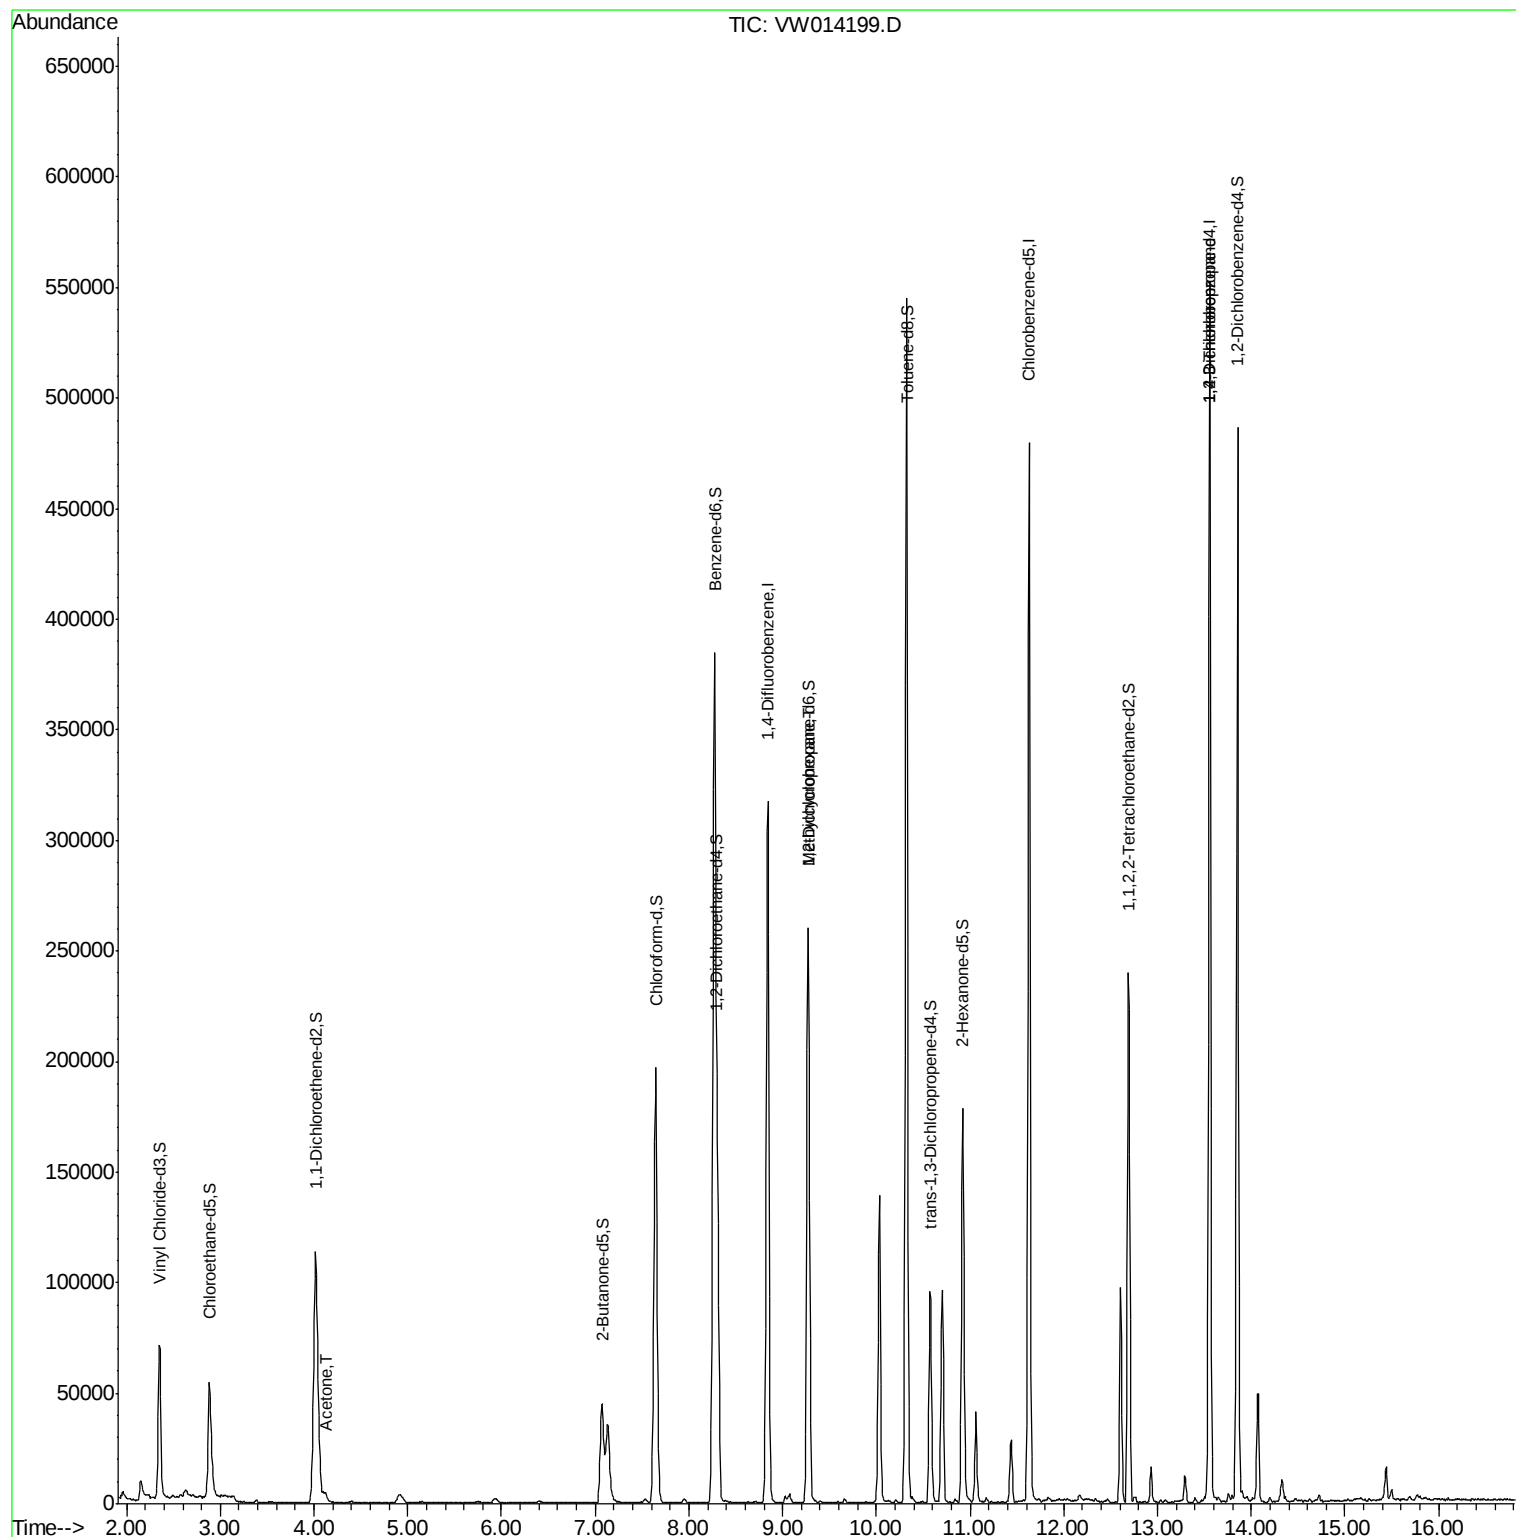


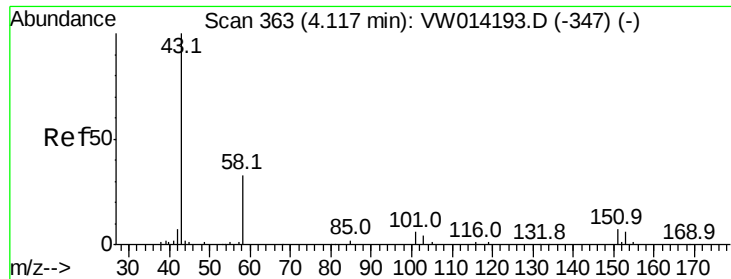

#13
Acetone
Concen: 5.765 ug/L
RT: 4.13 min Scan# 365
Delta R.T. 0.01 min
Lab File: VW014199.D
Acq: 02 Dec 2019 13:16




Instrument :
MSVOA_W
ClientSampled :


Tot Ion: 43 Resp: 7622
Ion Ratio Lower Upper
43 100
58 25.7 0.0 65.4

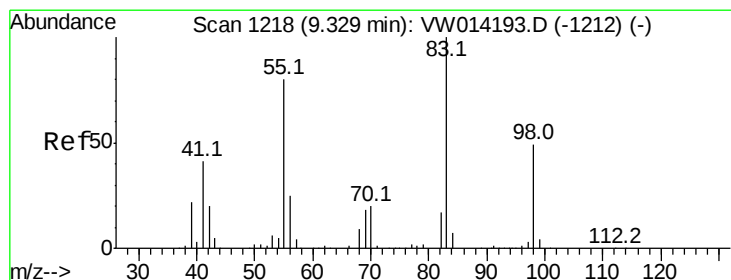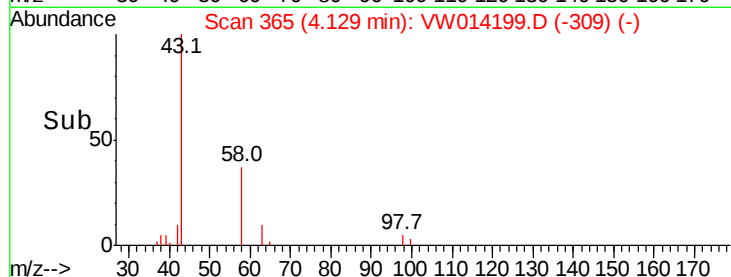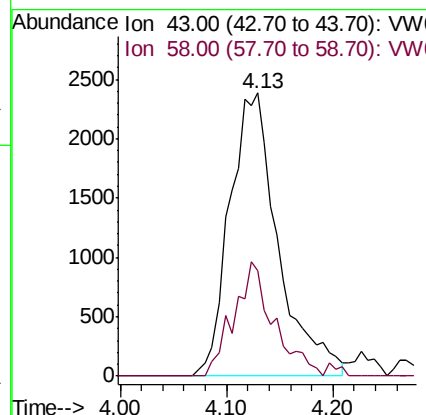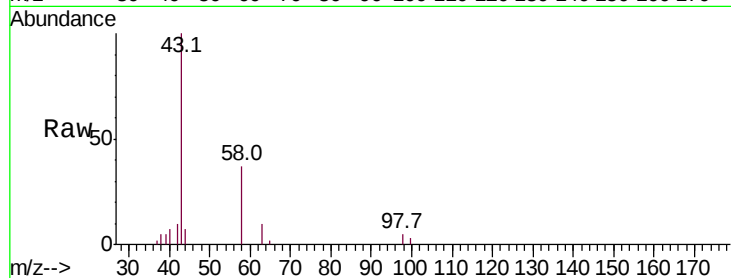

#36
Methylcyclohexane
Concen: 3.216 ug/L
RT: 9.27 min Scan# 1209
Delta R.T. -0.06 min
Lab File: VW014199.D
Acq: 02 Dec 2019 13:16

Tgt Ion: 83 Resp: 31467
Ion Ratio Lower Upper
83 100
55 0.5 59.8 89.8#
98 1.9 39.5 59.3#

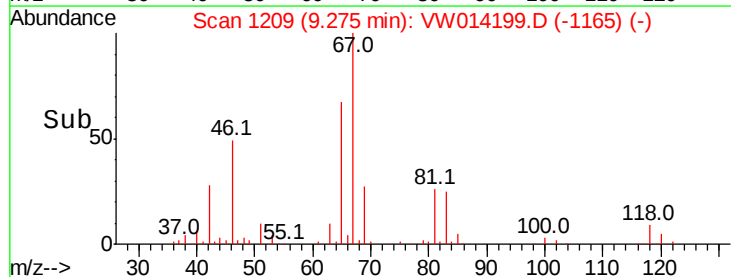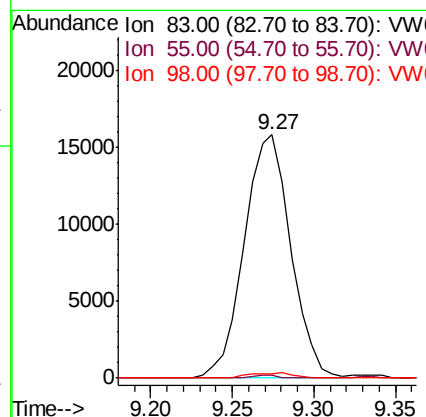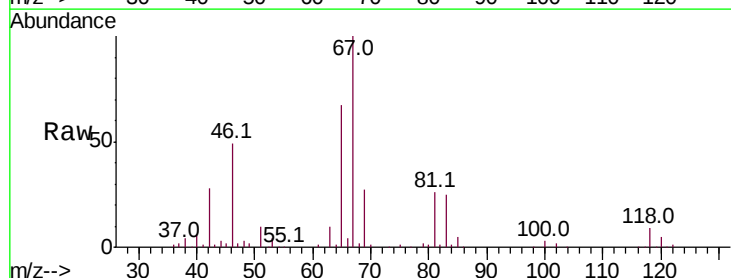

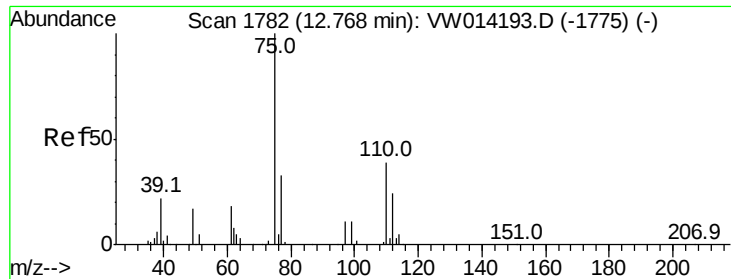

#59

1,2,3-Trichloropropane

Concen: 4.975 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW014199.D

Acq: 02 Dec 2019 13:16

Instrument :

MSVOA_W

ClientSampleId :

Tot Ion: 75 Resp: 15807

Ion Ratio Lower Upper

75 100

77 36.6 25.9 38.9

